

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012233.D
 Acq On : 21 Oct 2022 02:13
 Operator : CG/JU
 Sample : N5144-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	42	46	57	rVB	76687	112863	1.12%	0.119%
2	3.681	115	118	139	rBV	695466	1069303	10.64%	1.125%
3	3.899	150	155	162	rBV	47648	73544	0.73%	0.077%
4	3.999	168	172	180	rVB	28124	42366	0.42%	0.045%
5	4.375	233	236	242	rVB5	8932	13955	0.14%	0.015%
6	4.916	326	328	340	rVB2	10109	20677	0.21%	0.022%
7	6.993	675	681	700	rVB	310565	535901	5.33%	0.564%
8	7.157	702	709	725	rBV	1496937	2402703	23.91%	2.528%
9	7.351	735	742	753	rBV	1289692	2097007	20.87%	2.206%
10	7.428	753	755	761	rVB5	10986	14766	0.15%	0.016%
11	7.822	815	822	832	rBV	1486362	2435040	24.23%	2.562%
12	8.534	937	943	962	rBV	970514	1671848	16.64%	1.759%
13	8.992	1013	1021	1039	rBV	1712061	2912416	28.98%	3.064%
14	9.381	1084	1087	1098	rVB	16522	29310	0.29%	0.031%
15	9.710	1136	1143	1156	rBV	969903	1637669	16.30%	1.723%
16	10.251	1223	1235	1251	rBV	1769246	3185475	31.70%	3.351%
17	10.628	1289	1299	1312	rBV	2219428	3754256	37.36%	3.950%
18	10.769	1316	1323	1339	rBV	1610047	2983133	29.69%	3.139%
19	11.886	1508	1513	1518	rVB8	5238	10740	0.11%	0.011%
20	12.045	1534	1540	1547	rBV8	7581	16178	0.16%	0.017%
21	12.222	1563	1570	1578	rBV2	32180	57896	0.58%	0.061%
22	13.439	1773	1777	1788	rVB5	10989	23977	0.24%	0.025%
23	13.798	1834	1838	1846	rBV2	19135	30840	0.31%	0.032%
24	13.886	1846	1853	1865	rBV	3863278	5416813	53.91%	5.699%
25	14.163	1891	1900	1912	rBV	4265901	6722616	66.90%	7.073%
26	14.474	1946	1953	1967	rBV	3351007	4995378	49.71%	5.256%
27	14.727	1989	1996	2004	rBV	8539	26440	0.26%	0.028%
28	15.269	2083	2088	2091	rBV2	8812	11115	0.11%	0.012%
29	15.469	2115	2122	2140	rBV	5684374	8513759	84.72%	8.957%
30	15.604	2140	2145	2158	rVV3	30111	63103	0.63%	0.066%
31	15.710	2158	2163	2170	rVB	24654	40627	0.40%	0.043%
32	16.904	2363	2366	2372	rBV7	7421	12370	0.12%	0.013%
33	17.021	2382	2386	2393	rVB3	9463	15568	0.15%	0.016%
34	17.233	2415	2422	2432	rBV	3866040	5658636	56.31%	5.953%
35	17.333	2432	2439	2452	rVV2	6895195	9809148	97.62%	10.320%
36	17.433	2452	2456	2464	rVB3	57774	92250	0.92%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012233.D
 Acq On : 21 Oct 2022 02:13
 Operator : CG/JU
 Sample : N5144-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BT0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	18.121	2570	2573	2578	rBV5	19167	31303	0.31%	0.033%
38	18.192	2582	2585	2589	rVV	11258	15123	0.15%	0.016%
39	19.145	2743	2747	2754	rBV	89713	128935	1.28%	0.136%
40	19.215	2755	2759	2764	rBV	76836	112061	1.12%	0.118%
41	19.574	2814	2820	2832	rBV	7282786	10048761	100.00%	10.572%
42	21.321	3112	3117	3127	rBV	3602250	4809293	47.86%	5.060%
43	23.574	3493	3500	3514	rVB2	4388432	8879602	88.37%	9.342%
44	23.727	3520	3526	3539	rVB2	2285293	4513845	44.92%	4.749%




Sum of corrected areas: 95048609

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012233.D
Acq On : 21 Oct 2022 02:13
Operator : CG/JU
Sample : N5144-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COBT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

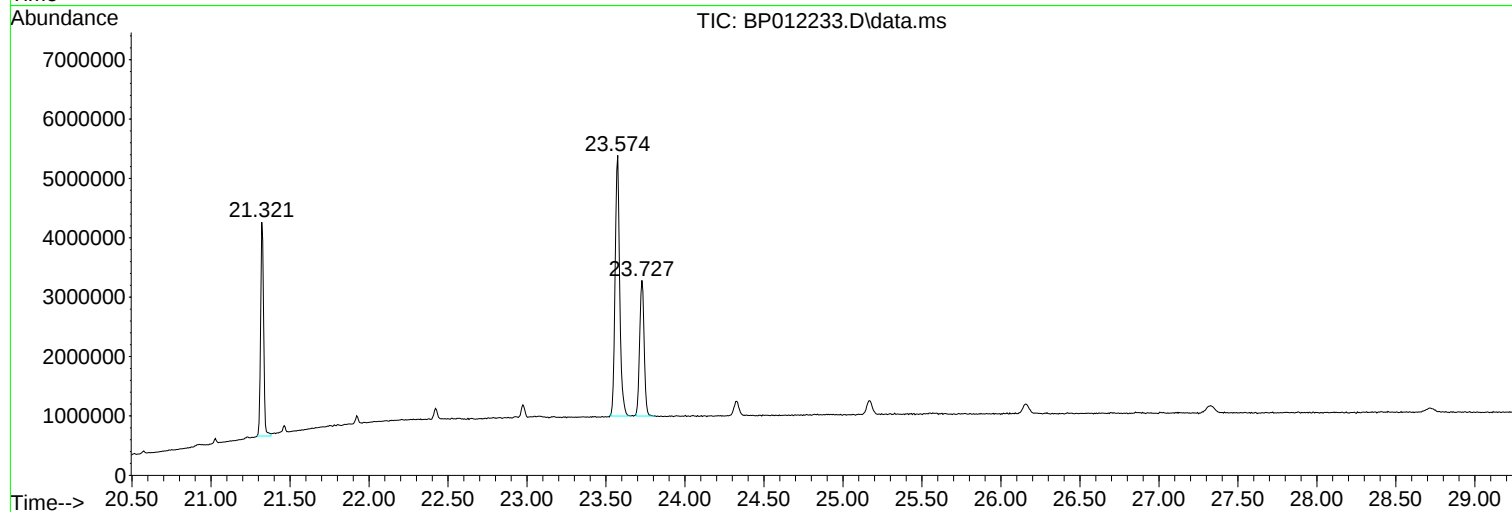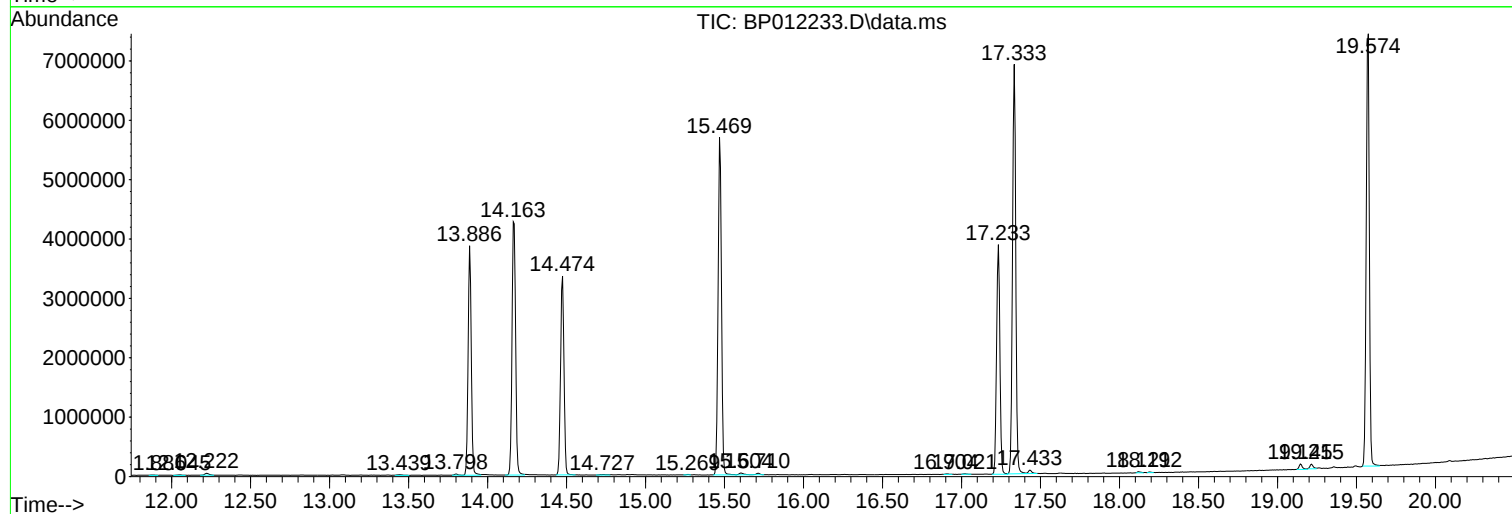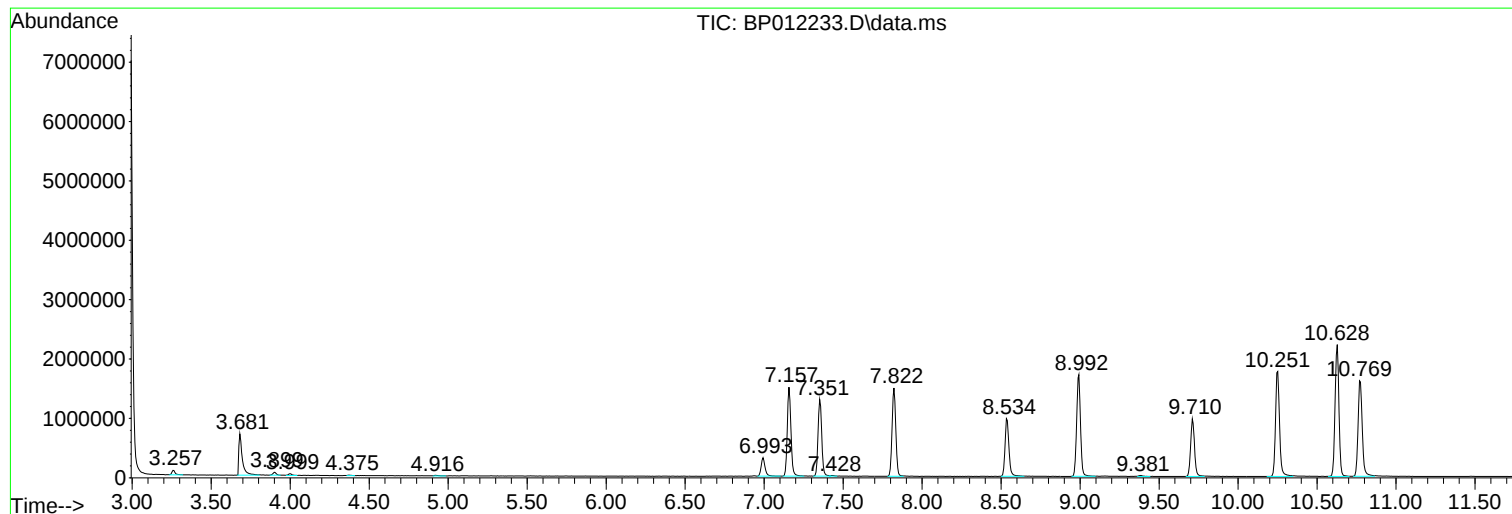

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012233.D
Acq On : 21 Oct 2022 02:13
Operator : CG/JU
Sample : N5144-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012233.D
Acq On : 21 Oct 2022 02:13
Operator : CG/JU
Sample : N5144-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc