

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012235.D
 Acq On : 21 Oct 2022 09:13
 Operator : CG/JU
 Sample : PB148441BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	55	rVB	115475	148047	1.79%	0.156%
2	3.681	115	118	148	rVV	1386367	2171195	26.18%	2.285%
3	4.005	168	173	178	rVB	29491	44206	0.53%	0.047%
4	6.999	675	682	701	rVB	1657915	2648422	31.94%	2.788%
5	7.163	703	710	726	rVB	1388583	2191611	26.43%	2.307%
6	7.357	735	743	766	rBV	1685282	2651204	31.97%	2.791%
7	7.828	814	823	839	rBV	1373829	2211420	26.67%	2.328%
8	8.546	937	945	966	rBV	2002313	3356605	40.48%	3.533%
9	8.999	1015	1022	1035	rBV	1541162	2582234	31.14%	2.718%
10	9.722	1136	1145	1159	rBV	1281843	2137104	25.77%	2.249%
11	10.257	1228	1236	1253	rBV	1951662	3405951	41.07%	3.585%
12	10.634	1292	1300	1315	rBV	2034056	3376941	40.72%	3.554%
13	10.781	1317	1325	1348	rBV	1929715	3481708	41.99%	3.665%
14	11.446	1433	1438	1445	rBV10	4328	9992	0.12%	0.011%
15	12.228	1564	1571	1581	rBV2	33344	63820	0.77%	0.067%
16	13.445	1773	1778	1785	rBV5	7359	13745	0.17%	0.014%
17	13.898	1848	1855	1867	rBV	3270203	4800381	57.89%	5.053%
18	13.987	1868	1870	1878	rVB9	7692	13889	0.17%	0.015%
19	14.175	1893	1902	1919	rBV	4107028	6014963	72.54%	6.331%
20	14.481	1947	1954	1967	rBV	3085925	4563605	55.04%	4.803%
21	14.692	1984	1990	2012	rBV	1217895	2147294	25.90%	2.260%
22	15.263	2080	2087	2092	rBV	5373	11828	0.14%	0.012%
23	15.404	2104	2111	2112	rBV5	9664	18242	0.22%	0.019%
24	15.481	2117	2124	2136	rVB	5247533	7432181	89.63%	7.823%
25	15.604	2139	2145	2158	rBV	1029151	1501624	18.11%	1.581%
26	15.716	2161	2164	2172	rVB	25131	38891	0.47%	0.041%
27	16.269	2253	2258	2263	rBV9	7552	12378	0.15%	0.013%
28	16.522	2297	2301	2303	rBV4	7645	9592	0.12%	0.010%
29	16.692	2325	2330	2338	rBV6	15767	34463	0.42%	0.036%
30	16.916	2366	2368	2374	rVB6	7775	12615	0.15%	0.013%
31	17.028	2383	2387	2392	rBV3	9881	17702	0.21%	0.019%
32	17.245	2417	2424	2433	rBV	3614844	5188773	62.57%	5.461%
33	17.345	2434	2441	2452	rVV	5331633	7824359	94.36%	8.236%
34	17.639	2484	2491	2500	rBV6	27123	74202	0.89%	0.078%
35	18.198	2583	2586	2592	rVB5	15078	24245	0.29%	0.026%
36	19.157	2746	2749	2753	rVB3	60915	79777	0.96%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012235.D
Acq On : 21 Oct 2022 09:13
Operator : CG/JU
Sample : PB148441BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Title : SVOA CALIBRATION

37	19.227	2757	2761	2770	rBV2	65298	134067	1.62%	0.141%
38	19.586	2816	2822	2827	rBV	5947107	8292095	100.00%	8.728%
39	21.333	3115	3119	3124	rBV	3519055	4505004	54.33%	4.742%
40	23.592	3496	3503	3517	rVB2	3609809	7391338	89.14%	7.780%
41	23.745	3523	3529	3538	rVB2	2160701	4368861	52.69%	4.598%




Sum of corrected areas: 95006574

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012235.D
Acq On : 21 Oct 2022 09:13
Operator : CG/JU
Sample : PB148441BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

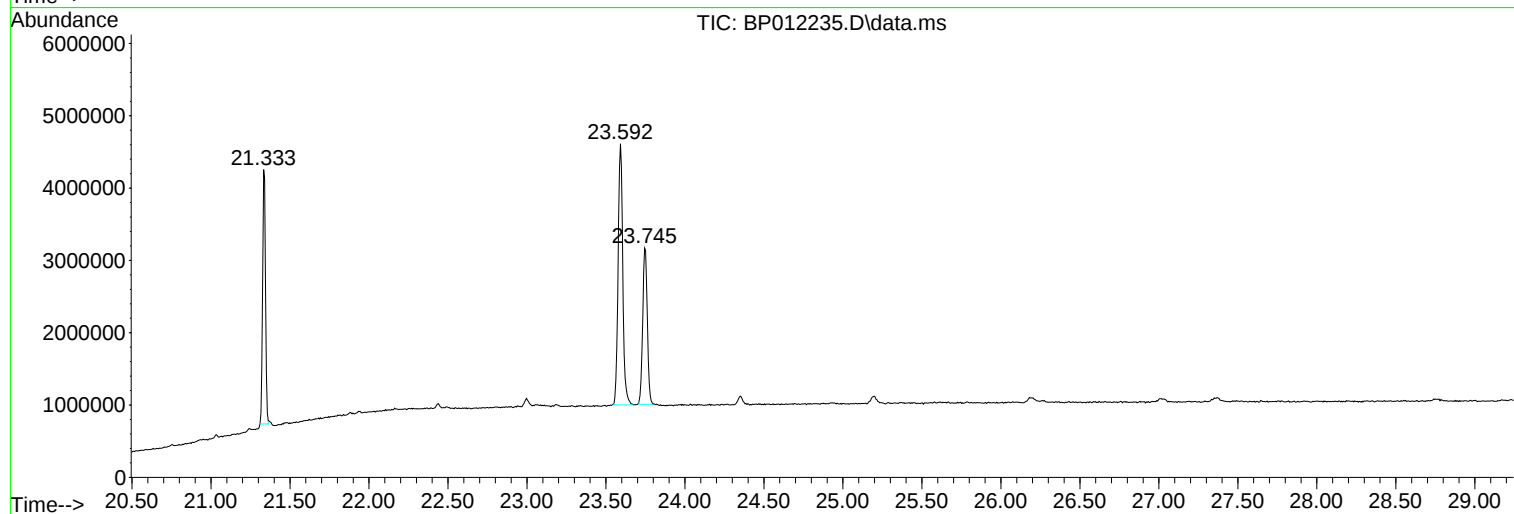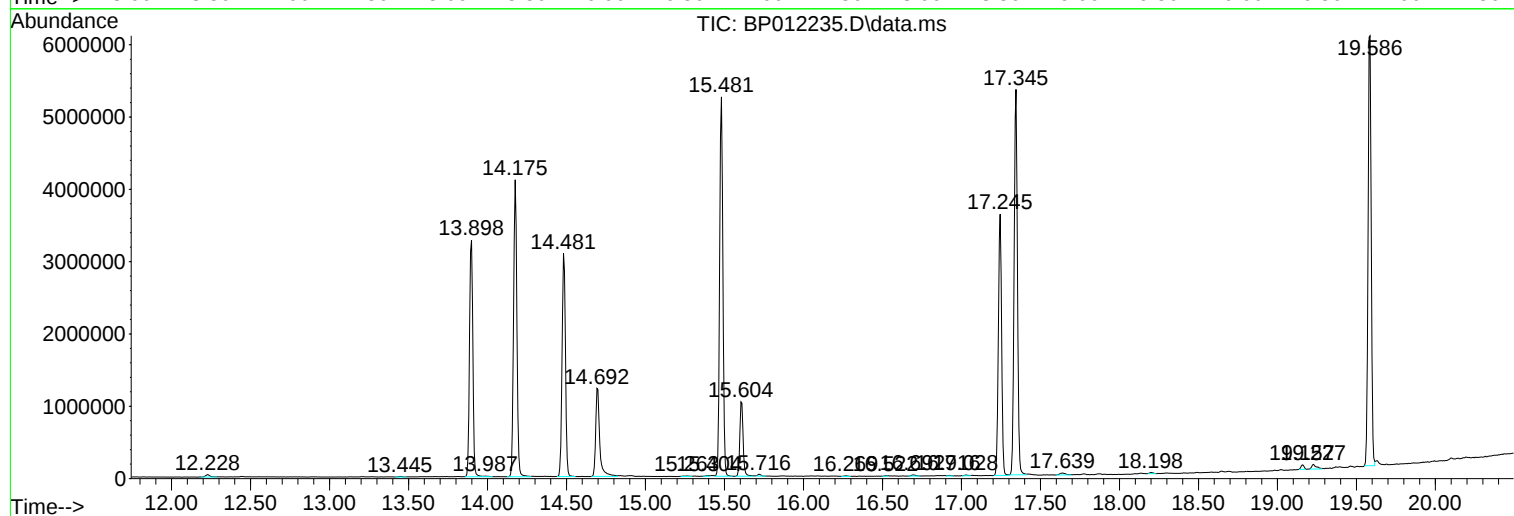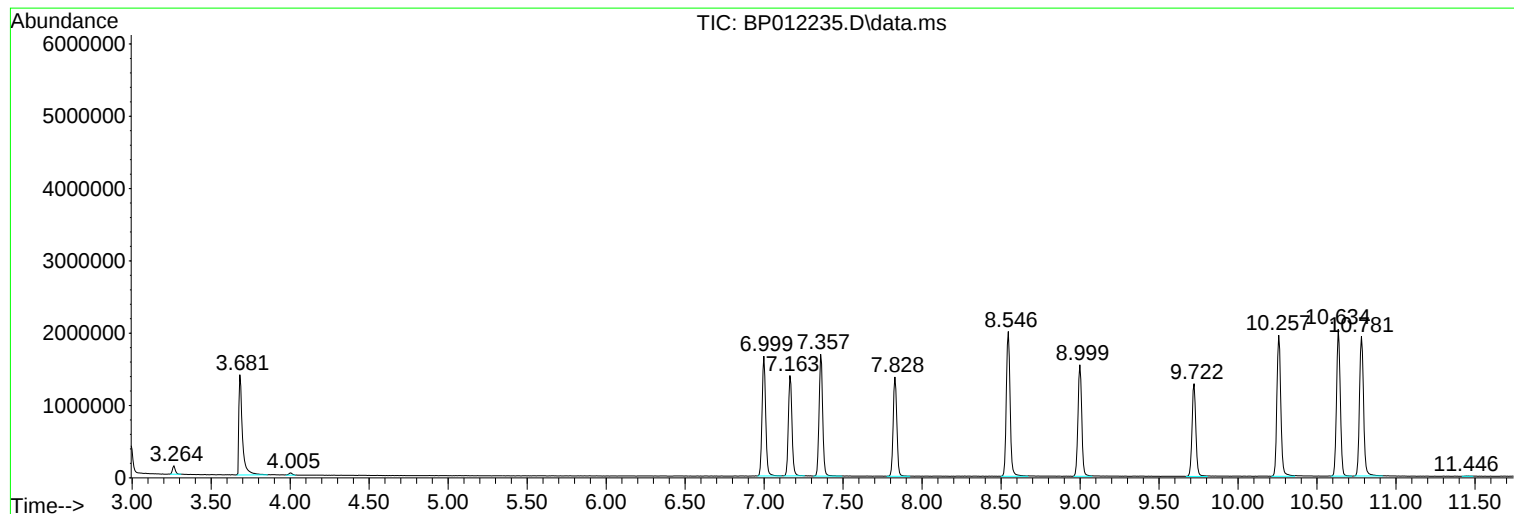

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012235.D
Acq On : 21 Oct 2022 09:13
Operator : CG/JU
Sample : PB148441BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012235.D
Acq On : 21 Oct 2022 09:13
Operator : CG/JU
Sample : PB148441BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc