

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012239.D
 Acq On : 21 Oct 2022 11:29
 Operator : CG/JU
 Sample : PB148371BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	56	rVB	119619	154789	2.22%	0.175%
2	3.676	114	117	148	rBV	1425005	2203150	31.60%	2.498%
3	3.999	168	172	180	rVB	30290	45015	0.65%	0.051%
4	6.993	674	681	700	rBV	1707556	2739344	39.29%	3.105%
5	7.158	702	709	724	rVV	1422866	2271026	32.57%	2.575%
6	7.352	735	742	761	rBV	1709278	2742799	39.34%	3.109%
7	7.822	814	822	835	rBV	1422160	2309133	33.12%	2.618%
8	8.534	936	943	961	rBV	1984480	3440191	49.34%	3.900%
9	8.993	1013	1021	1035	rBV	1558013	2678059	38.41%	3.036%
10	9.710	1135	1143	1158	rBV	1282742	2168416	31.10%	2.458%
11	10.252	1227	1235	1261	rBV	1931048	3460560	49.63%	3.923%
12	10.628	1288	1299	1314	rBV	2008101	3456174	49.57%	3.918%
13	10.775	1314	1324	1347	rBV	1882627	3531322	50.65%	4.003%
14	12.222	1564	1570	1577	rBV2	26427	54607	0.78%	0.062%
15	12.440	1602	1607	1609	rBV5	5226	7698	0.11%	0.009%
16	13.440	1772	1777	1783	rBV6	6778	12264	0.18%	0.014%
17	13.887	1846	1853	1868	rBV	3207299	4573668	65.60%	5.185%
18	13.987	1868	1870	1875	rVB6	8114	9227	0.13%	0.010%
19	14.163	1890	1900	1917	rBV	3799493	5784553	82.97%	6.558%
20	14.475	1946	1953	1965	rBV	2866975	4396138	63.05%	4.984%
21	14.687	1982	1989	2012	rBV	845387	1651615	23.69%	1.872%
22	15.146	2063	2067	2073	rVB9	4975	8699	0.12%	0.010%
23	15.469	2114	2122	2136	rBV	4712646	6972255	100.00%	7.904%
24	15.598	2138	2144	2157	rVV	602673	945055	13.55%	1.071%
25	15.710	2158	2163	2169	rVB2	24175	44889	0.64%	0.051%
26	16.904	2361	2366	2371	rBV9	12054	21744	0.31%	0.025%
27	17.234	2415	2422	2432	rBV	3112390	4440474	63.69%	5.034%
28	17.334	2432	2439	2458	rVV	4630324	6662628	95.56%	7.553%
29	19.145	2744	2747	2752	rBV2	49166	61255	0.88%	0.069%
30	19.216	2756	2759	2763	rVB	46642	61420	0.88%	0.070%
31	19.569	2814	2819	2828	rBV	4905267	6667917	95.64%	7.559%
32	21.322	3113	3117	3127	rBV	2895393	3829966	54.93%	4.342%
33	23.574	3493	3500	3516	rVB2	3359495	6830943	97.97%	7.744%
34	23.727	3520	3526	3536	rVB2	1972106	3974091	57.00%	4.505%

Sum of corrected areas: 88211084




Instrument :
BNA_P
ClientSampleId :
SBLK371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012239.D
Acq On : 21 Oct 2022 11:29
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

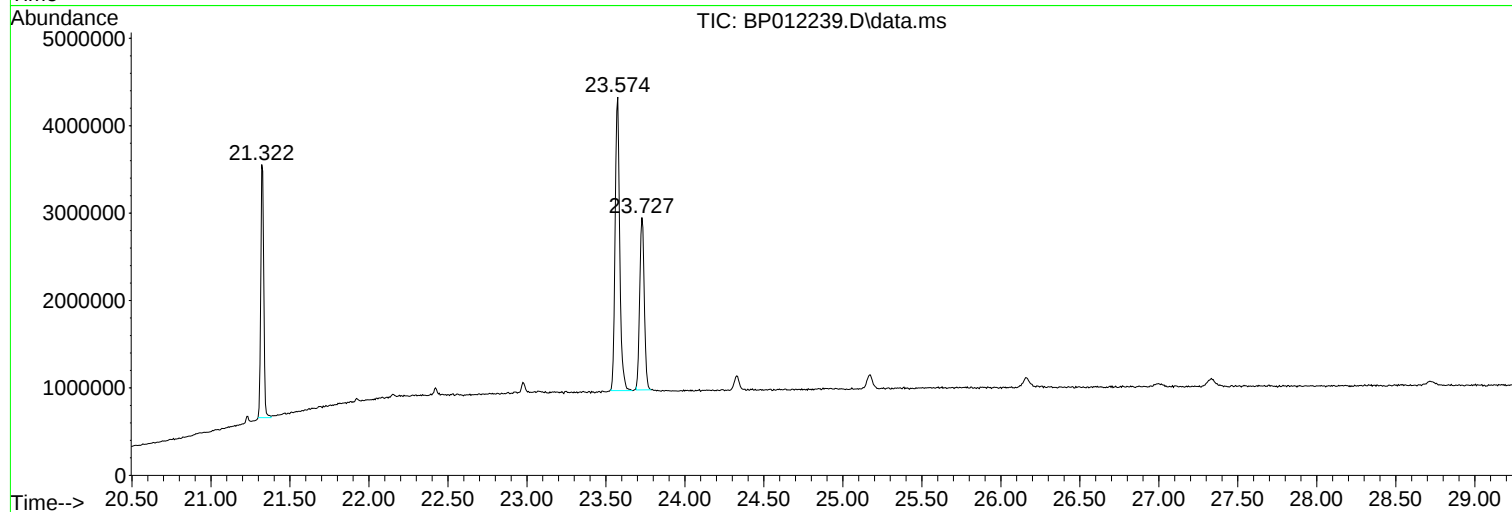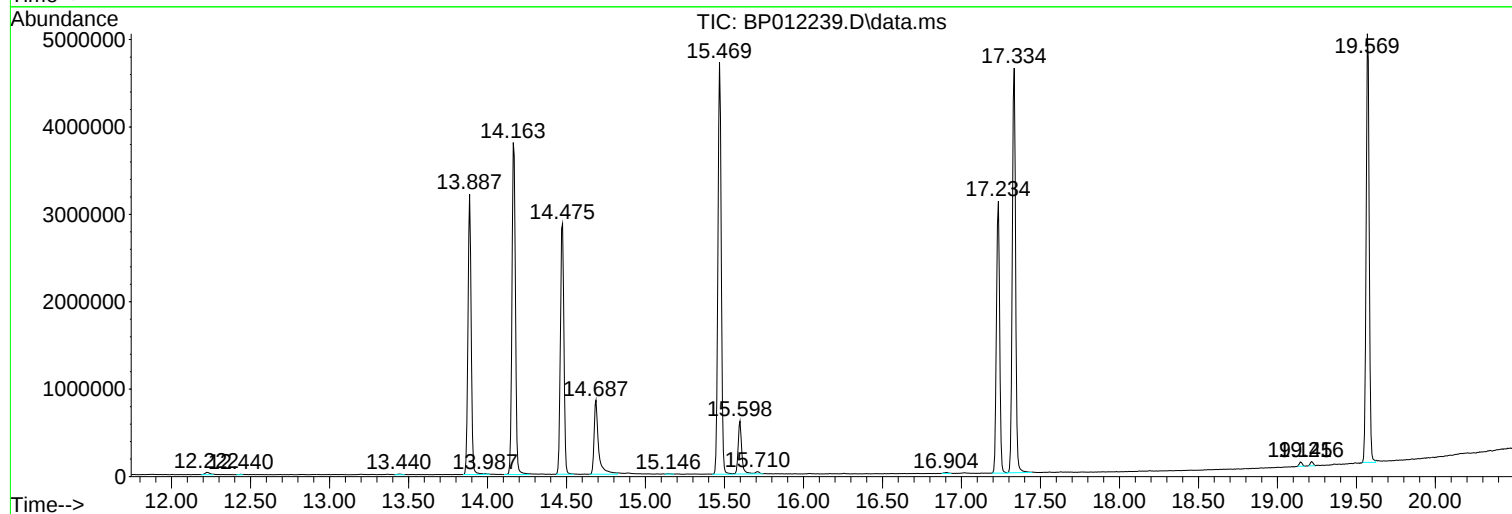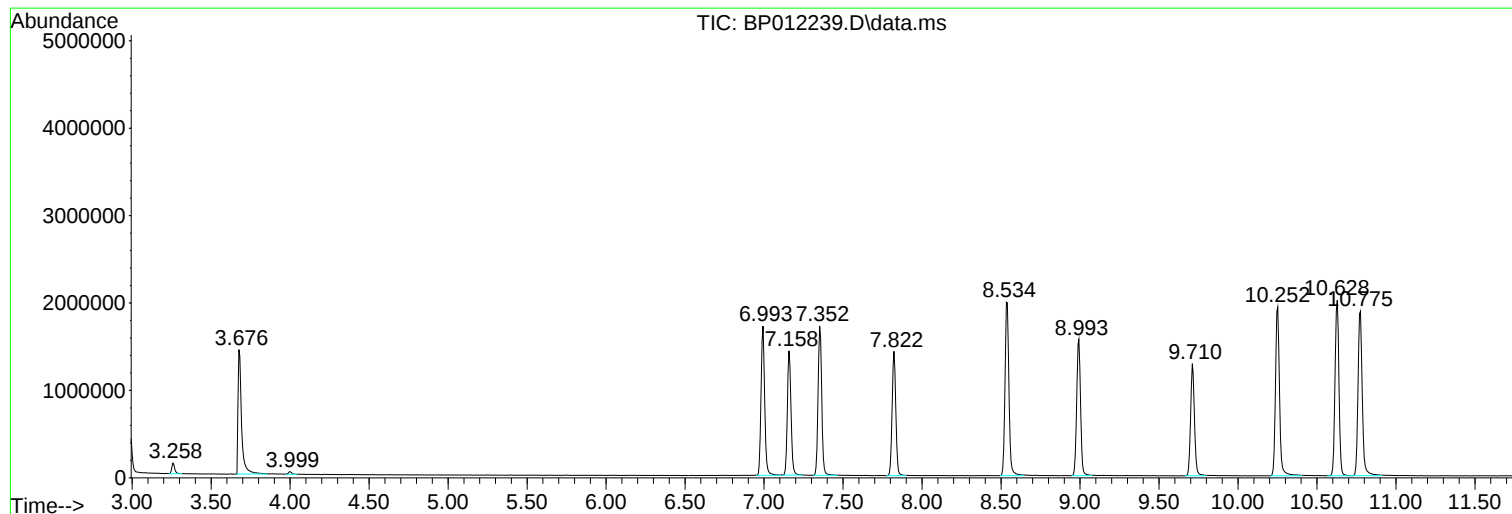

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012239.D
Acq On : 21 Oct 2022 11:29
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012239.D
Acq On : 21 Oct 2022 11:29
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc