

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012246.D
 Acq On : 21 Oct 2022 15:31
 Operator : CG/JU
 Sample : PB148371BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	57	rVB	108541	140128	2.29%	0.174%
2	3.681	114	118	135	rBV	1250750	1906400	31.14%	2.374%
3	3.999	168	172	178	rVB	26035	36681	0.60%	0.046%
4	6.993	673	681	701	rBV	1538228	2525360	41.25%	3.144%
5	7.158	703	709	722	rVV	1307030	2055863	33.58%	2.560%
6	7.352	735	742	757	rBV	1586445	2554077	41.72%	3.180%
7	7.822	814	822	835	rBV	1384148	2224659	36.34%	2.770%
8	8.540	936	944	960	rBV	1913310	3196859	52.21%	3.980%
9	8.993	1013	1021	1040	rBV	1454531	2469697	40.34%	3.075%
10	9.710	1135	1143	1157	rBV	1211658	2071989	33.84%	2.580%
11	10.252	1227	1235	1257	rBV	1798645	3197146	52.22%	3.981%
12	10.628	1291	1299	1313	rVB	1910035	3281551	53.60%	4.086%
13	10.775	1316	1324	1343	rBV	1753214	3224403	52.66%	4.015%
14	12.222	1564	1570	1581	rBV	27187	59359	0.97%	0.074%
15	12.434	1601	1606	1608	rBV6	4126	6216	0.10%	0.008%
16	13.446	1773	1778	1783	rBV4	6097	10872	0.18%	0.014%
17	13.887	1845	1853	1867	rBV	2912362	4017983	65.63%	5.003%
18	14.169	1893	1901	1919	rBV	3418646	5217429	85.22%	6.496%
19	14.475	1946	1953	1964	rBV	2738541	4017276	65.61%	5.002%
20	14.687	1983	1989	2008	rBV	772093	1580849	25.82%	1.968%
21	15.469	2115	2122	2137	rBV	4122569	6122550	100.00%	7.623%
22	15.598	2138	2144	2155	rVV	792008	1161217	18.97%	1.446%
23	15.710	2159	2163	2171	rVB2	23795	39057	0.64%	0.049%
24	16.045	2216	2220	2224	rBV7	4211	6430	0.11%	0.008%
25	16.263	2254	2257	2262	rVB7	5184	7334	0.12%	0.009%
26	16.904	2364	2366	2370	rVB5	6998	8942	0.15%	0.011%
27	17.022	2382	2386	2389	rBV2	6023	8820	0.14%	0.011%
28	17.234	2415	2422	2432	rBV	2769724	3983491	65.06%	4.960%
29	17.334	2432	2439	2455	rVV	3991580	5864006	95.78%	7.301%
30	17.522	2466	2471	2476	rBV8	16505	37723	0.62%	0.047%
31	19.151	2744	2748	2752	rBV2	43861	60458	0.99%	0.075%
32	19.216	2756	2759	2764	rBV	44926	67184	1.10%	0.084%
33	19.575	2814	2820	2830	rBV	4347352	5829349	95.21%	7.258%
34	21.327	3113	3118	3126	rBV	2806117	3598190	58.77%	4.480%
35	23.574	3494	3500	3512	rVB2	2963108	6019486	98.32%	7.495%
36	23.727	3521	3526	3535	rVB2	1847943	3706326	60.54%	4.615%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012246.D
Acq On : 21 Oct 2022 15:31
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Title : SVOA CALIBRATION


Sum of corrected areas: 80315360

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012246.D
Acq On : 21 Oct 2022 15:31
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

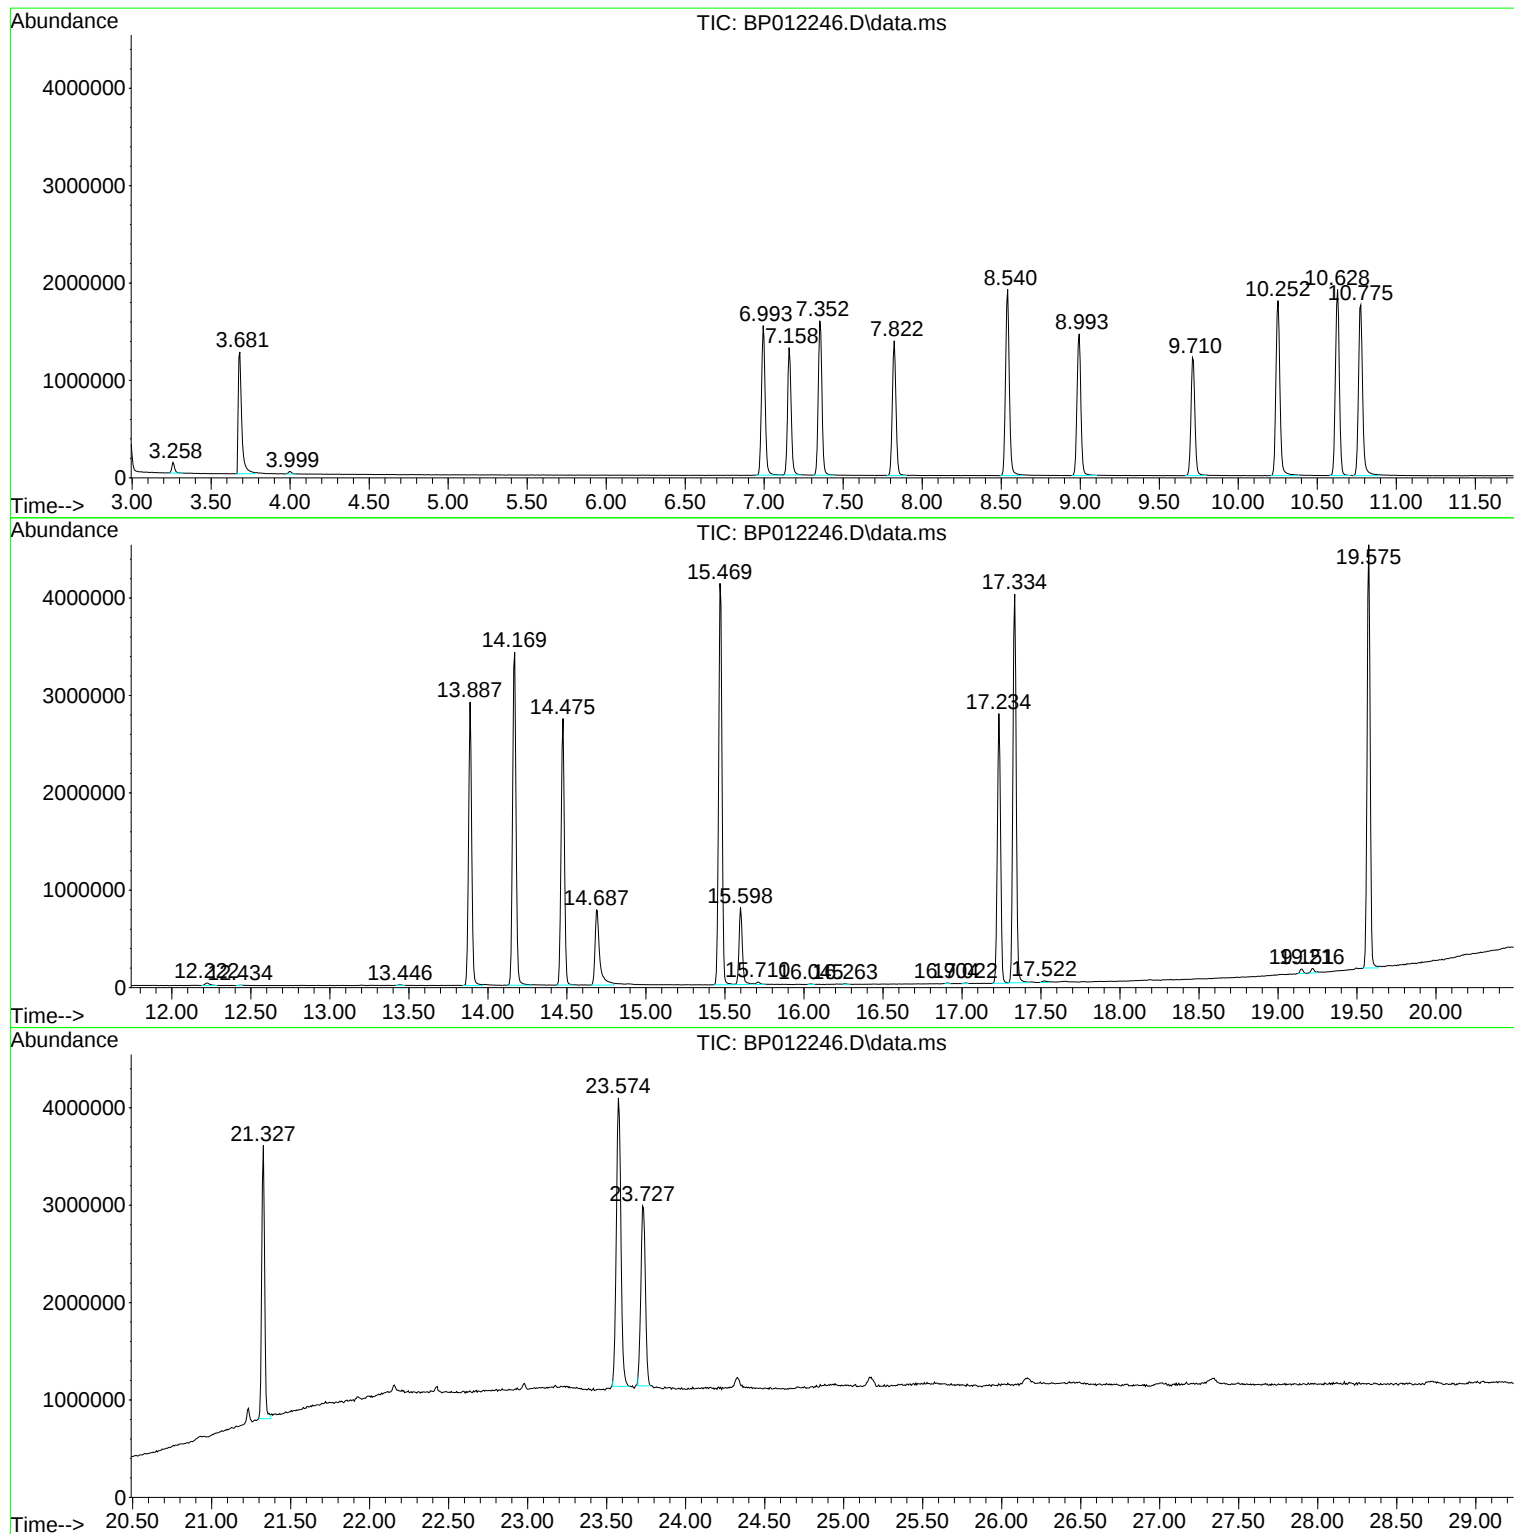

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012246.D
Acq On : 21 Oct 2022 15:31
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012246.D
Acq On : 21 Oct 2022 15:31
Operator : CG/JU
Sample : PB148371BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc