

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012259.D
 Acq On : 21 Oct 2022 22:58
 Operator : CG/JU
 Sample : N5064-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	43	46	57	rVB	66021	90333	1.94%	0.139%
2	3.564	94	98	102	rVB4	7001	11741	0.25%	0.018%
3	3.687	116	119	121	rBV2	12763	12128	0.26%	0.019%
4	3.705	121	122	131	rVV	25469	38577	0.83%	0.059%
5	3.781	131	135	142	rVB	58818	79020	1.70%	0.121%
6	3.899	150	155	160	rVB	77600	112051	2.41%	0.172%
7	3.999	167	172	179	rVB	32345	46650	1.00%	0.072%
8	4.164	197	200	205	rVB4	7196	11581	0.25%	0.018%
9	4.375	232	236	242	rVB2	21504	28175	0.61%	0.043%
10	4.558	263	267	275	rVB5	17271	24390	0.53%	0.037%
11	4.917	324	328	339	rBV3	50614	108604	2.34%	0.167%
12	5.028	343	347	353	rBV4	8475	15568	0.34%	0.024%
13	5.452	416	419	425	rVB8	7387	11755	0.25%	0.018%
14	5.822	478	482	486	rBV2	10218	15951	0.34%	0.025%
15	6.328	562	568	573	rVB	25260	38406	0.83%	0.059%
16	6.846	651	656	663	rBV5	12884	27172	0.58%	0.042%
17	6.993	674	681	696	rBV	1002932	1717868	36.98%	2.641%
18	7.116	696	702	704	rVV	32041	48728	1.05%	0.075%
19	7.158	704	709	721	rVB	893094	1417947	30.52%	2.180%
20	7.352	735	742	752	rBV	1056866	1670021	35.95%	2.567%
21	7.428	752	755	767	rVB5	16069	36669	0.79%	0.056%
22	7.640	785	791	797	rBV2	12785	24713	0.53%	0.038%
23	7.822	812	822	830	rBV	1428623	2333250	50.22%	3.587%
24	8.099	865	869	875	rVB9	6225	12547	0.27%	0.019%
25	8.534	937	943	959	rBV	814739	1402496	30.19%	2.156%
26	8.652	959	963	972	rVB	20553	36568	0.79%	0.056%
27	8.987	1013	1020	1038	rBV	996243	1664464	35.83%	2.559%
28	9.152	1044	1048	1055	rVB8	16468	30944	0.67%	0.048%
29	9.381	1082	1087	1093	rVB2	29289	47493	1.02%	0.073%
30	9.710	1135	1143	1155	rBV	797958	1359481	29.26%	2.090%
31	10.246	1227	1234	1248	rBV	1168606	2084331	44.87%	3.204%
32	10.410	1254	1262	1278	rBV	144199	335717	7.23%	0.516%
33	10.622	1289	1298	1312	rBV	1966273	3434884	73.94%	5.280%
34	10.769	1316	1323	1339	rBV	825907	1526879	32.87%	2.347%
35	11.163	1384	1390	1396	rVB10	6383	13882	0.30%	0.021%
36	11.446	1432	1438	1445	rBV10	6779	20086	0.43%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012259.D
 Acq On : 21 Oct 2022 22:58
 Operator : CG/JU
 Sample : N5064-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

37	11.640	1465	1471	1476	rBV9	7856	16449	0.35%	0.025%
38	11.881	1508	1512	1516	rVB4	8477	12826	0.28%	0.020%
39	12.040	1534	1539	1545	rVB2	14335	20647	0.44%	0.032%
40	12.157	1553	1559	1565	rBV3	26061	52672	1.13%	0.081%
41	12.216	1565	1569	1577	rVV2	21644	37286	0.80%	0.057%
42	12.293	1577	1582	1587	rVB	14508	22677	0.49%	0.035%
43	12.510	1613	1619	1625	rVB2	13729	26527	0.57%	0.041%
44	12.822	1668	1672	1675	rBV5	7174	10180	0.22%	0.016%
45	12.993	1695	1701	1706	rBV10	5777	11302	0.24%	0.017%
46	13.075	1708	1715	1723	rVB9	7501	13814	0.30%	0.021%
47	13.287	1746	1751	1757	rBV2	34017	58557	1.26%	0.090%
48	13.363	1759	1764	1769	rVV3	13774	27515	0.59%	0.042%
49	13.434	1772	1776	1782	rVB6	7925	15602	0.34%	0.024%
50	13.798	1831	1838	1843	rBV7	14905	32255	0.69%	0.050%
51	13.887	1843	1853	1861	rBV	2014228	2927627	63.02%	4.500%
52	13.987	1866	1870	1874	rVB6	6902	13319	0.29%	0.020%
53	14.163	1893	1900	1917	rVB	2446697	3634365	78.23%	5.587%
54	14.363	1929	1934	1940	rVB	23733	34682	0.75%	0.053%
55	14.469	1943	1952	1960	rBV	2717769	4191844	90.23%	6.444%
56	14.687	1983	1989	2004	rBV	452135	940926	20.25%	1.446%
57	14.851	2014	2017	2019	rBV4	9095	13423	0.29%	0.021%
58	14.898	2021	2025	2036	rVB4	50455	97478	2.10%	0.150%
59	15.263	2082	2087	2091	rBV	11032	19290	0.42%	0.030%
60	15.316	2091	2096	2101	rVB2	27052	39917	0.86%	0.061%
61	15.469	2114	2122	2129	rBV	3138783	4467688	96.17%	6.868%
62	15.598	2138	2144	2156	rBV	406021	619487	13.33%	0.952%
63	15.710	2159	2163	2168	rVB4	16192	27529	0.59%	0.042%
64	15.822	2178	2182	2189	rVB10	6258	10677	0.23%	0.016%
65	15.928	2197	2200	2203	rBV4	8878	11611	0.25%	0.018%
66	16.045	2214	2220	2224	rBV9	6451	14419	0.31%	0.022%
67	16.186	2240	2244	2252	rVB5	22230	48814	1.05%	0.075%
68	16.386	2273	2278	2283	rVB8	10731	21333	0.46%	0.033%
69	16.769	2338	2343	2350	rBV2	36027	60379	1.30%	0.093%
70	16.886	2361	2363	2370	rVB8	8010	16116	0.35%	0.025%
71	16.986	2376	2380	2383	rBV2	15640	21445	0.46%	0.033%
72	17.128	2400	2404	2412	rVB7	23242	45959	0.99%	0.071%
73	17.228	2412	2421	2432	rBV	2712469	4184798	90.08%	6.433%
74	17.328	2432	2438	2449	rVV	2835255	4097912	88.21%	6.299%
75	17.433	2452	2456	2462	rVB6	29436	52791	1.14%	0.081%
76	17.722	2503	2505	2509	rVB5	10600	14221	0.31%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
 Data File : BP012259.D
 Acq On : 21 Oct 2022 22:58
 Operator : CG/JU
 Sample : N5064-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COBL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
 Title : SVOA CALIBRATION

77	17.863	2527	2529	2532	rBV4	8612	10678	0.23%	0.016%
78	17.898	2532	2535	2539	rVB2	29185	32606	0.70%	0.050%
79	18.116	2567	2572	2578	rBV	231111	360870	7.77%	0.555%
80	18.169	2578	2581	2585	rVB4	70308	97711	2.10%	0.150%
81	18.263	2595	2597	2605	rVB9	14135	22143	0.48%	0.034%
82	18.404	2615	2621	2626	rBV7	25106	67108	1.44%	0.103%
83	18.510	2636	2639	2643	rBV6	21949	32593	0.70%	0.050%
84	18.716	2671	2674	2679	rVB6	48278	59225	1.27%	0.091%
85	18.775	2681	2684	2687	rVV4	32982	35881	0.77%	0.055%
86	18.857	2695	2698	2703	rBV5	74487	95626	2.06%	0.147%
87	18.969	2712	2717	2720	rBV	131254	165300	3.56%	0.254%
88	19.004	2721	2723	2728	rVV4	24106	33620	0.72%	0.052%
89	19.145	2744	2747	2753	rVB4	38565	58462	1.26%	0.090%
90	19.216	2755	2759	2761	rBV	58548	77768	1.67%	0.120%
91	19.351	2778	2782	2791	rBV3	140865	243912	5.25%	0.375%
92	19.569	2813	2819	2831	rBV	3285987	4393059	94.56%	6.753%
93	20.122	2910	2913	2916	rBV4	94278	120896	2.60%	0.186%
94	21.027	3064	3067	3078	rVB2	357352	535556	11.53%	0.823%
95	21.322	3112	3117	3127	rBV	3030297	3960607	85.25%	6.088%
96	23.568	3493	3499	3511	rVB2	2174877	4645619	100.00%	7.141%
97	23.721	3519	3525	3535	rVB2	2103877	4125576	88.81%	6.342%


Sum of corrected areas: 65052245

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012259.D
Acq On : 21 Oct 2022 22:58
Operator : CG/JU
Sample : N5064-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COBL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

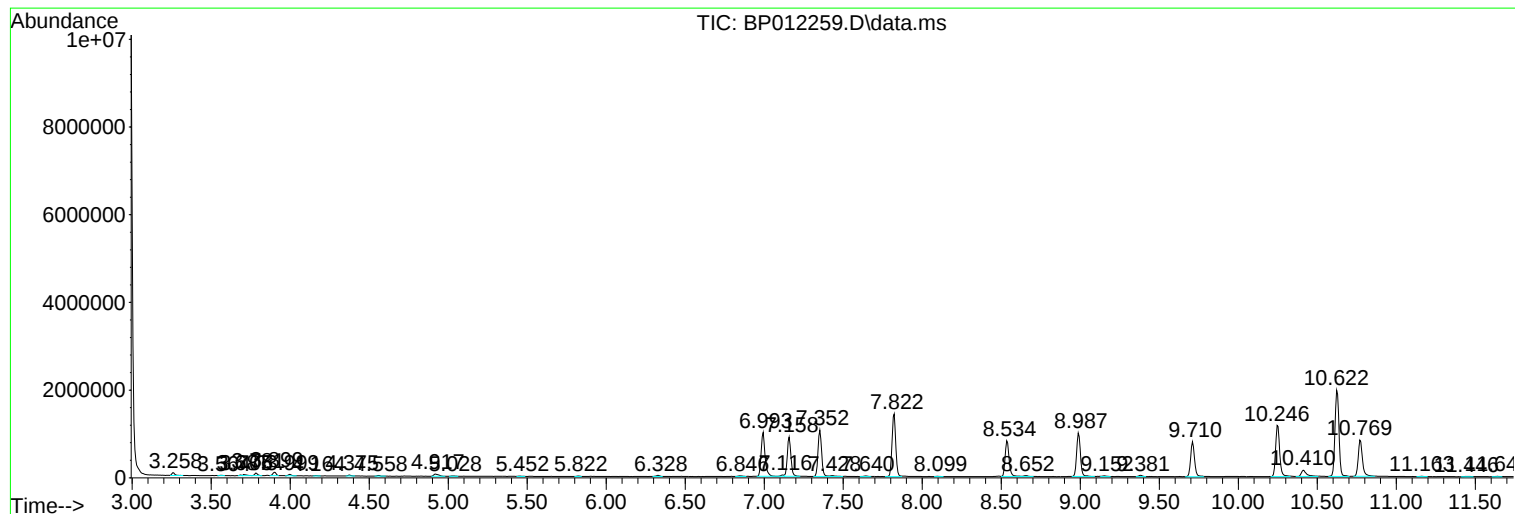

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012259.D
Acq On : 21 Oct 2022 22:58
Operator : CG/JU
Sample : N5064-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COBL3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.027 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.027	2.70 ng/ul	535556	Chrysene-d12	21.322

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentane, (4-octyldodecyl)-	350	C25H50	005638-09-5	91
2			1-Dodecanol, 2-octyl-	298	C20H42O	005333-42-6	91
3			1-Decanol, 2-hexyl-	242	C16H34O	002425-77-6	91
4			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	91
5			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	91

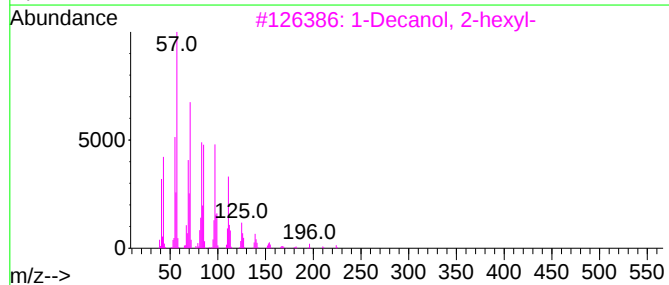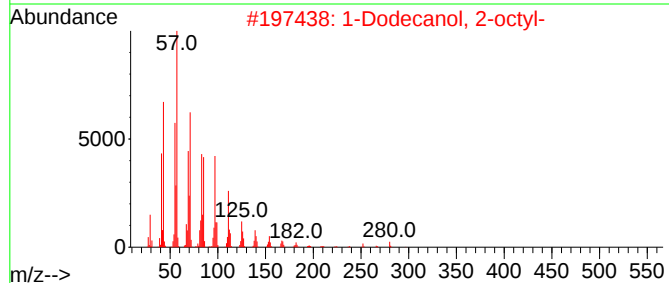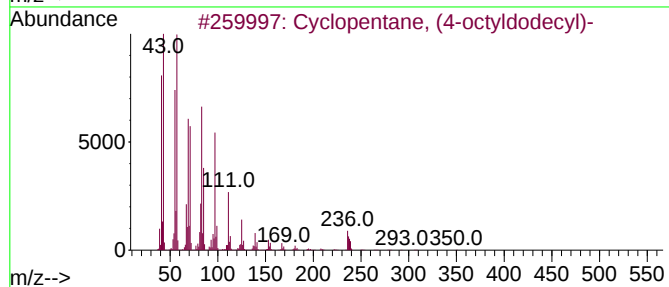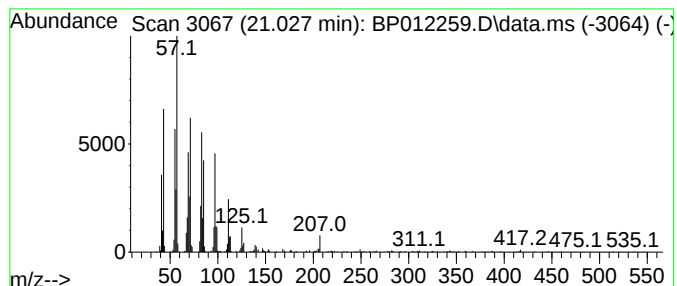

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102022\
Data File : BP012259.D
Acq On : 21 Oct 2022 22:58
Operator : CG/JU
Sample : N5064-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.027	2.7	ng/u1	535556	5	21.322	3960610	20.0