
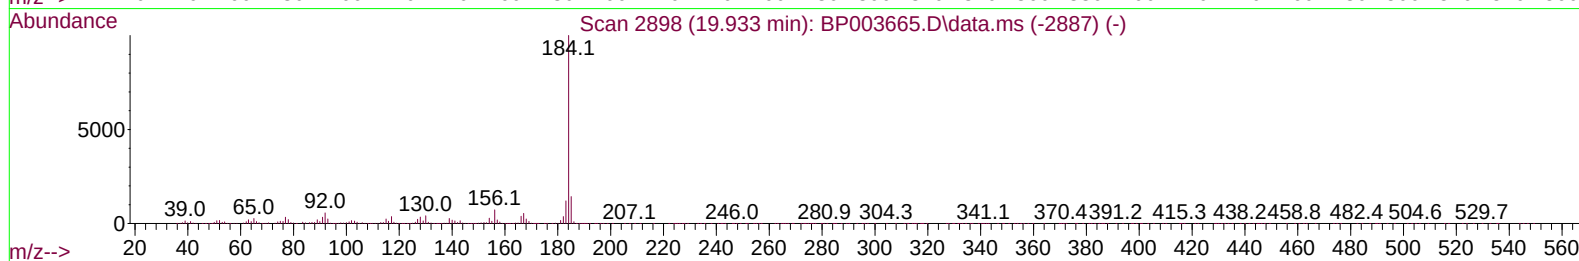
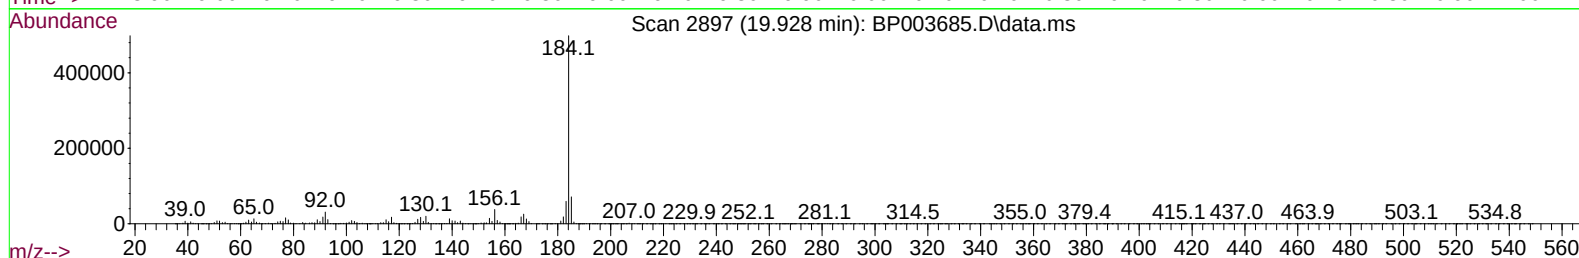


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
Data File : BP003685.D
Acq On : 21 Oct 2020 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 18:35:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

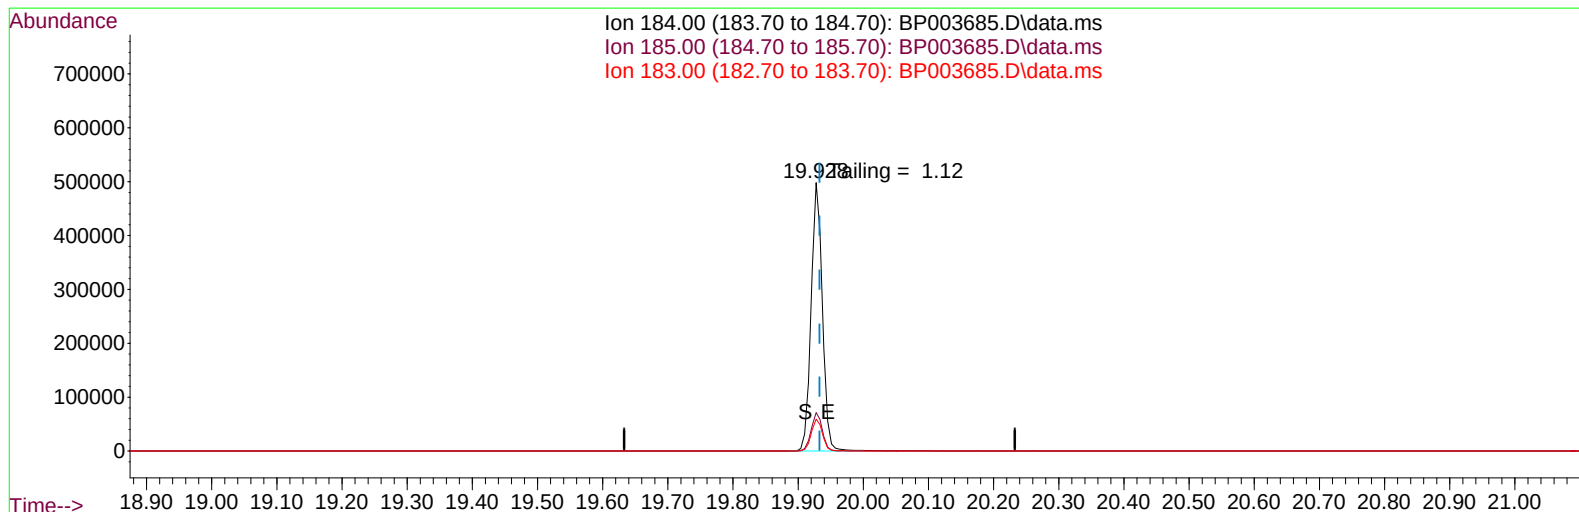

TIC: BP003685.D\data.ms

(77) Benzidine




19.928min (-0.005) 423234.89 ng

response 598306

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	12.00	11.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
Data File : BP003685.D
Acq On : 21 Oct 2020 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 18:35:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 19 14:54:24 2020
Response via : Initial Calibration

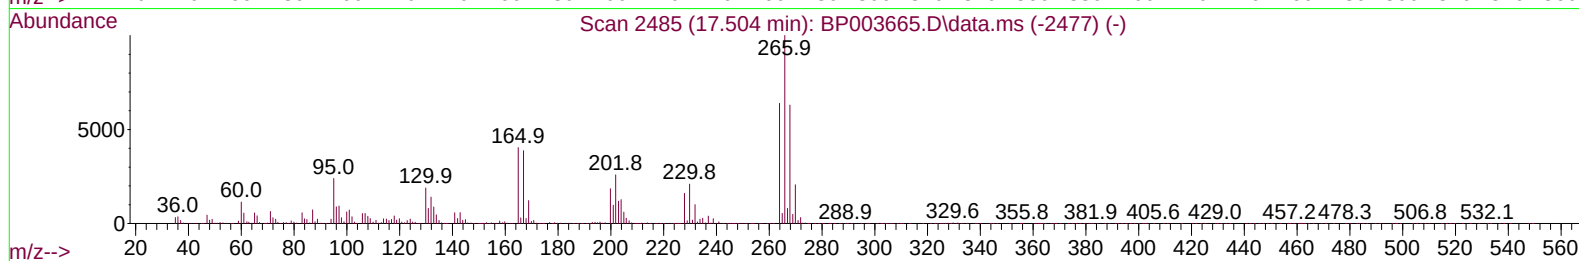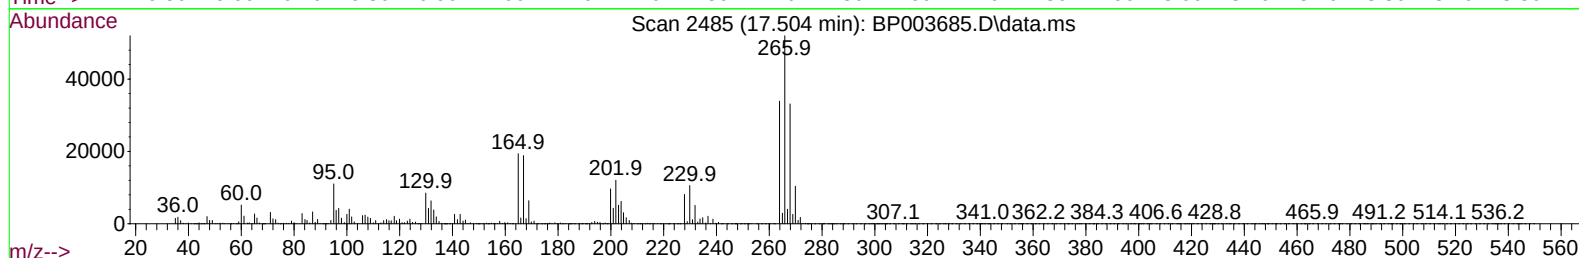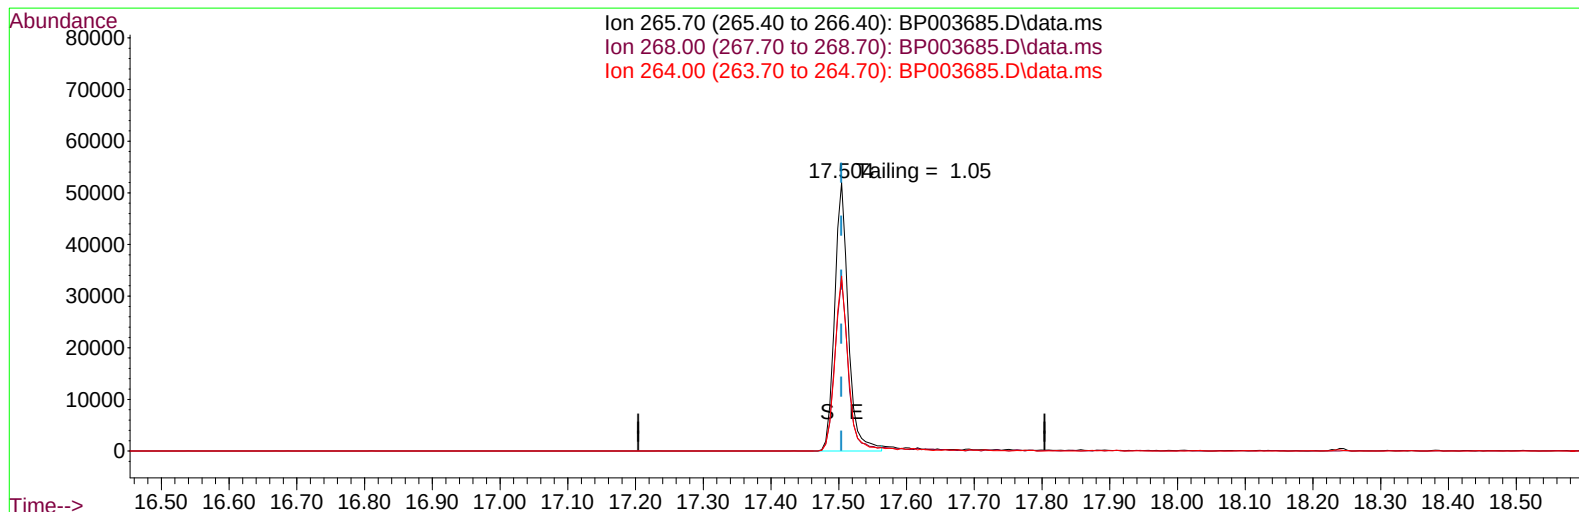

TIC: BP003685.D\data.ms

(70) Pentachlorophenol (C)

17.504min (+ 0.000) 1956402.84 ng

response 74435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.78
264.00	63.30	65.18
0.00	0.00	0.00