

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
 Data File : BP003687.D
 Acq On : 21 Oct 2020 11:41
 Operator : CG/JU
 Sample : PB132413BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132413BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	31	37	54	rVB	3905683	4730776	49.87%	10.281%
2	3.270	54	65	76	rBV3	43973	131157	1.38%	0.285%
3	6.022	525	533	553	rBV	2920986	4350975	45.87%	9.456%
4	7.675	803	814	829	rBV	2700441	4337702	45.73%	9.427%
5	8.528	951	959	968	rBV	561582	906080	9.55%	1.969%
6	9.693	1147	1157	1172	rBV	1787622	3011081	31.74%	6.544%
7	11.369	1434	1442	1450	rBV	664392	1151987	12.14%	2.504%
8	13.757	1840	1848	1855	rBV	4751416	6790045	71.58%	14.757%
9	15.122	2073	2080	2088	rBV	1018964	1518385	16.01%	3.300%
10	16.598	2320	2331	2351	rBV	3238658	4489283	47.33%	9.757%
11	17.845	2536	2543	2555	rBV	1244342	1761868	18.57%	3.829%
12	20.310	2956	2962	2969	rBV	8195000	9485793	100.00%	20.615%
13	21.851	3218	3224	3236	rVB	1343165	1807826	19.06%	3.929%
14	24.427	3653	3662	3672	rBV	737663	1540195	16.24%	3.347%




Sum of corrected areas: 46013153

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
Data File : BP003687.D
Acq On : 21 Oct 2020 11:41
Operator : CG/JU
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132413BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

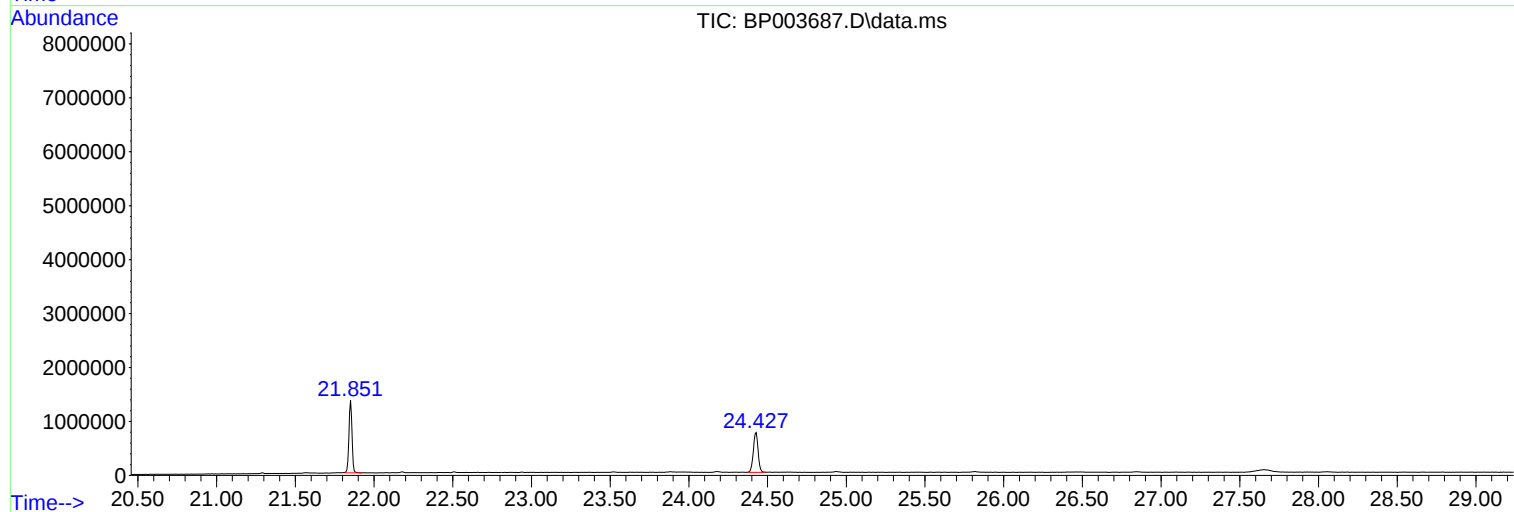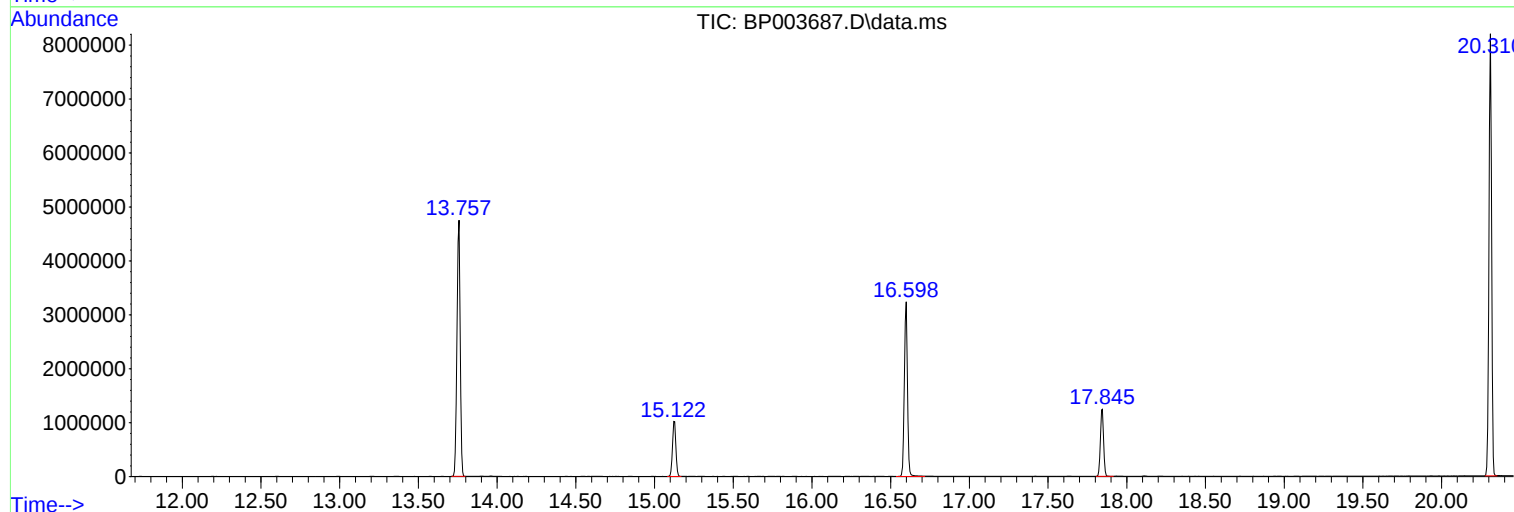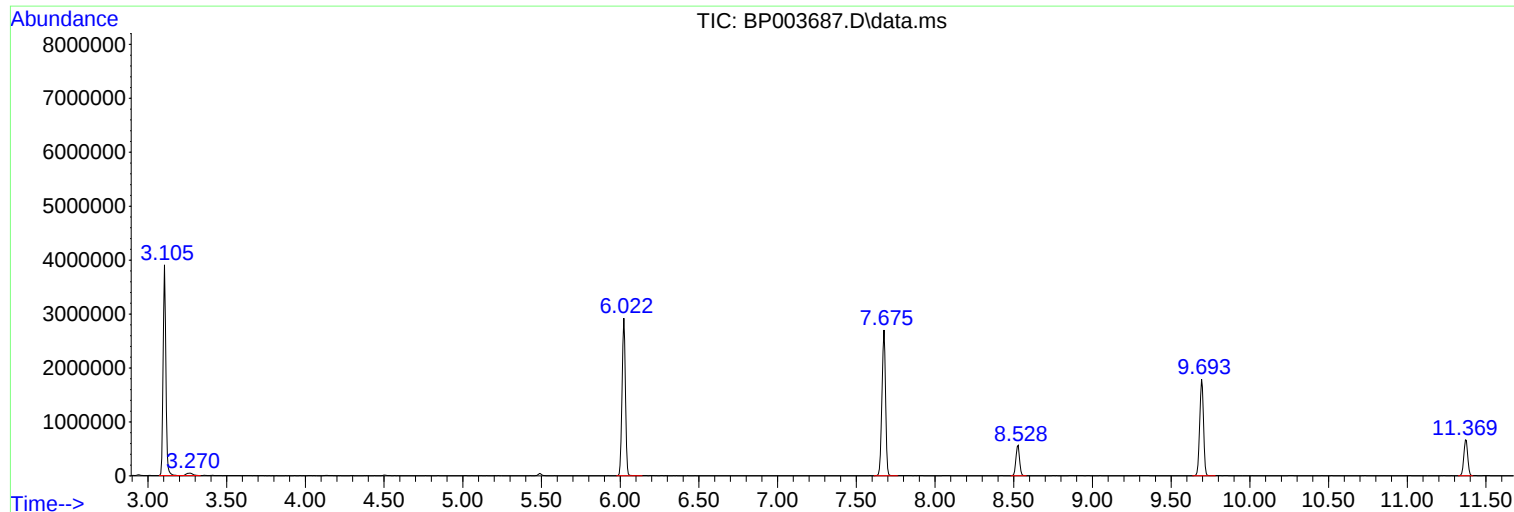

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
Data File : BP003687.D
Acq On : 21 Oct 2020 11:41
Operator : CG/JU
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132413BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.105	104.42 ng	4730780	1,4-Dichlorobenzene-d4	8.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	50
2			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9
4			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
5			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	7

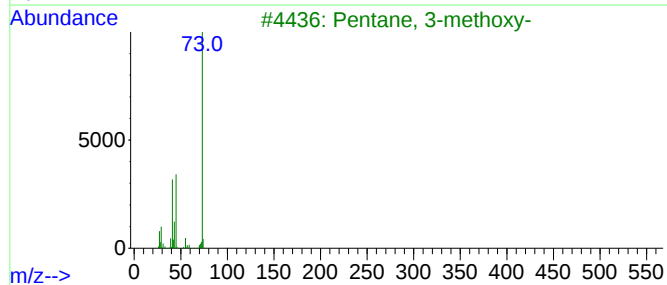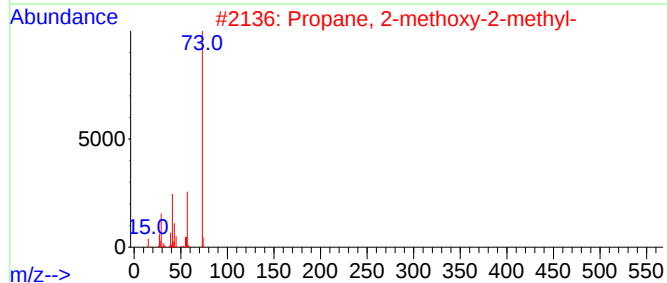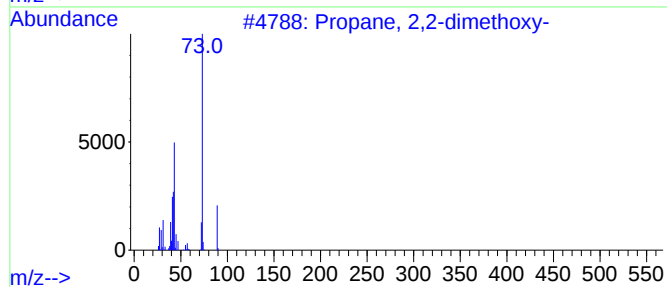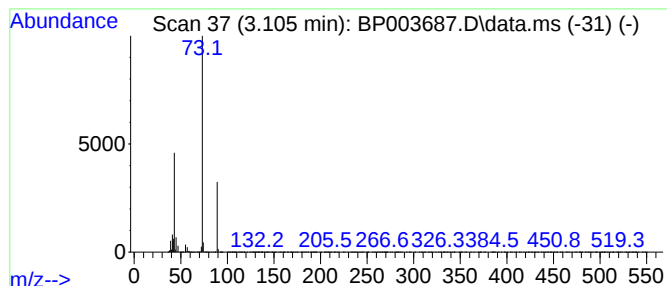

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
Data File : BP003687.D
Acq On : 21 Oct 2020 11:41
Operator : CG/JU
Sample : PB132413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132413BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-di...	3.105	104.4	ng	4730780	1	8.528	906080	20.0