


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102120\
 Data File : BP003685.D
 Acq On : 21 Oct 2020 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP101920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 19 14:54:24 2020

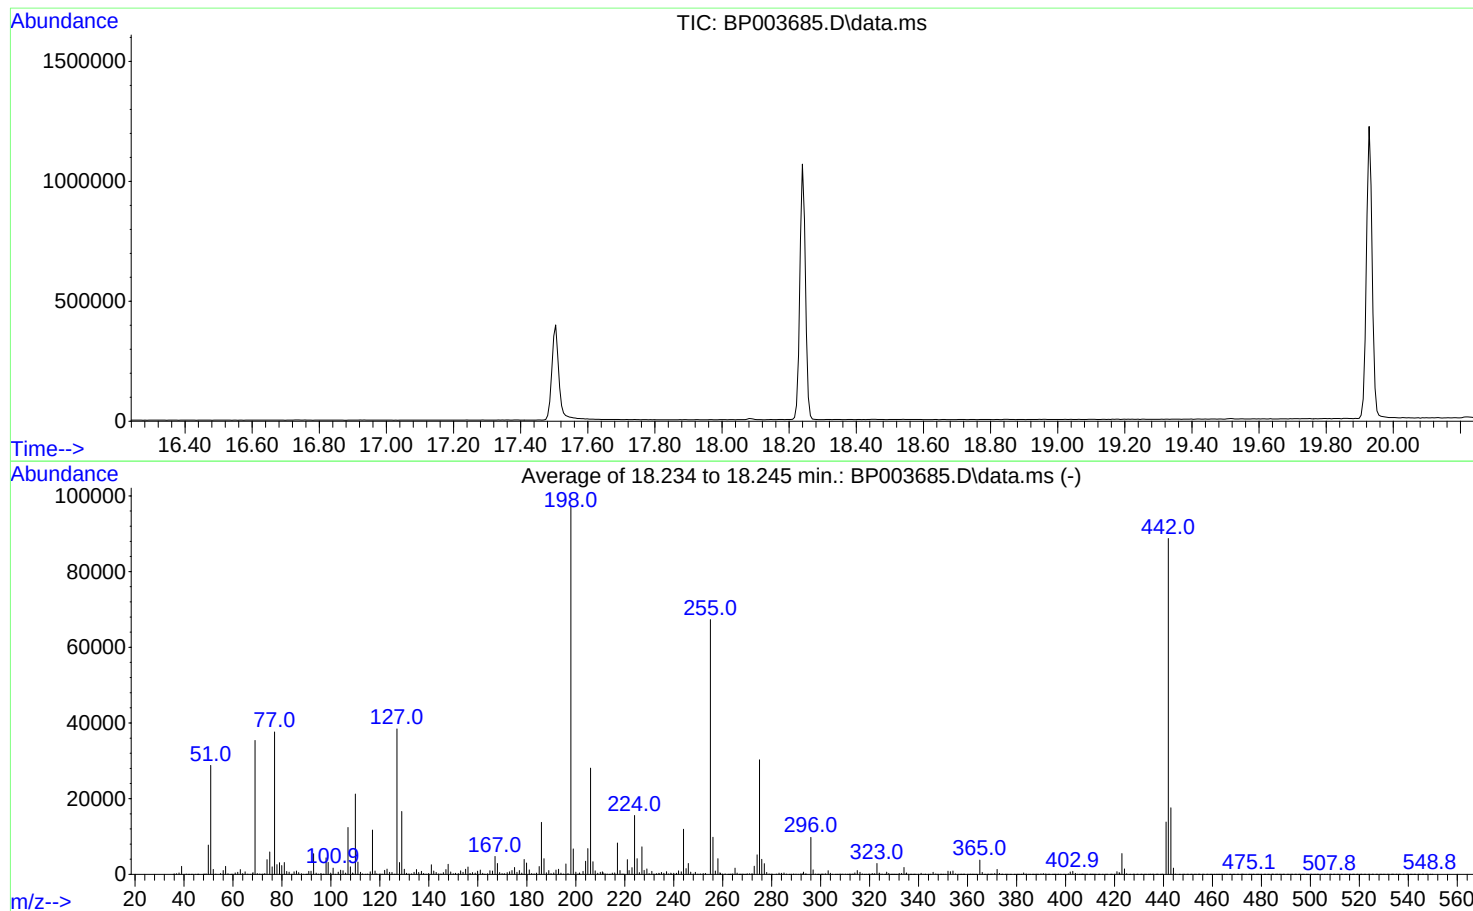

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	28791	PASS
68	69	0.00	2	1.3	467	PASS
69	198	0.00	100	36.4	35373	PASS
70	69	0.00	2	0.6	227	PASS
127	198	10	80	39.5	38419	PASS
197	198	0.00	2	0.2	213	PASS
198	198	100	100	100.0	97200	PASS
199	198	5	9	6.9	6723	PASS
275	198	10	60	31.2	30292	PASS
365	198	1	100	3.9	3757	PASS
441	198	0.01	100	14.2	13846	PASS
442	198	50	100	91.3	88752	PASS
443	442	15	24	19.8	17579	PASS