


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007659.D
Acq On : 26 Oct 2021 01:36
Operator : CG/JU
Sample : M4304-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P061-TW001-01

Manual Integrations
APPROVED

mohammad
10/26/2021 11:34:49 AM

Quant Time: Oct 26 04:22:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 25 16:57:16 2021
Response via : Initial Calibration

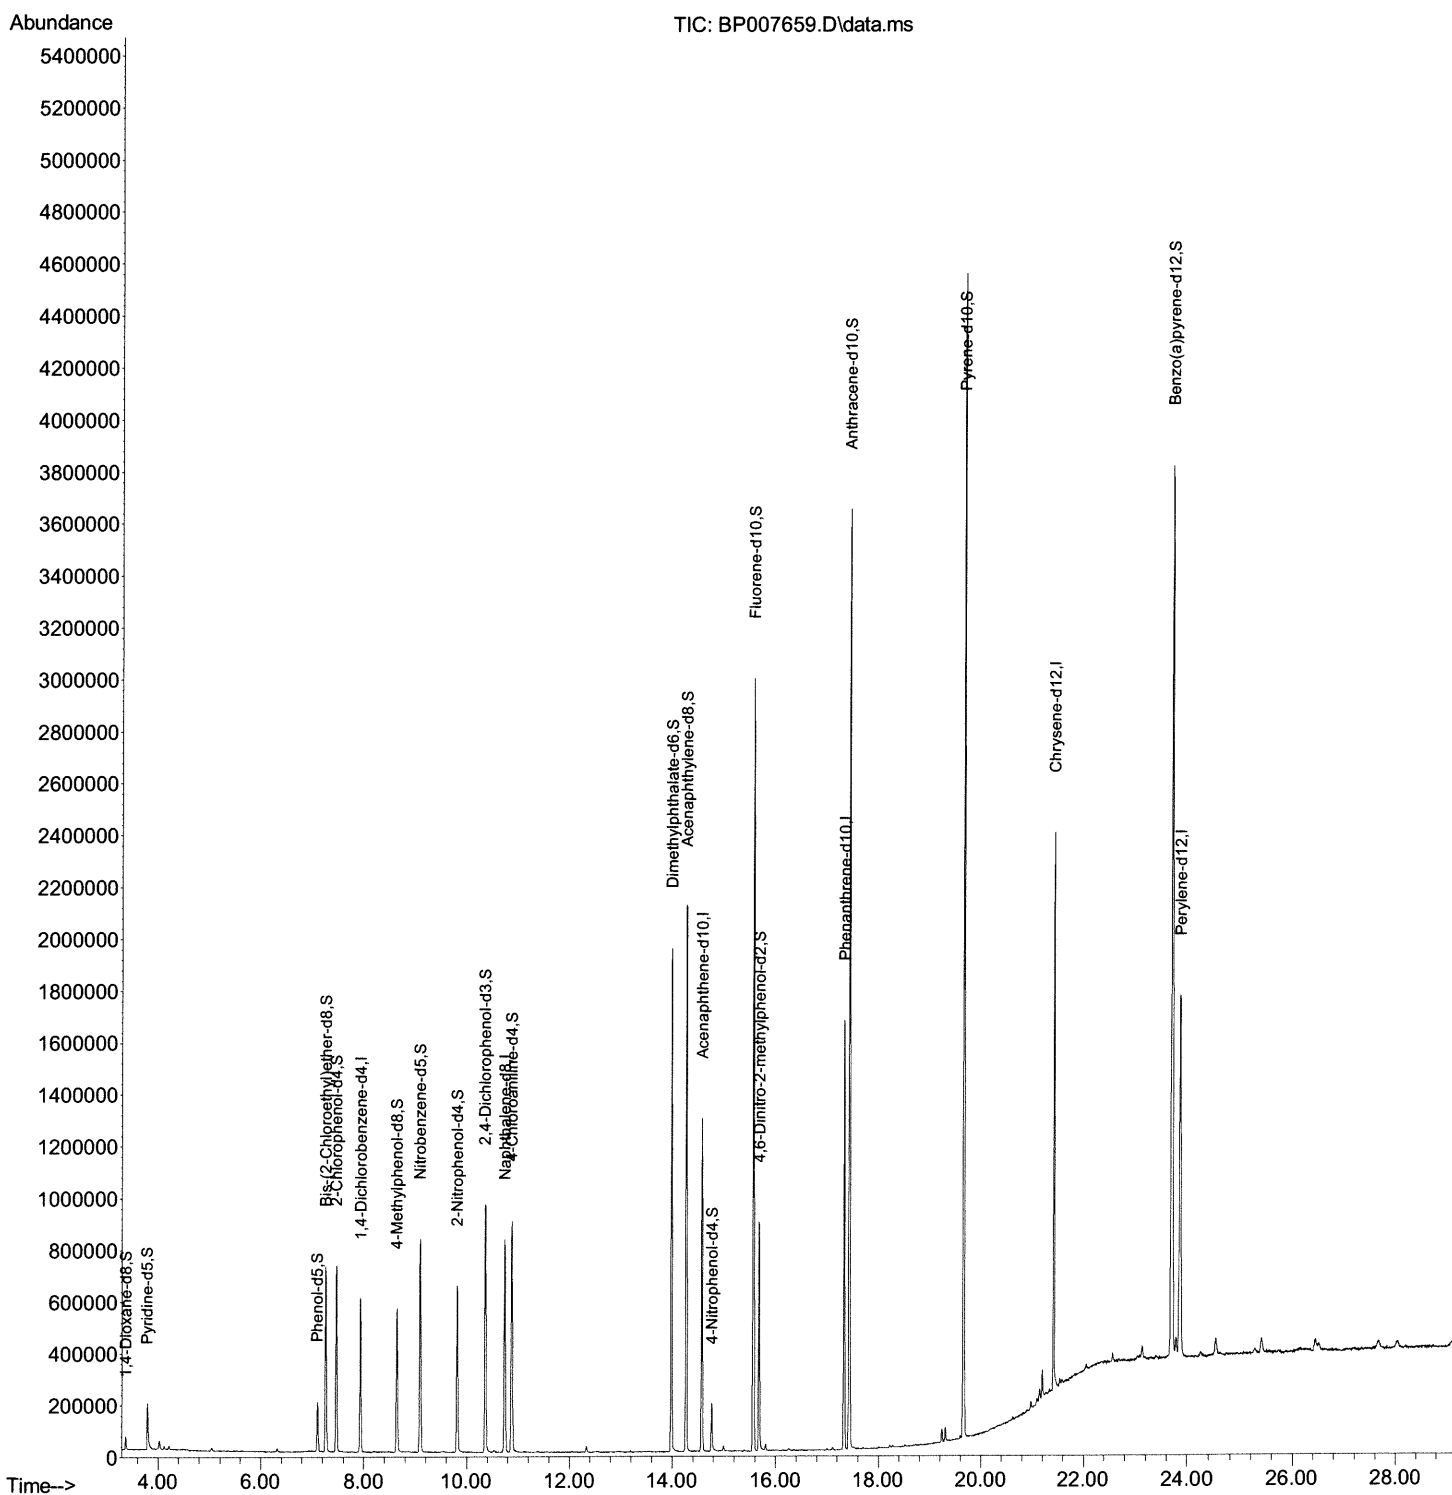

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007659.D
 Acq On : 26 Oct 2021 01:36
 Operator : CG/JU
 Sample : M4304-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P061-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:49 AM

Quant Time: Oct 26 04:22:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

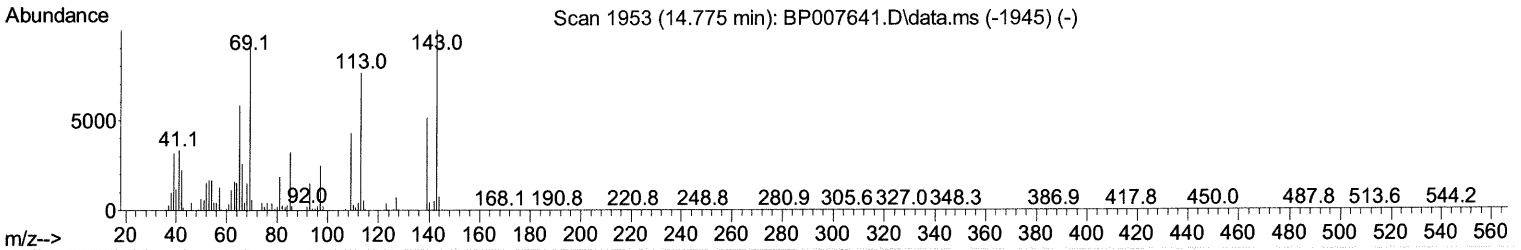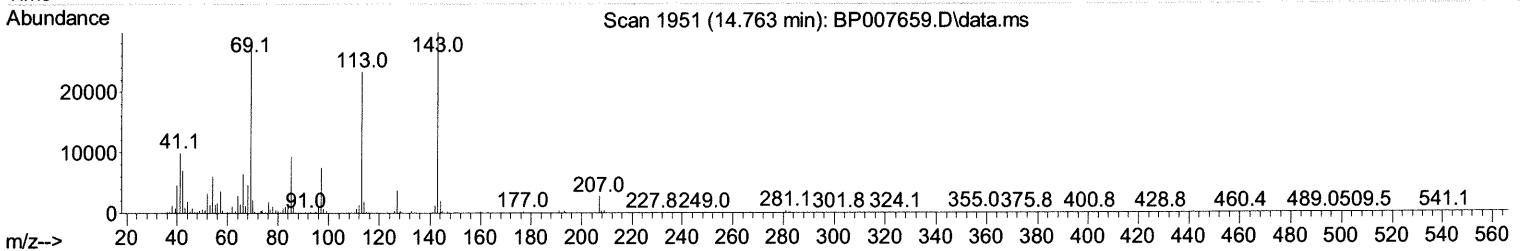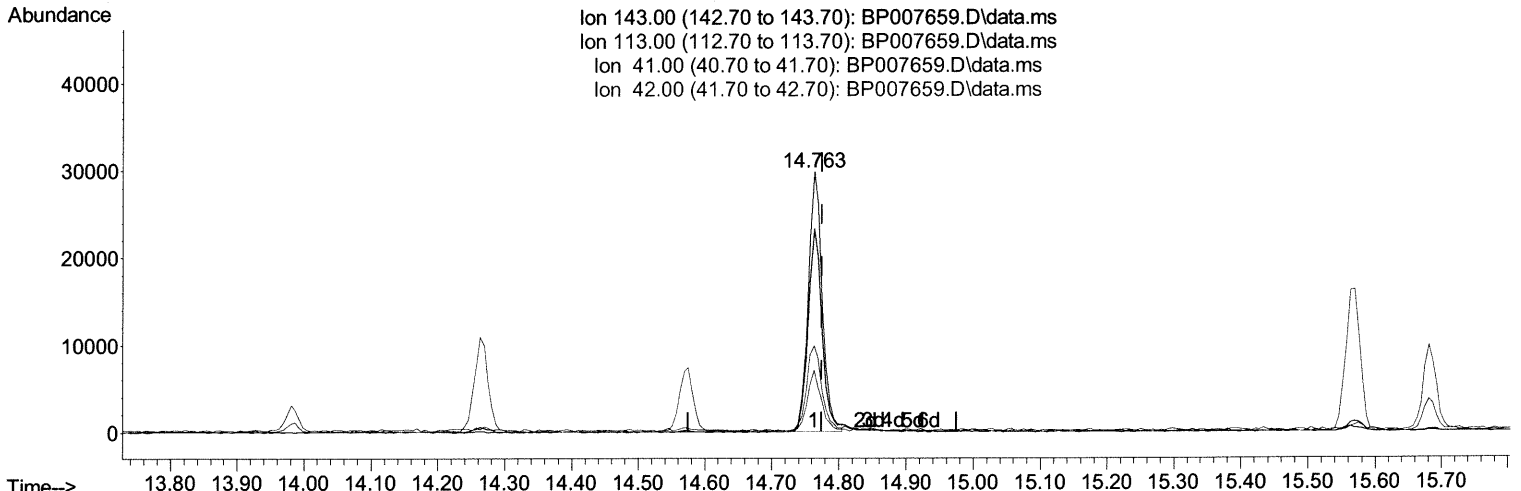

TIC: BP007659.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.012) 7.87 ng/ul

response 42819

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.90	78.09
41.00	39.60	33.24
42.00	25.40	23.71

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007659.D
 Acq On : 26 Oct 2021 01:36
 Operator : CG/JU
 Sample : M4304-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P061-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:49 AM

Quant Time: Oct 26 04:22:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

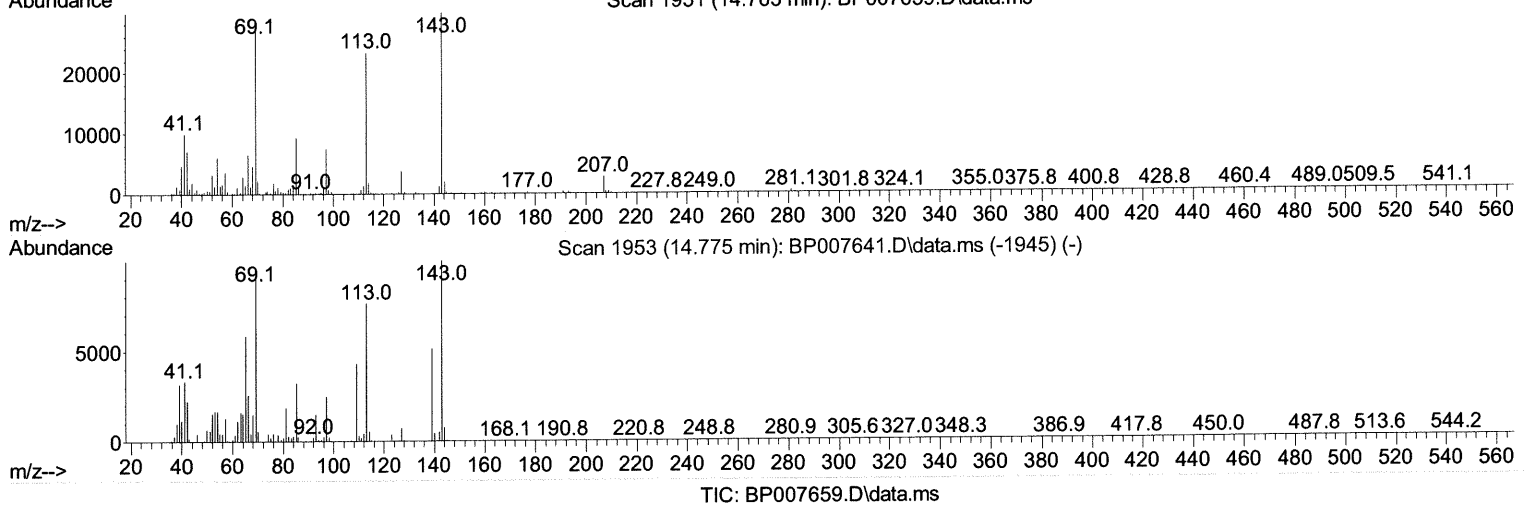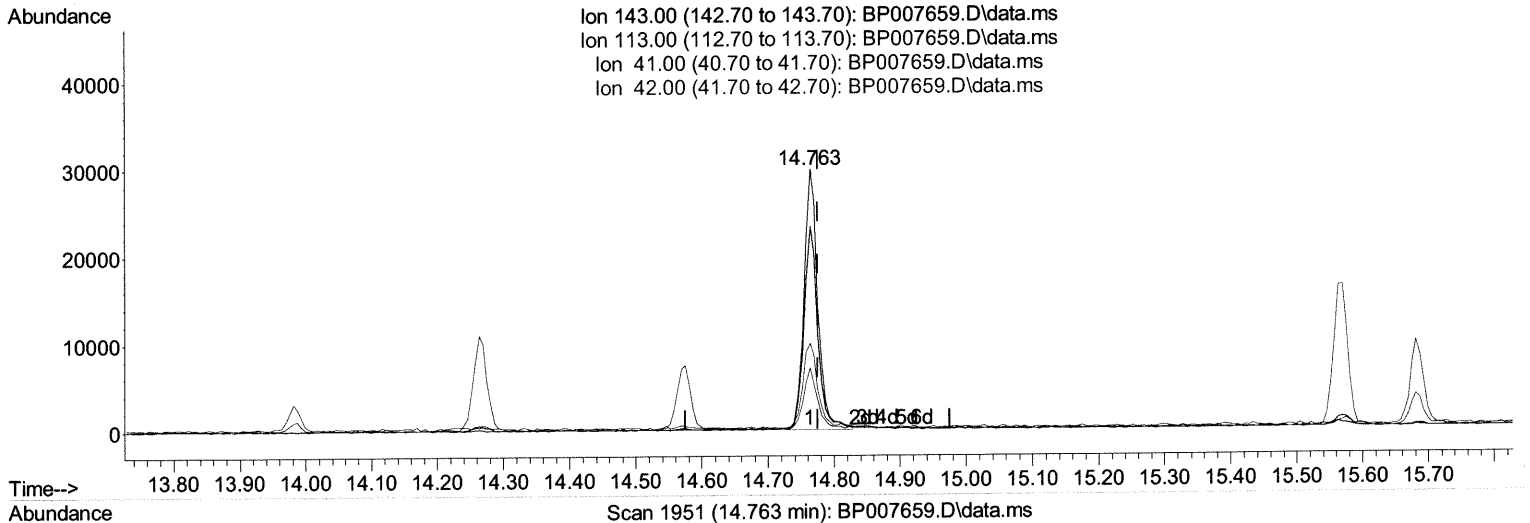

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.012) 8.01 ng/ul m

10/27/21 JU

response 43592

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.90	78.09
41.00	39.60	33.24
42.00	25.40	23.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007659.D
 Acq On : 26 Oct 2021 01:36
 Operator : CG/JU
 Sample : M4304-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P061-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:49 AM

Quant Time: Oct 26 04:22:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	167616	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	673999	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	438146	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	956666	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	1056115	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	1103759	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	24236	6.568	ng/uL	0.00
4) Pyridine-d5	3.787	84	105872	9.488	ng/ul	0.00
7) Phenol-d5	7.099	99	111369	8.748	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	306611	43.377	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	329150	33.241	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	205650	20.629	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	200214	43.590	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	208869	41.636	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.357	165	370583	36.292	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.875	131	474698	35.159	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	1346612	45.373	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1552574	42.681	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	43592m	8.013	ng/ul	>-0.01 10/27/21 JU
60) Fluorene-d10	15.569	176	1178124	47.087	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	197549	38.605	ng/ul	0.00
73) Anthracene-d10	17.428	188	2063593	52.488	ng/ul	0.00
81) Pyrene-d10	19.663	212	2523041	51.313	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	2658307	49.027	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed