


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007662.D
Acq On : 26 Oct 2021 03:18
Operator : CG/JU
Sample : M4304-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P059-TW001-01

Manual Integrations
APPROVED

mohammad
10/26/2021 11:34:51 AM

Quant Time: Oct 26 04:35:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 25 16:57:16 2021
Response via : Initial Calibration

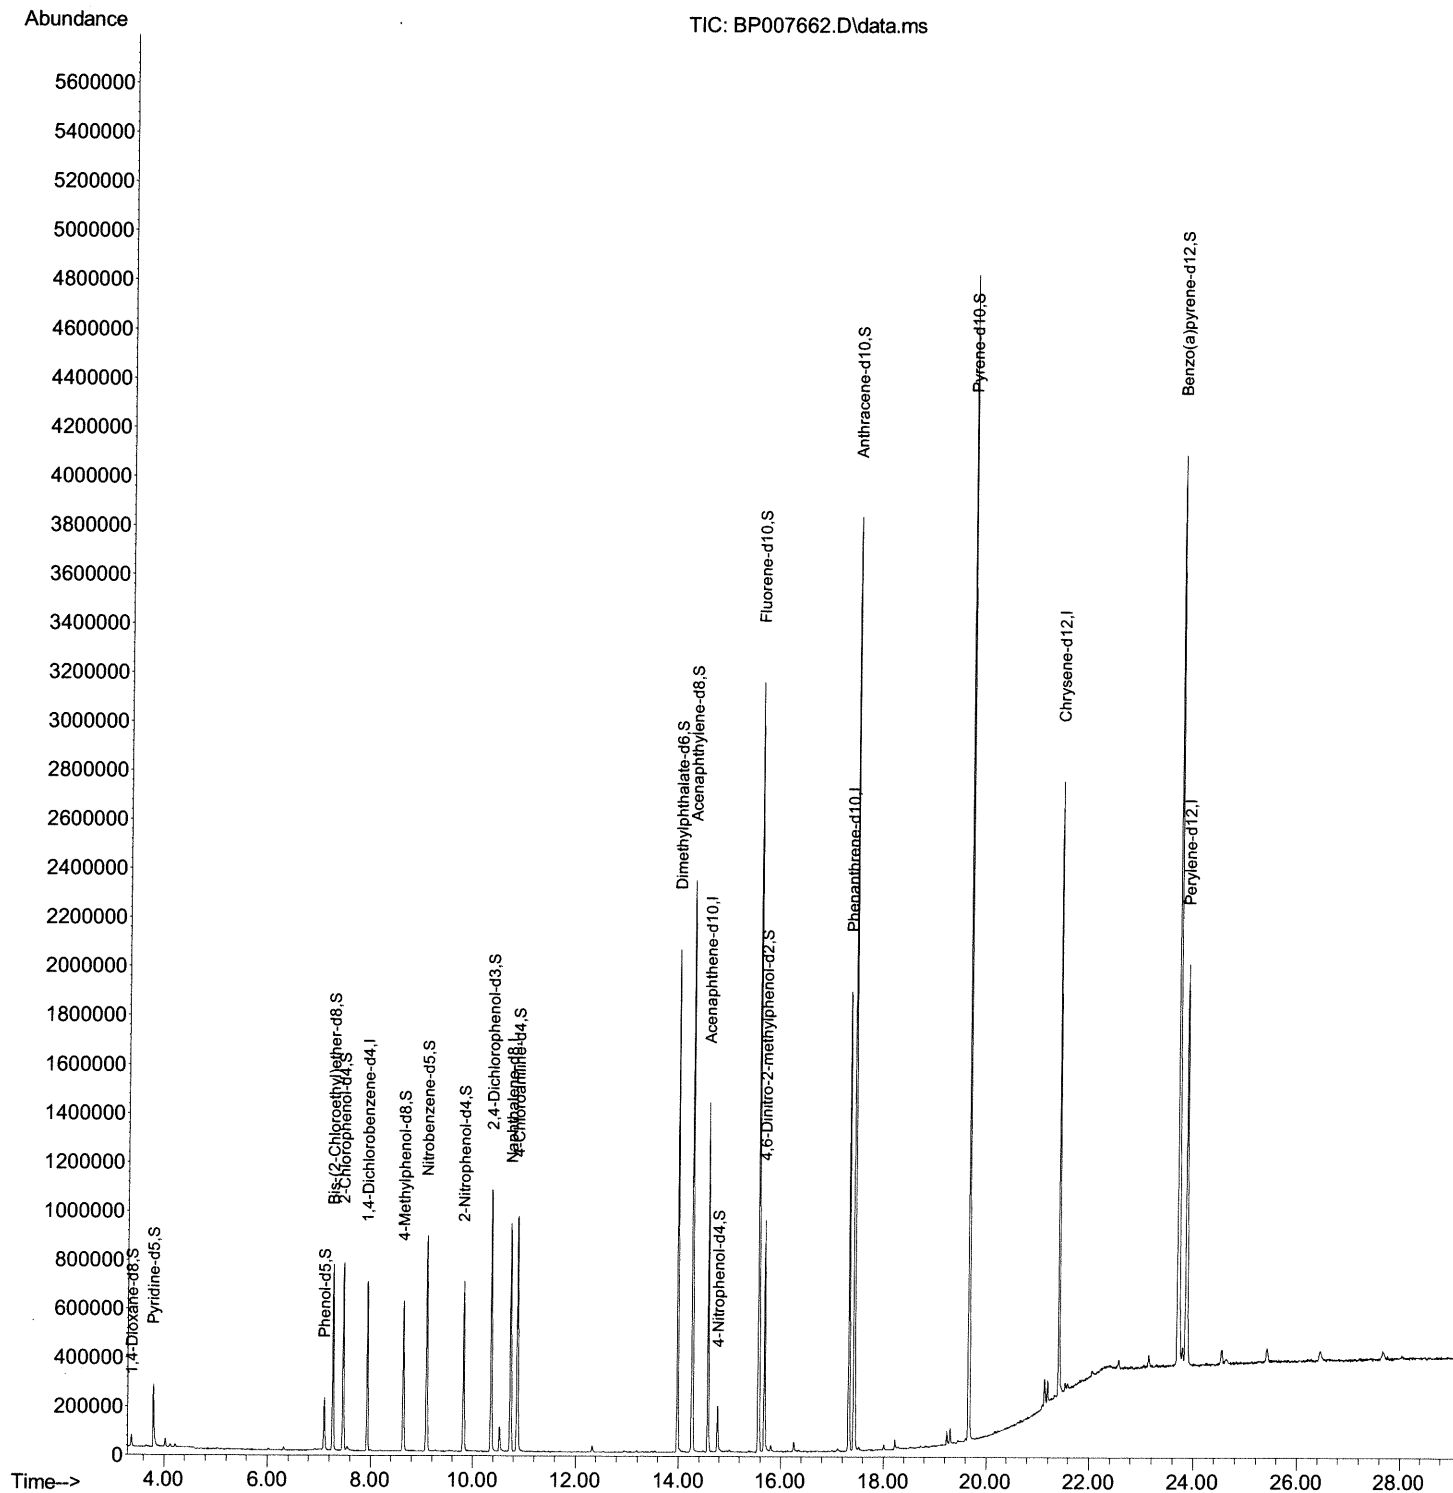

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007662.D
 Acq On : 26 Oct 2021 03:18
 Operator : CG/JU
 Sample : M4304-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P059-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:51 AM

Quant Time: Oct 26 04:35:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

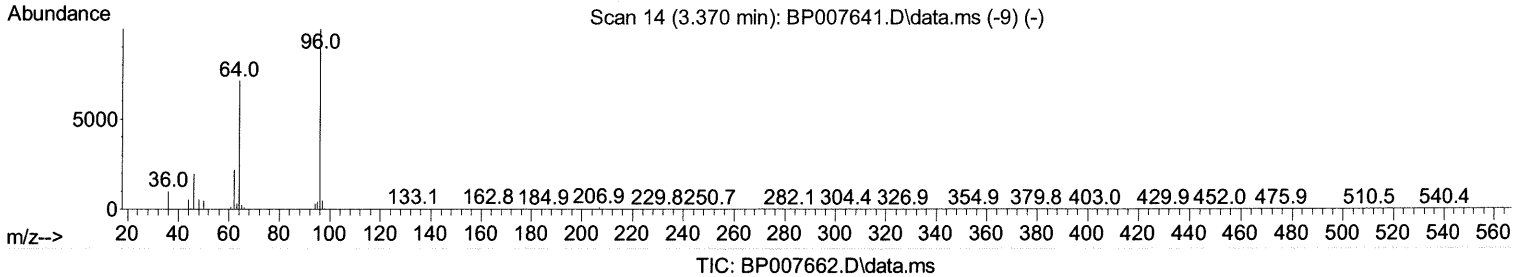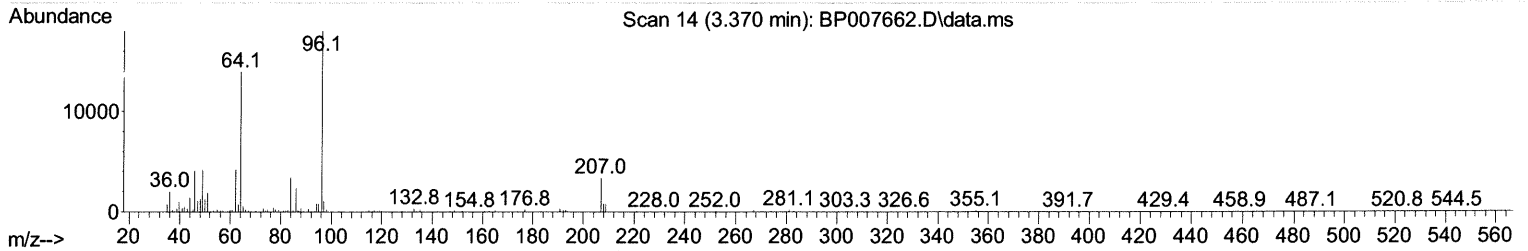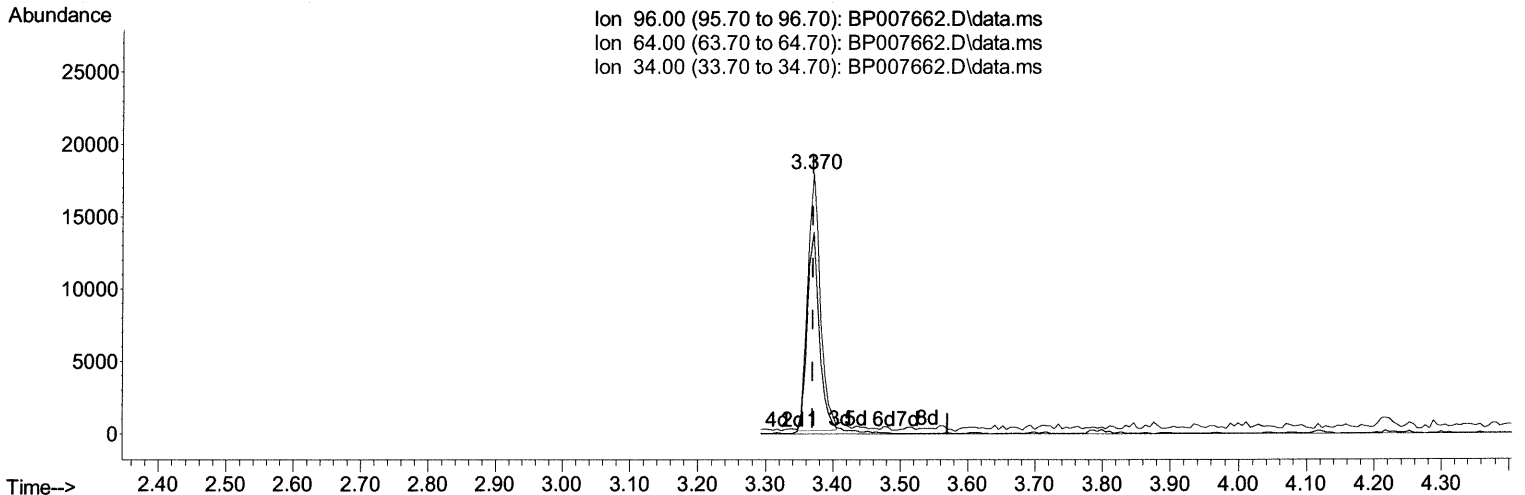

(3) 1,4-Dioxane-d8 (S)

3.370min (-0.000) 5.57 ng/uL

response 23752

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	77.48
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007662.D
 Acq On : 26 Oct 2021 03:18
 Operator : CG/JU
 Sample : M4304-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P059-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:51 AM

Quant Time: Oct 26 04:35:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

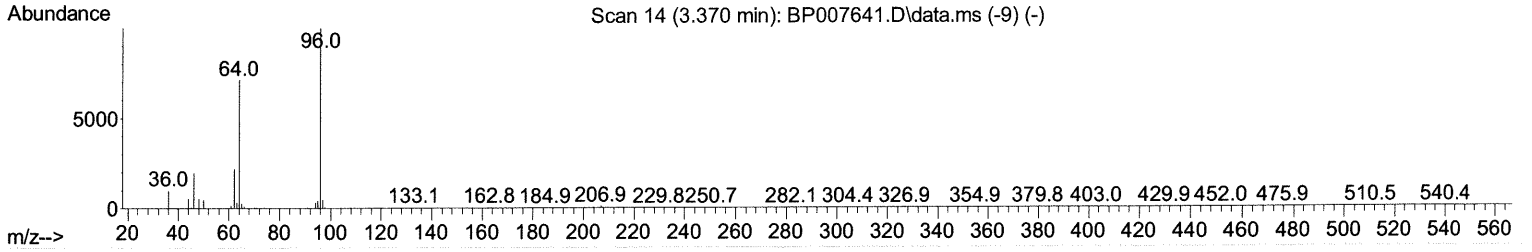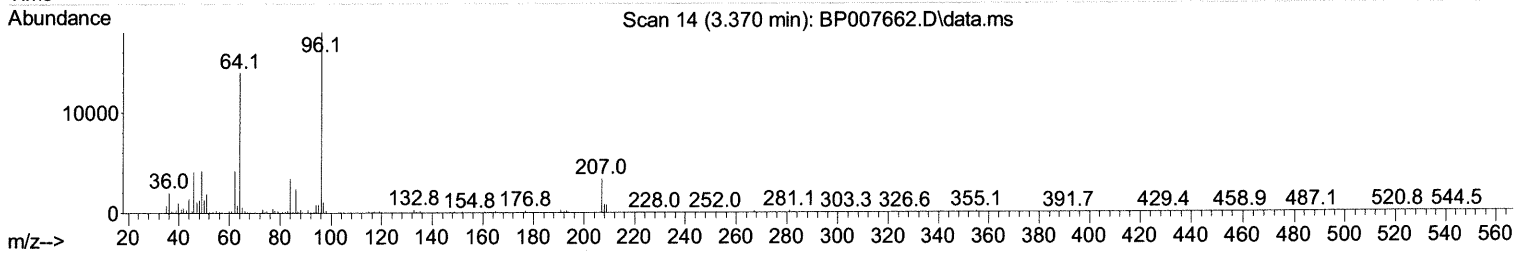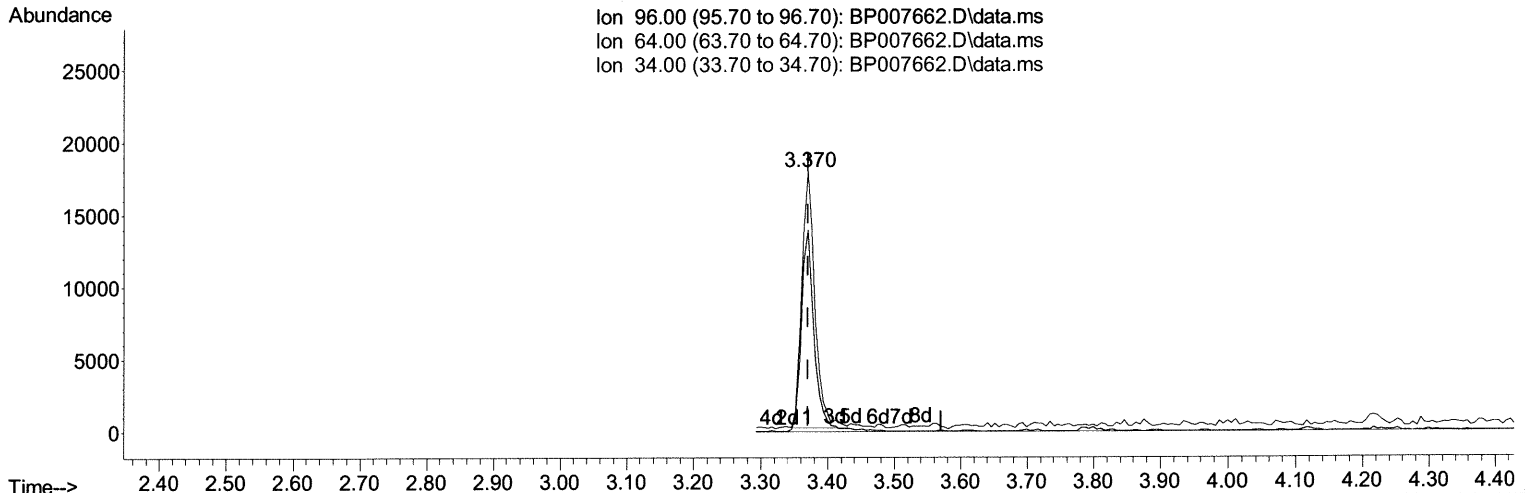

TIC: BP007662.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (-0.000) 5.67 ng/uL m 10/27/2021

response 24207

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	77.48
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007662.D
 Acq On : 26 Oct 2021 03:18
 Operator : CG/JU
 Sample : M4304-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P059-TW001-01

Manual Integrations
 APPROVED

mohammad
 10/26/2021 11:34:51 AM

Quant Time: Oct 26 04:35:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	193856	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	778627	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	512105	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1131240	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	1231984	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	1297313	20.000	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.370	96	24207m >	5.672	ng/ul >	0.00
4) Pyridine-d5	3.787	84	146305	11.337	ng/ul	0.00
7) Phenol-d5	7.099	99	121842	8.275	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	327490	40.060	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	351093	30.658	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	226799	19.671	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	215241	40.565	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	223135	38.502	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.358	165	397830	33.725	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.875	131	519098	33.281	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1383207	39.875	ng/ul	-0.01
49) Acenaphthylene-d8	14.263	160	1661698	39.084	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	47192	7.422	ng/ul	-0.01
60) Fluorene-d10	15.569	176	1234063	42.199	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	214550	35.457	ng/ul	0.00
73) Anthracene-d10	17.428	188	2188464	47.074	ng/ul	0.00
81) Pyrene-d10	19.657	212	2665114	46.465	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	2856532	44.823	ng/ul	0.00

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed