


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007687.D
Acq On : 26 Oct 2021 20:09
Operator : CG/JU
Sample : M4291-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P002-TW001-03

Manual Integrations
APPROVED

mohammad
10/27/2021 11:50:37 AM

Quant Time: Oct 27 00:55:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 25 16:57:16 2021
Response via : Initial Calibration

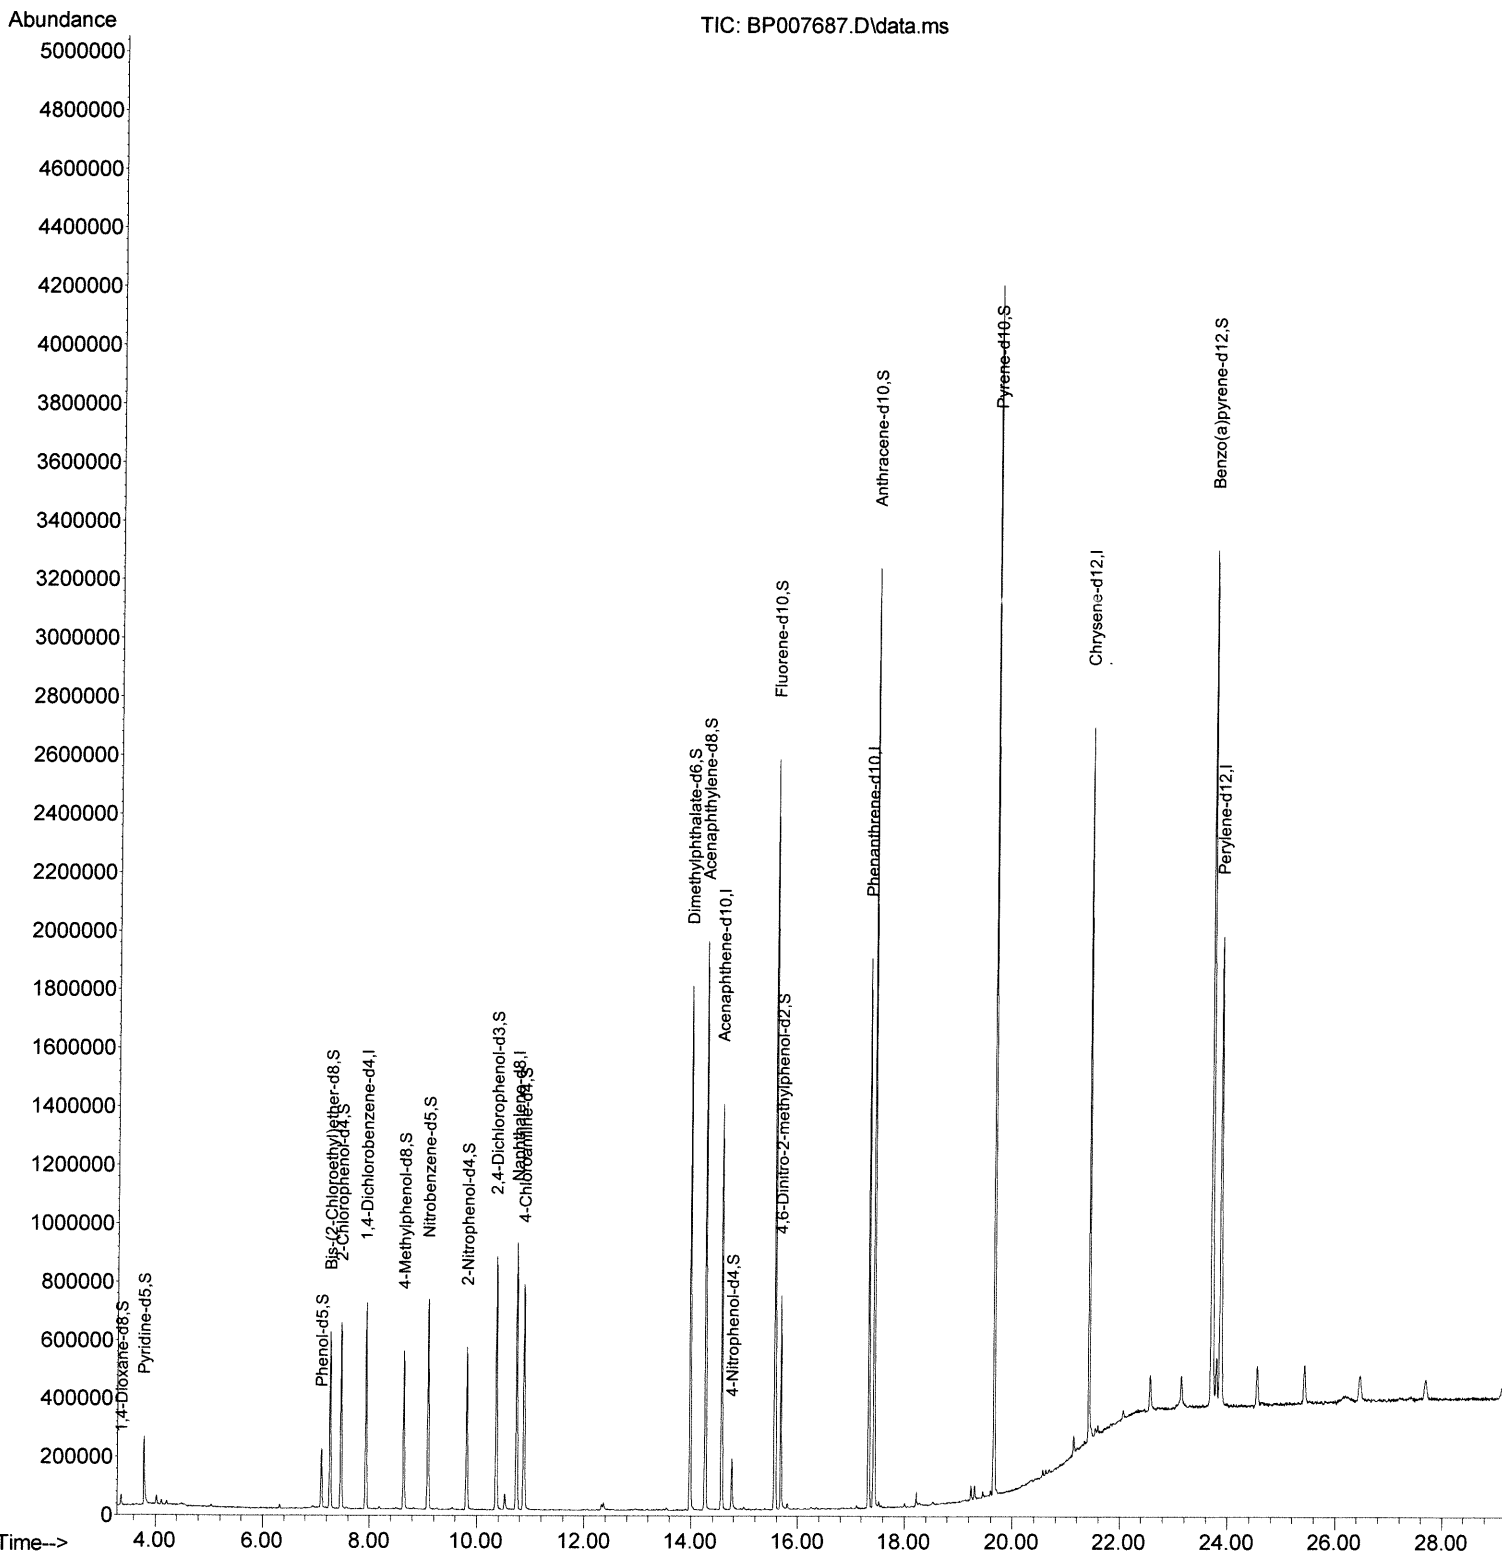




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007687.D
 Acq On : 26 Oct 2021 20:09
 Operator : CG/JU
 Sample : M4291-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P002-TW001-03

Manual Integrations
 APPROVED

mohammad
 10/27/2021 11:50:37 AM

Quant Time: Oct 27 00:55:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

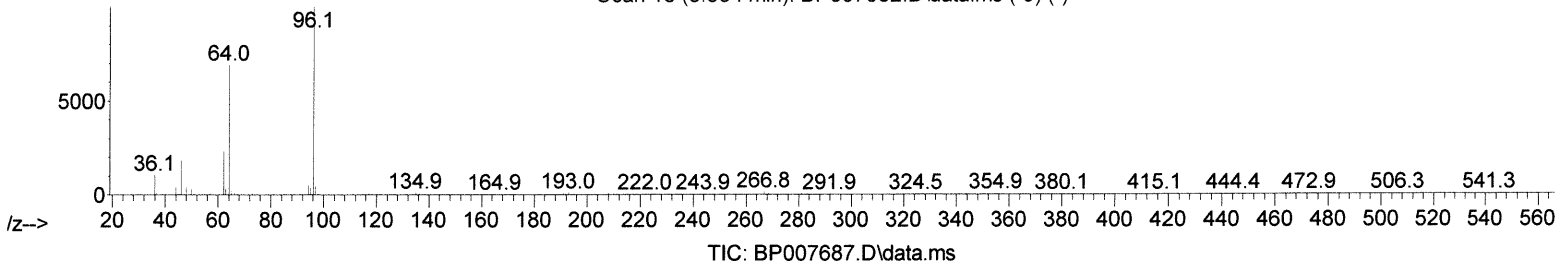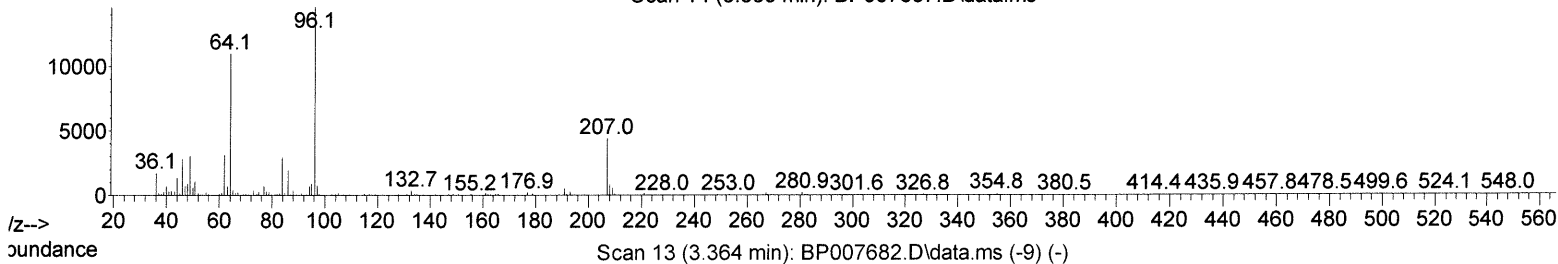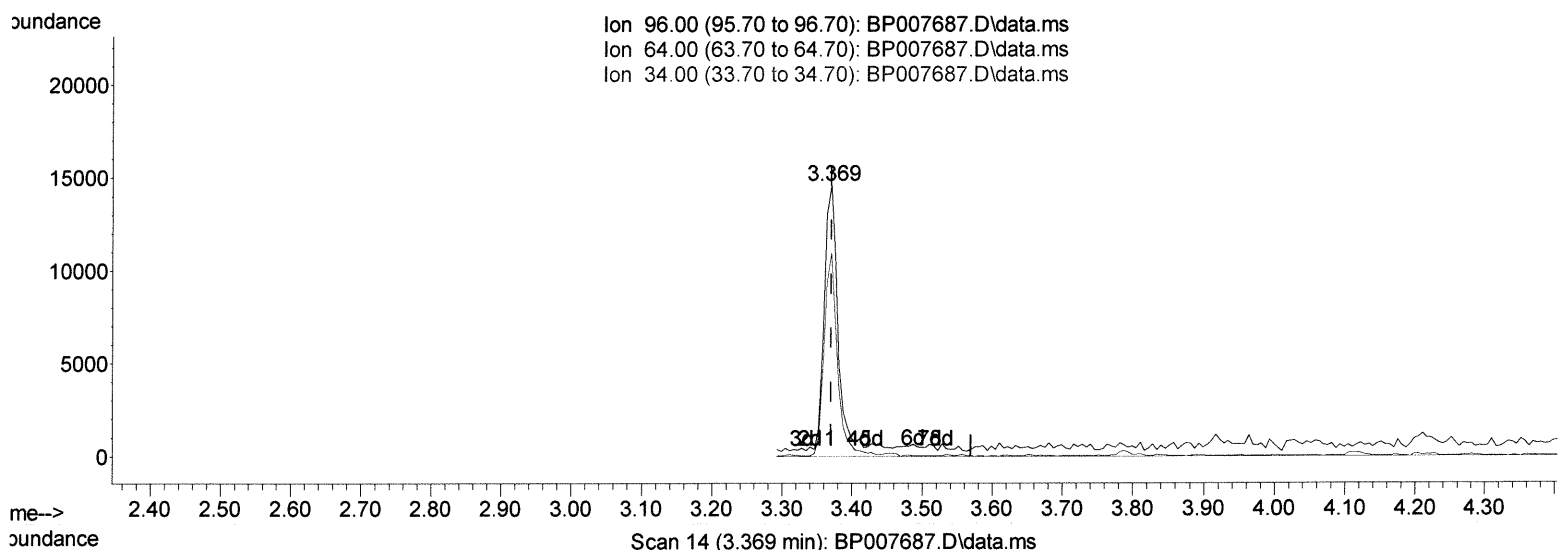

TIC: BP007687.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (-0.001) 4.54 ng/uL




response	19003	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	75.11
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007687.D
 Acq On : 26 Oct 2021 20:09
 Operator : CG/JU
 Sample : M4291-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P002-TW001-03

Manual Integrations
 APPROVED
 mohammad
 10/27/2021 11:50:37 AM

Quant Time: Oct 27 00:55:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

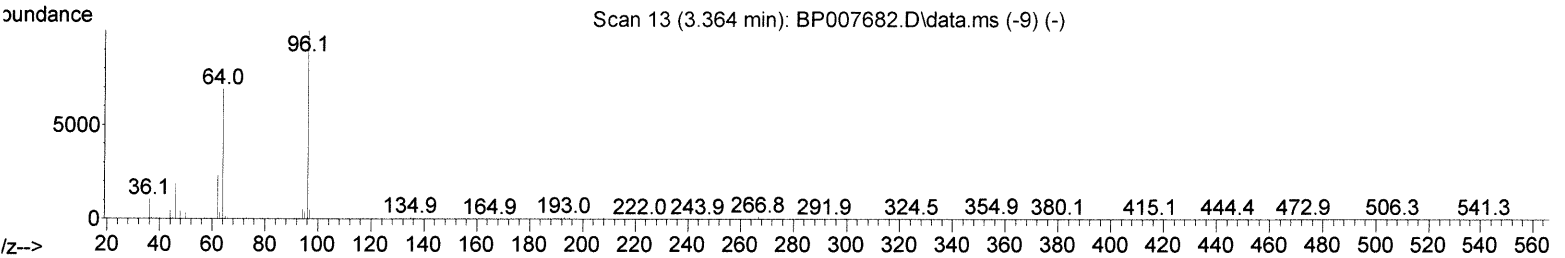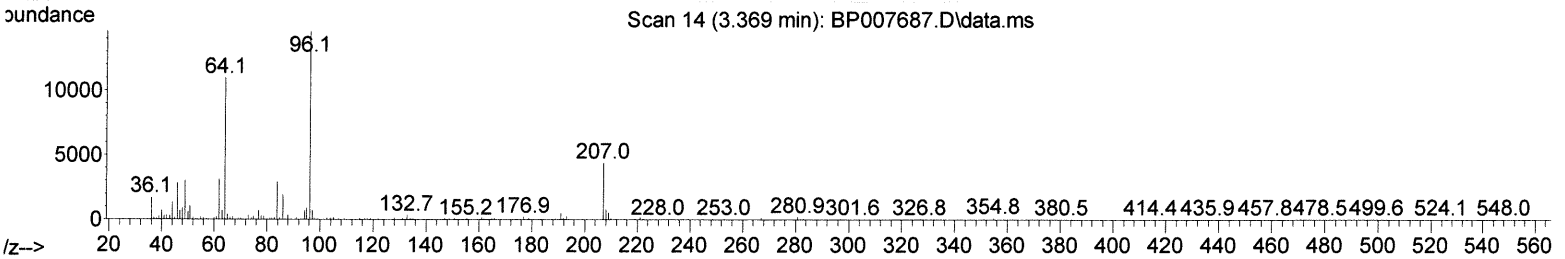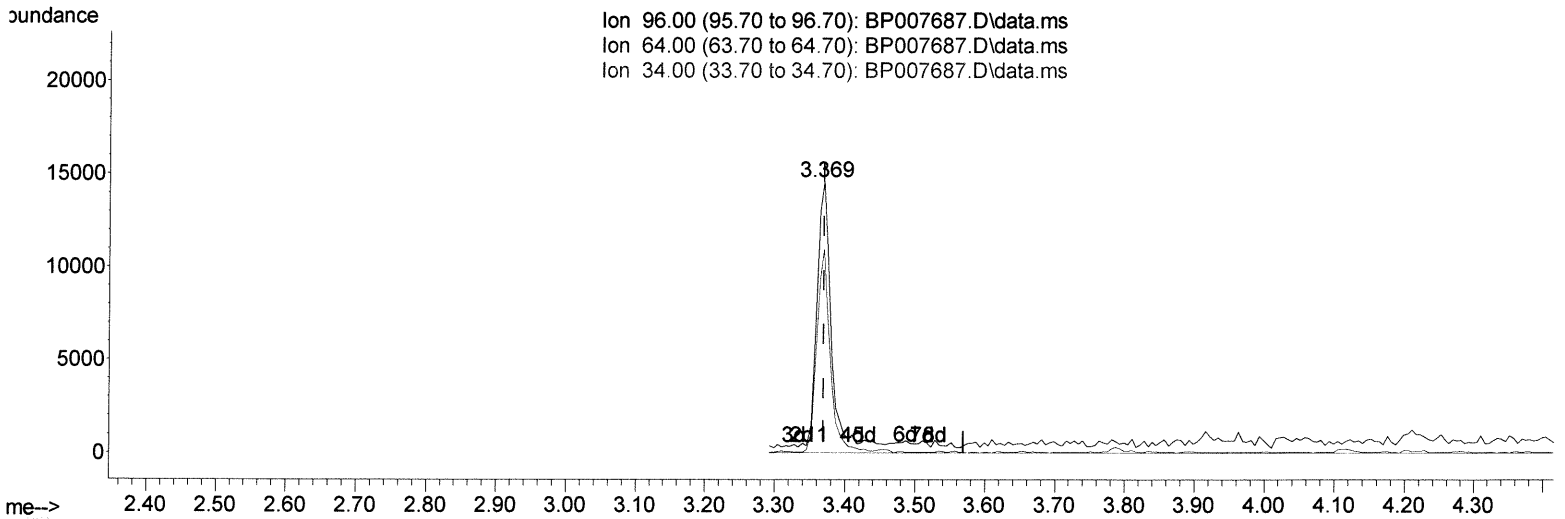

TIC: BP007687.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (-0.001) 4.60 ng/uL m 10/20/21 JU

response	19235	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	75.11
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007687.D
 Acq On : 26 Oct 2021 20:09
 Operator : CG/JU
 Sample : M4291-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P002-TW001-03

Manual Integrations
 APPROVED

mohammad
 10/27/2021 11:50:37 AM

Quant Time: Oct 27 00:55:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	189961	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	760092	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	502903	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.327	188	1096912	20.000	ng/ul	0.00
79) Chrysene-d12	21.415	240	1186082	20.000	ng/ul	0.00
88) Perylene-d12	23.862	264	1255703	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	19235m	4.600	ng/uL	0.00 10/29/21 JU
4) Pyridine-d5	3.787	84	132373	10.468	ng/ul	0.00
7) Phenol-d5	7.099	99	114100	7.908	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	259401	32.382	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	297480	26.509	ng/ul	-0.01
15) 4-Methylphenol-d8	8.640	113	199551	17.662	ng/ul	-0.01
21) Nitrobenzene-d5	9.093	128	171561	33.121	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	176505	31.199	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.357	165	324265	28.159	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.869	131	417480	27.419	ng/ul	-0.01
46) Dimethylphthalate-d6	13.981	166	1193450	35.034	ng/ul	-0.01
49) Acenaphthylene-d8	14.263	160	1353138	32.409	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	42842	6.861	ng/ul	-0.01
60) Fluorene-d10	15.569	176	1033617	35.992	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	159092	27.115	ng/ul	0.00
73) Anthracene-d10	17.427	188	1772136	39.312	ng/ul	0.00
81) Pyrene-d10	19.663	212	2170539	39.307	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	2231170	36.170	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed