


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007731.D
Acq On : 27 Oct 2021 21:45
Operator : CG/JU
Sample : M4215-17
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF4

Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:15 AM

Quant Time: Oct 28 01:36:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration

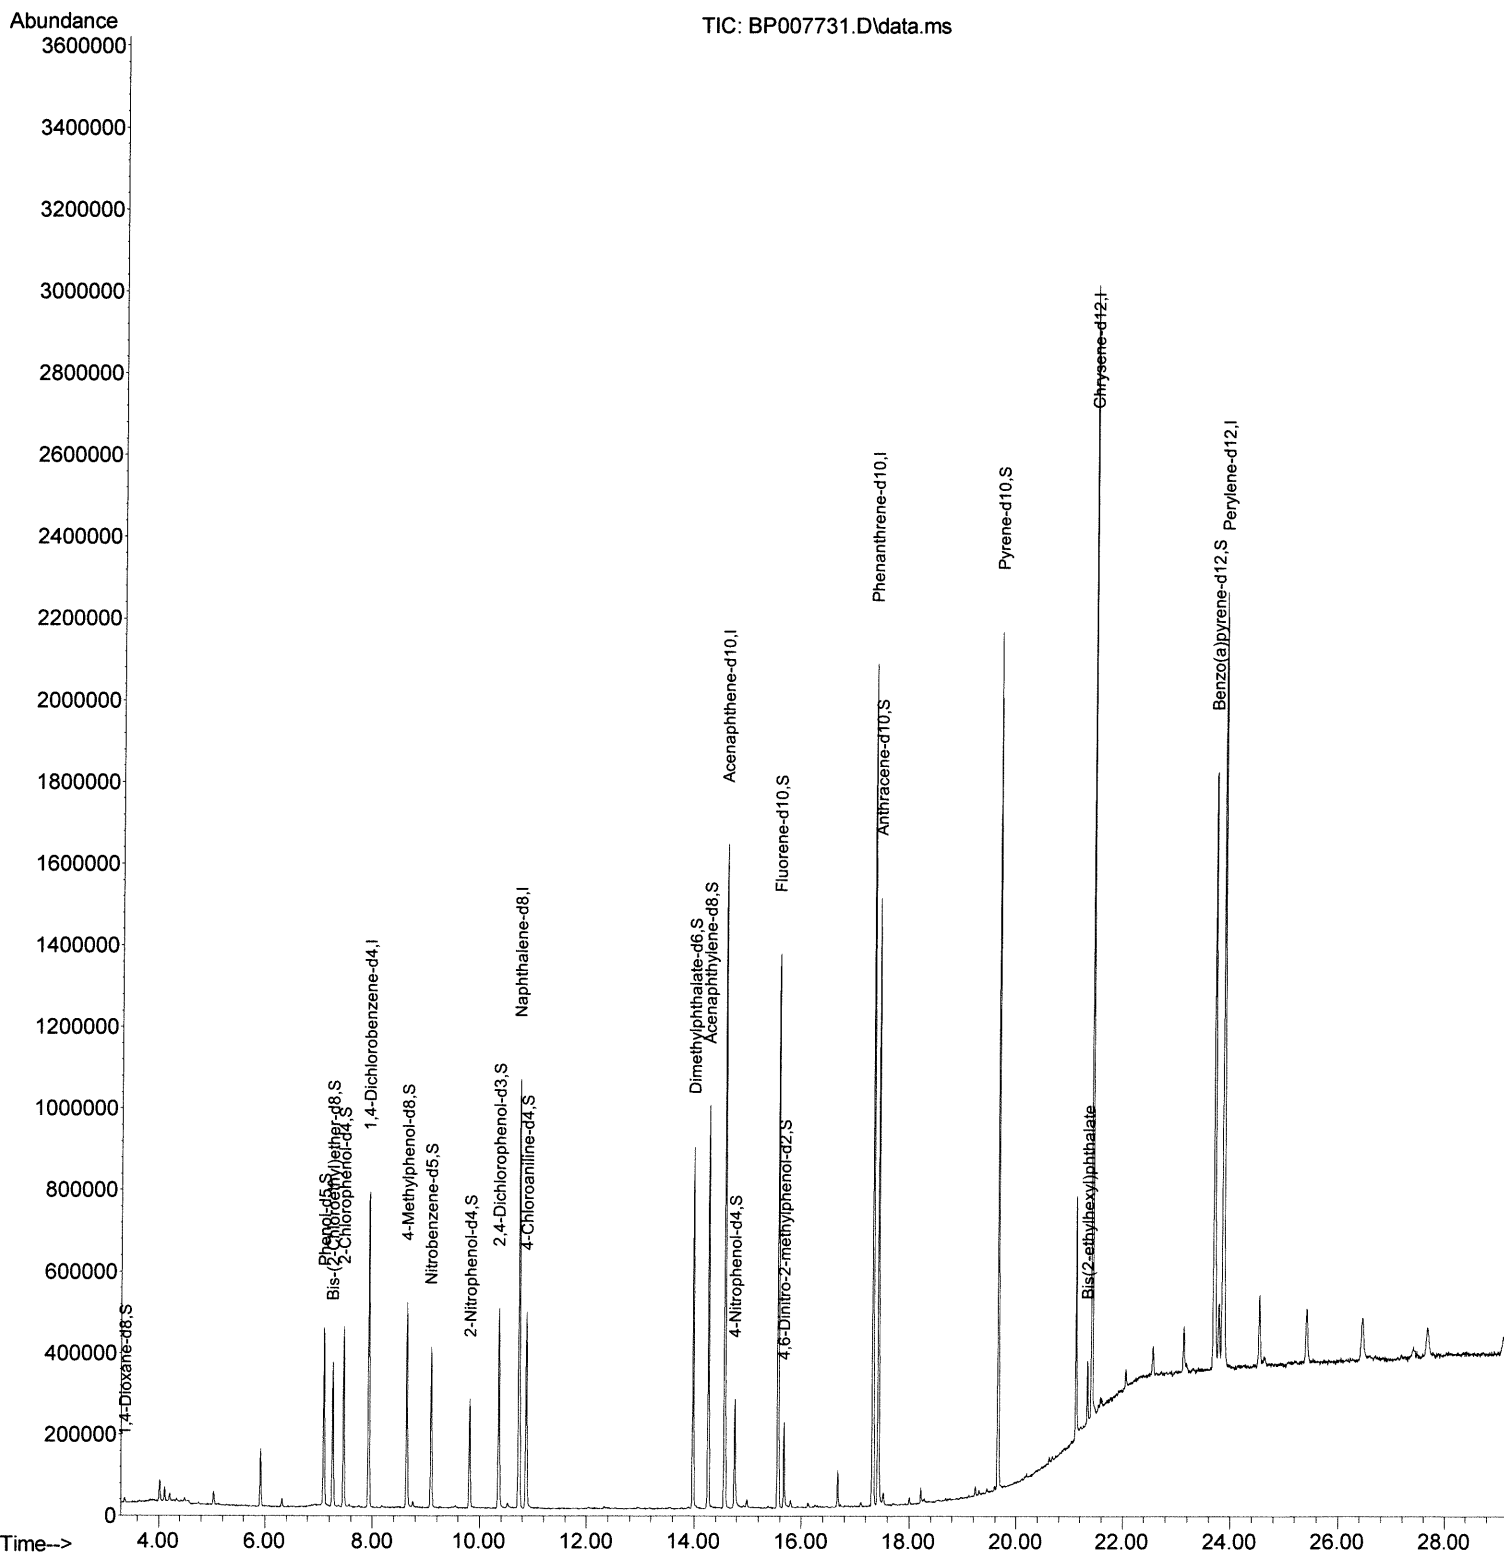




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007731.D
 Acq On : 27 Oct 2021 21:45
 Operator : CG/JU
 Sample : M4215-17
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF4

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:12:15 AM

Quant Time: Oct 28 01:36:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

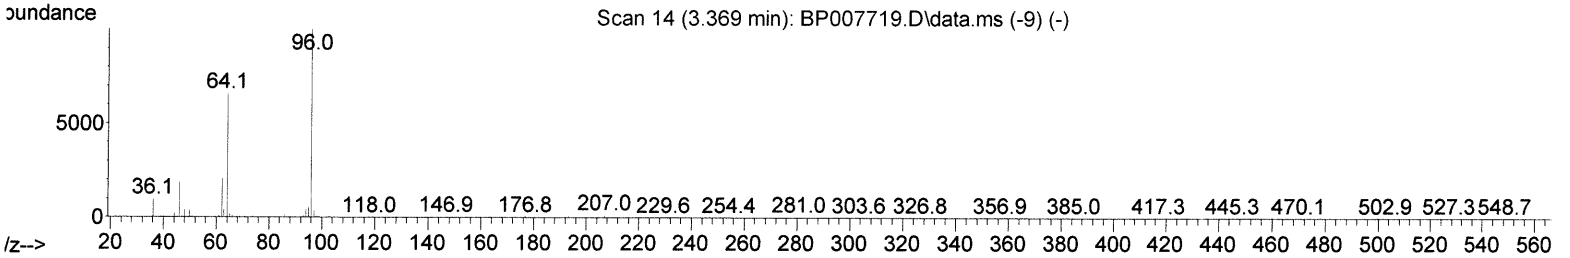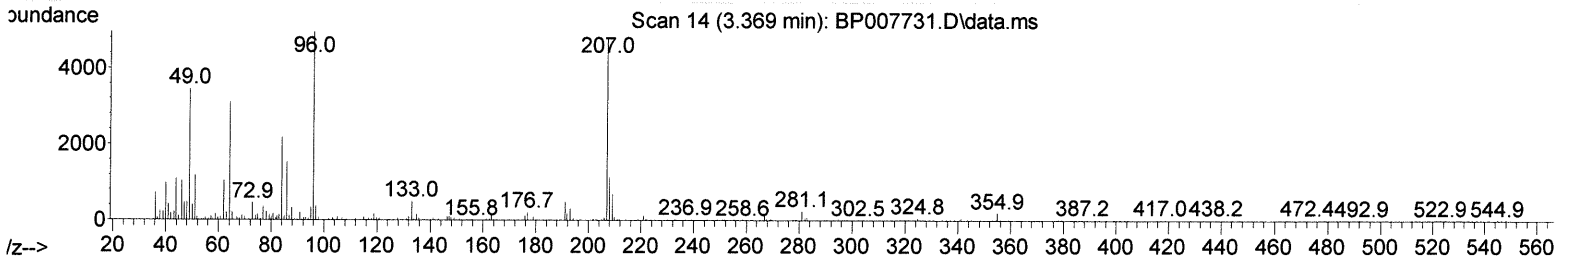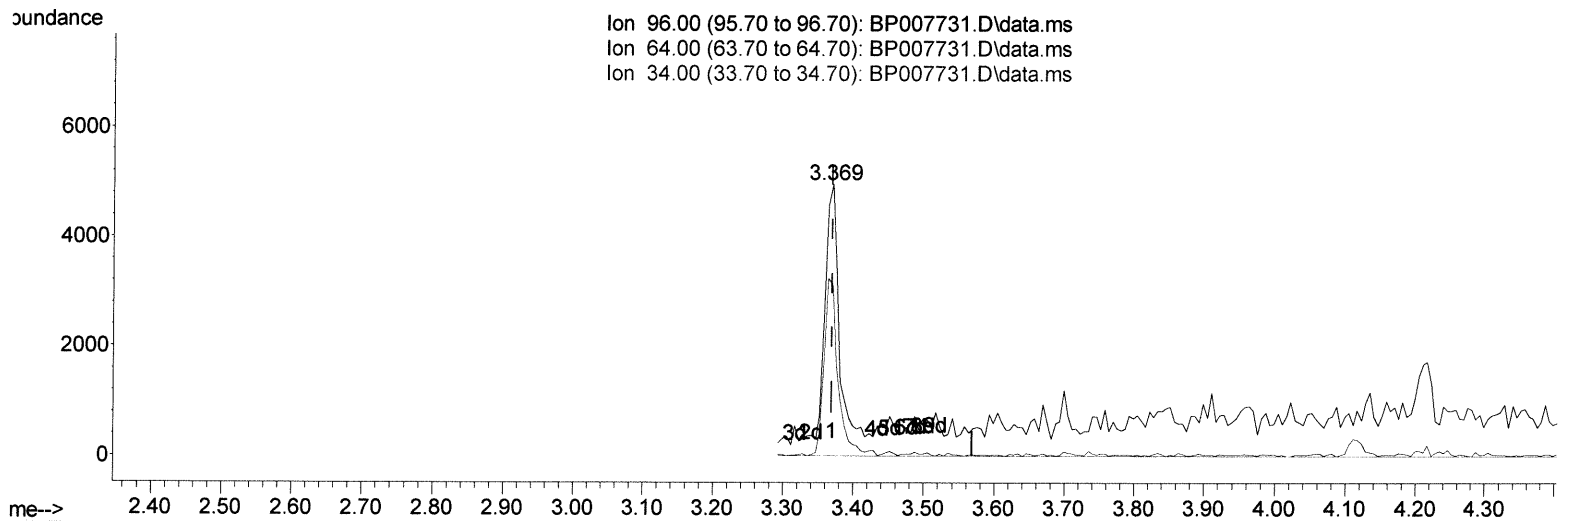

TIC: BP007731.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 1.35 ng/uL

response 6323

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	62.80
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007731.D
Acq On : 27 Oct 2021 21:45
Operator : CG/JU
Sample : M4215-17
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF4

Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:15 AM

Quant Time: Oct 28 01:36:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration

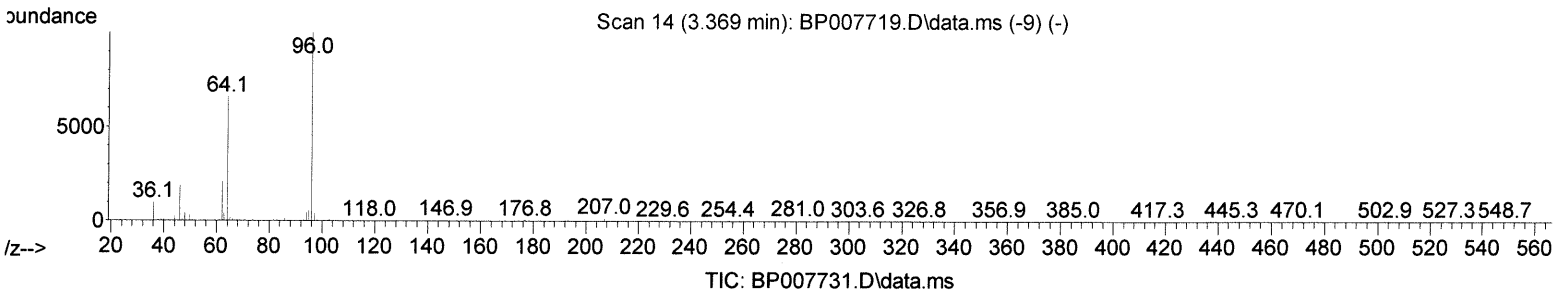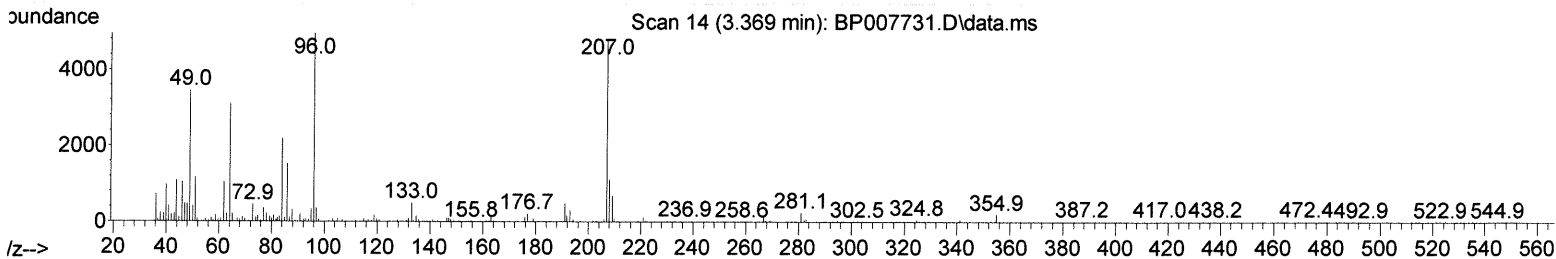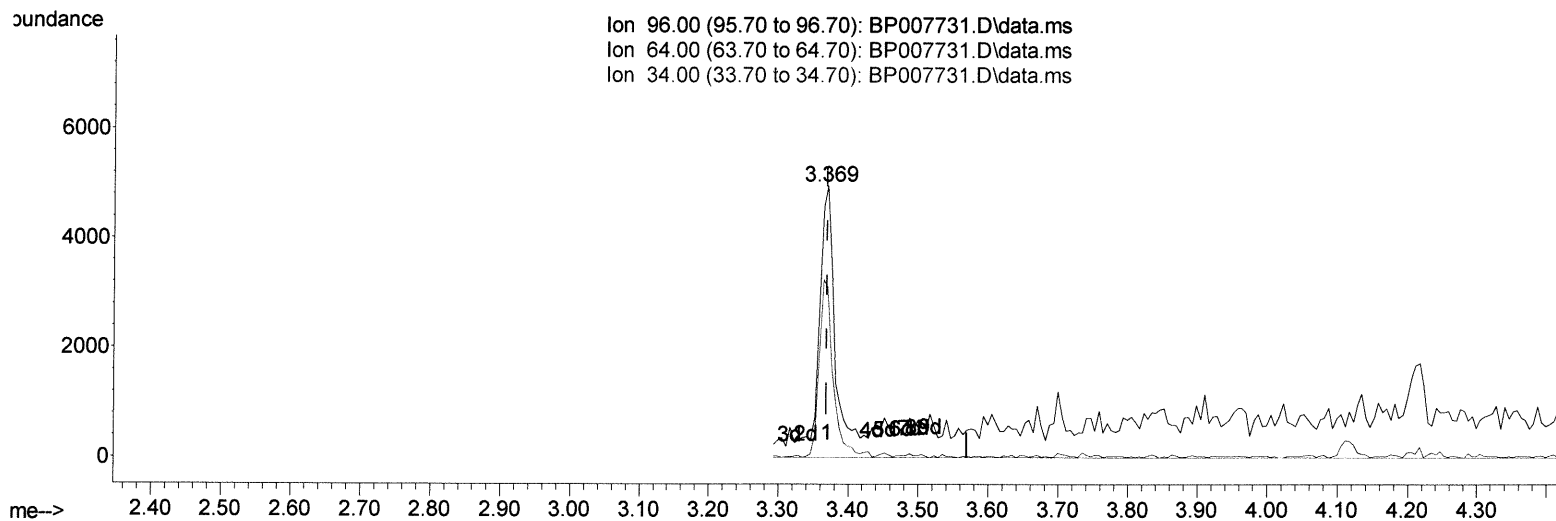

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 1.37 ng/uL m 10/29/21ju

response 6431

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	62.80
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007731.D
 Acq On : 27 Oct 2021 21:45
 Operator : CG/JU
 Sample : M4215-17
 Visc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF4

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:12:15 AM

Quant Time: Oct 28 01:36:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	212731	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	869554	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	566260	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1237819	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	1351666	20.000	ng/ul	-0.01
88) Perylene-d12	23.857	264	1447449	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	6431m >	1.373	ng/uL >	0.00 10/29/21JU
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.093	99	247435	15.313	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	153585	17.120	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	199341	15.862	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	190645	15.068	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	89537	15.110	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	88149	13.620	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.351	165	183052	13.895	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	255616	14.675	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	608445	15.863	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	710480	15.113	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	63751	9.067	ng/ul	0.00
60) Fluorene-d10	15.563	176	540188	16.705	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	47316	7.146	ng/ul	0.00
73) Anthracene-d10	17.422	188	854966	16.807	ng/ul	0.00
81) Pyrene-d10	19.657	212	1084211	17.229	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1110410	15.616	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.327	149	51690	1.145	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed