


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007733.D
Acq On : 27 Oct 2021 22:53
Operator : CG/JU
Sample : M4215-20
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JDGF7

Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:21 AM

Quant Time: Oct 28 02:02:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 27 15:37:43 2021
Response via : Initial Calibration



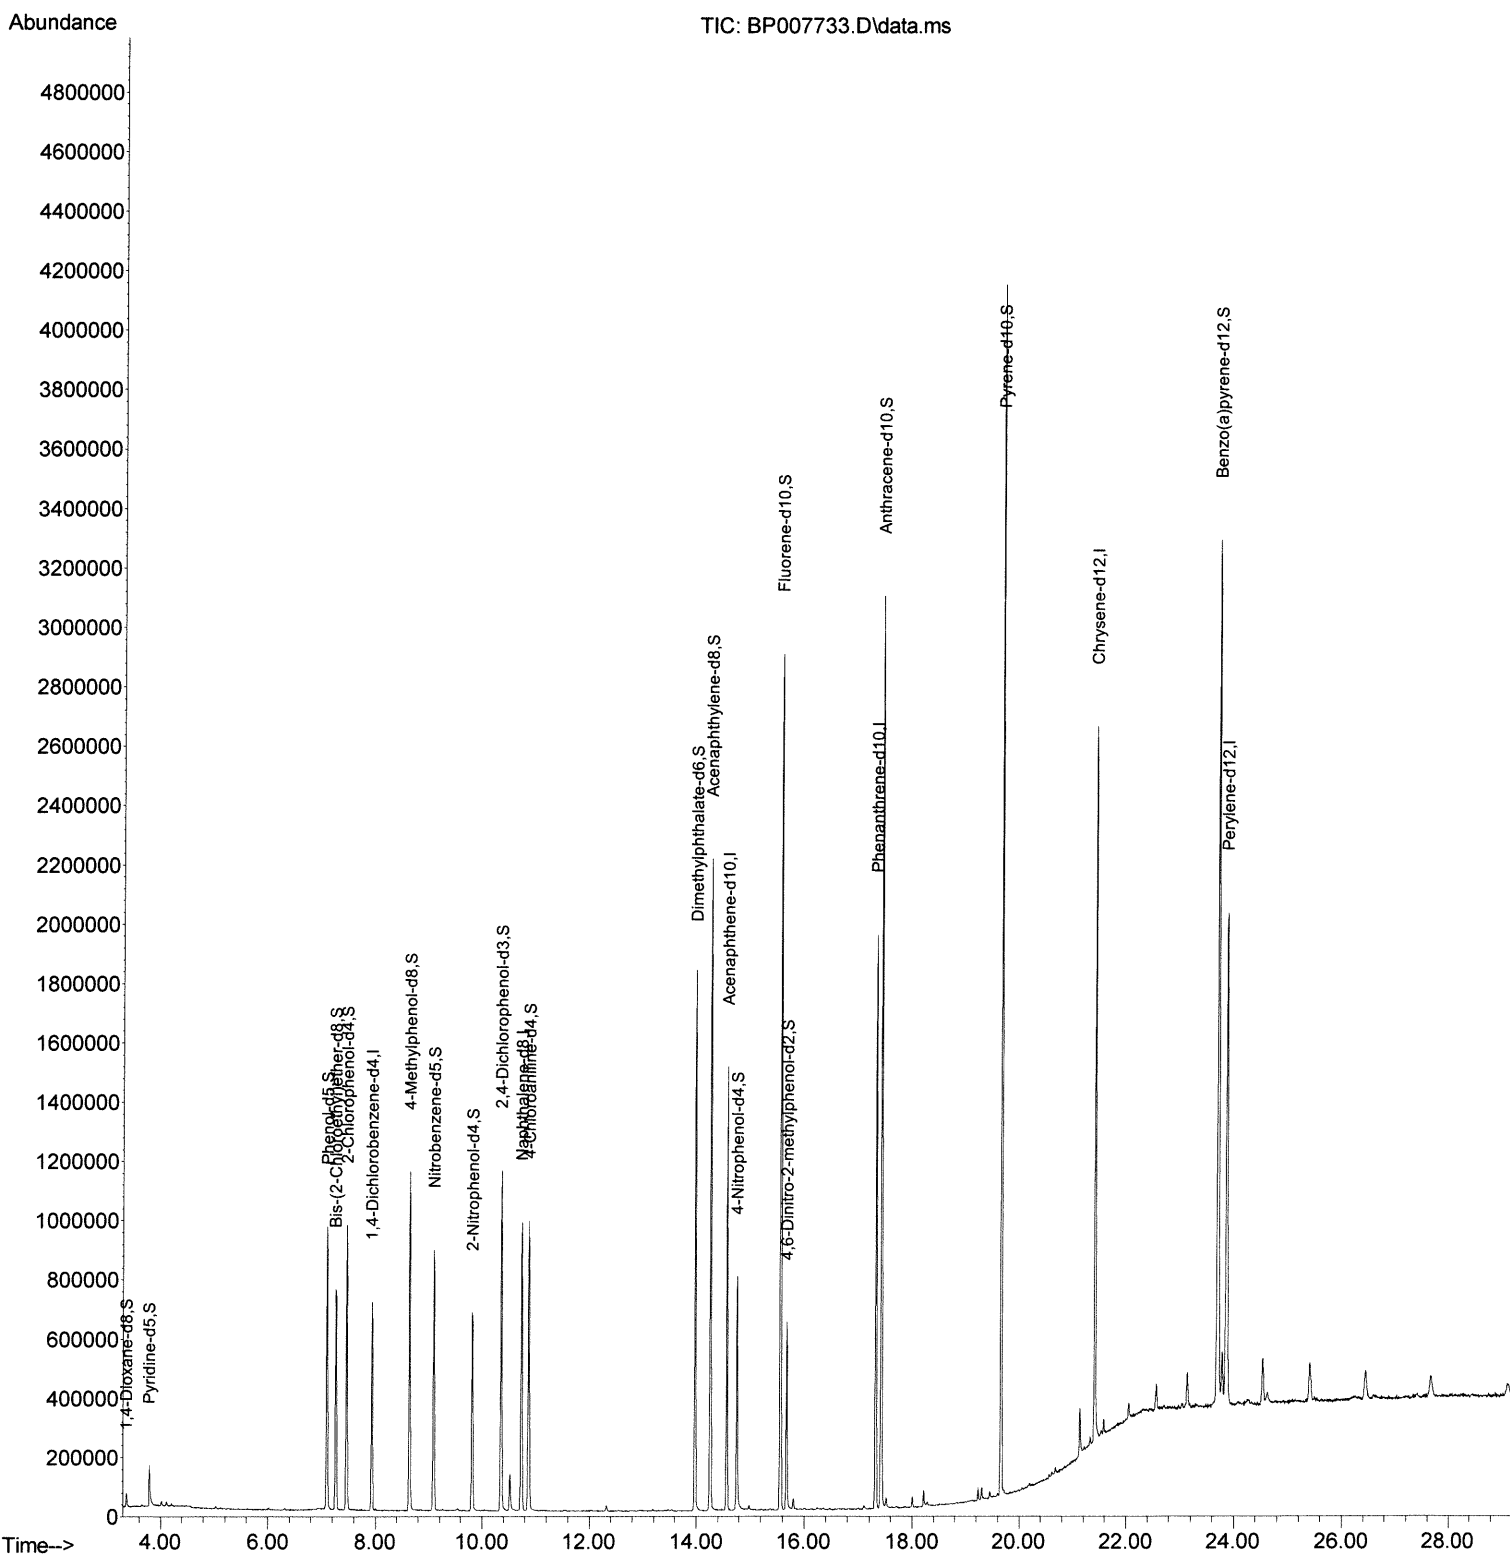


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007733.D
 Acq On : 27 Oct 2021 22:53
 Operator : CG/JU
 Sample : M4215-20
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF7

Manual Integrations
 APPROVED
 mohammad
 10/28/2021 11:12:21 AM

Quant Time: Oct 28 02:02:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

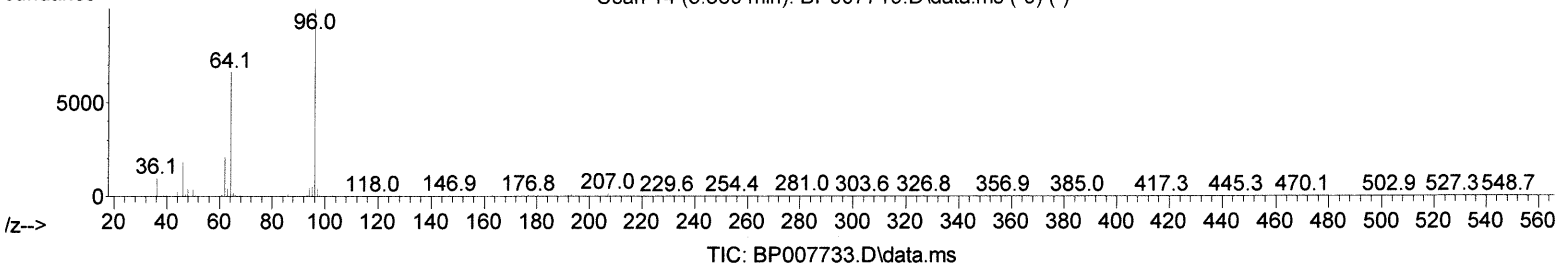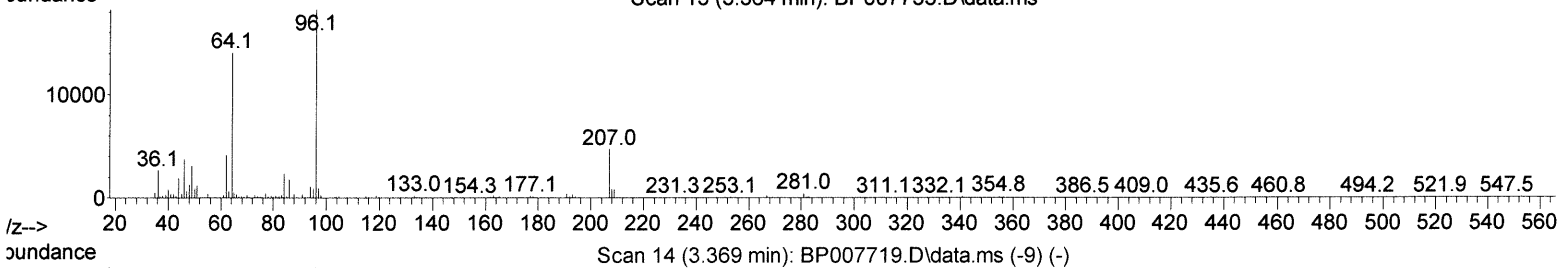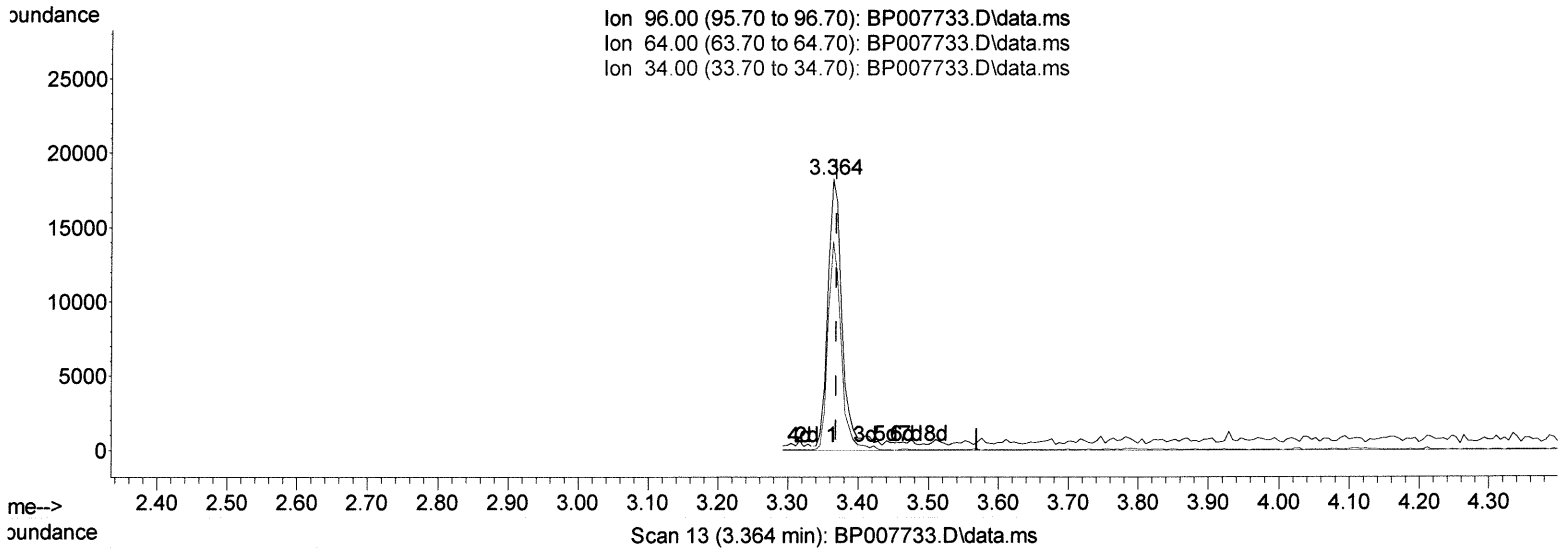

(3) 1,4-Dioxane-d8 (S)

3.364min (-0.005) 5.59 ng/uL

response 24198




Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	77.06
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007733.D
 Acq On : 27 Oct 2021 22:53
 Operator : CG/JU
 Sample : M4215-20
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF7

Manual Integrations
 APPROVED
 mohammad
 10/28/2021 11:12:21 AM

Quant Time: Oct 28 02:02:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

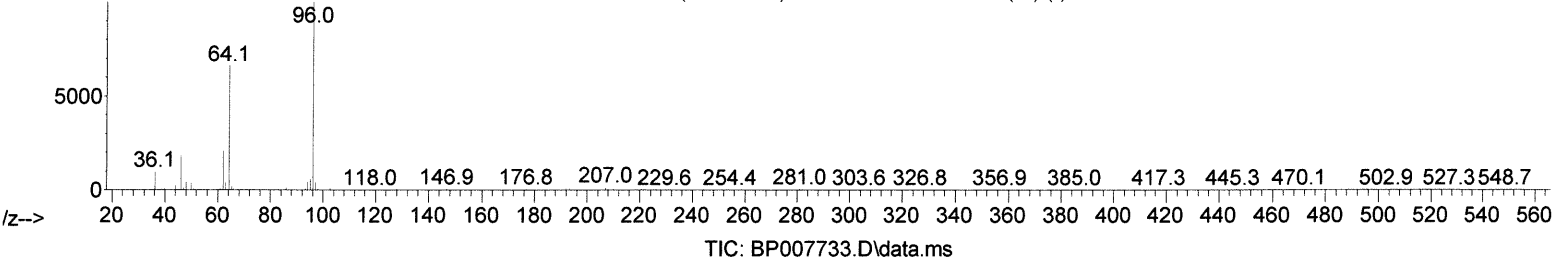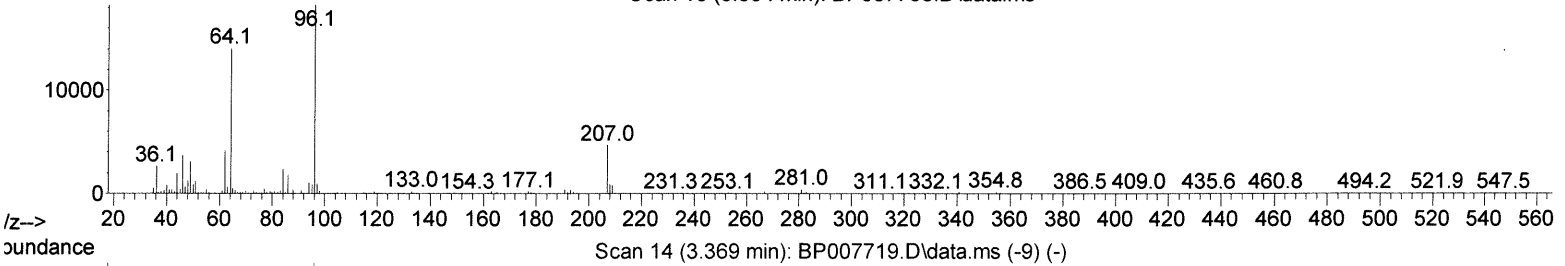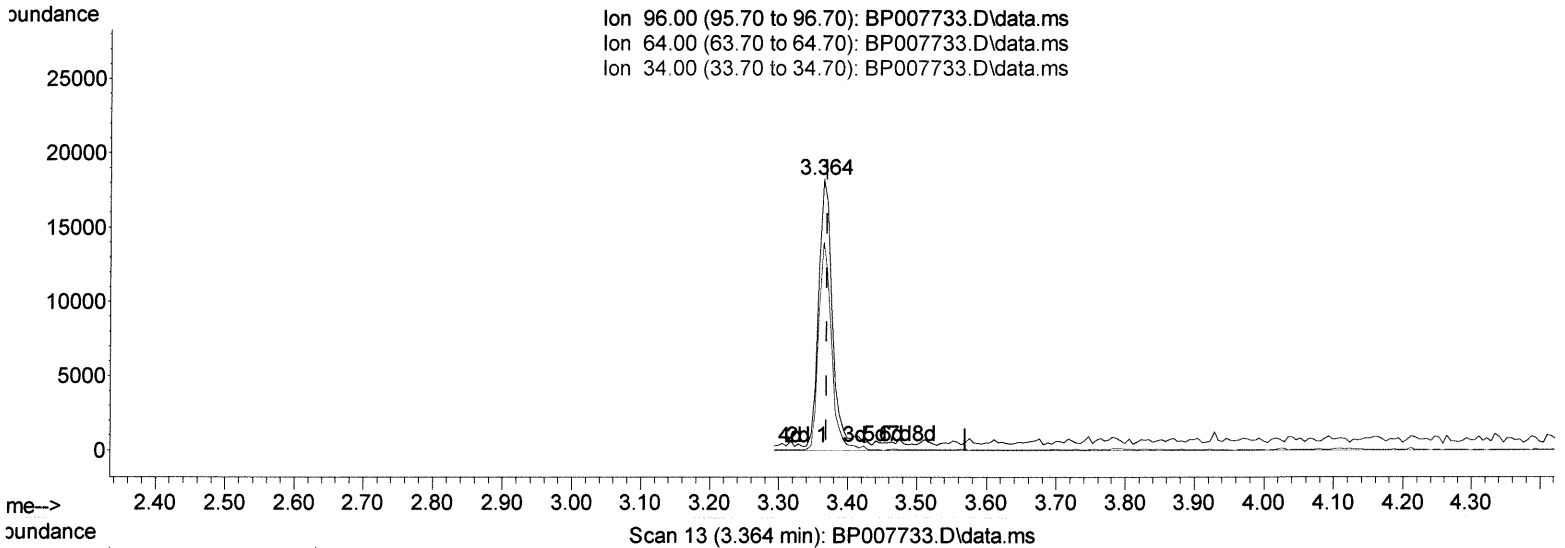

(3) 1,4-Dioxane-d8 (S)

3.364min (-0.005) 5.85 ng/uL m 10/27/21 JU

response	25300	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.20	77.06
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007733.D
 Acq On : 27 Oct 2021 22:53
 Operator : CG/JU
 Sample : M4215-20
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JDGF7

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:12:21 AM

Quant Time: Oct 28 02:02:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	196614	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	803474	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	520503	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1119608	20.000	ng/ul	0.00
79) Chrysene-d12	21.410	240	1210366	20.000	ng/ul	-0.01
88) Perylene-d12	23.857	264	1286901	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	25300m	5.845	ng/uL	> 0.00
4) Pyridine-d5	3.787	84	80734	6.168	ng/ul	0.00
7) Phenol-d5	7.093	99	547580	36.667	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	324859	39.181	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	447816	38.555	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	434418	37.150	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	210518	38.448	ng/ul	0.00
24) 2-Nitrophenol-d4	9.811	143	216386	36.183	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	421445	34.622	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	534507	33.209	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1286531	36.490	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1571599	36.368	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	186996	28.934	ng/ul	0.00
60) Fluorene-d10	15.563	176	1133940	38.150	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	136267	22.754	ng/ul	0.00
73) Anthracene-d10	17.422	188	1778537	38.654	ng/ul	0.00
81) Pyrene-d10	19.657	212	2136109	37.907	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	2229919	35.273	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed