

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007676.D
 Acq On : 26 Oct 2021 11:47
 Operator : CG/JU
 Sample : M4291-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P045-TW001-01

Quant Time: Oct 26 12:24:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 25 16:57:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	226289	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	891686	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	576700	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1227353	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	1317739	20.000	ng/ul	0.00
88) Perylene-d12	23.868	264	1446231	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	25492	5.117	ng/uL	0.00
4) Pyridine-d5	3.787	84	122524	8.133	ng/ul	0.00
7) Phenol-d5	7.099	99	128530	7.478	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	294118	30.821	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	332850	24.899	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	220359	16.373	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	196664	32.364	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	202700	30.542	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.357	165	367449	27.200	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.875	131	445773	24.956	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166	1240409	31.753	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1514537	31.632	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	44613	6.230	ng/ul	-0.01
60) Fluorene-d10	15.569	176	1099277	33.380	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	166454	25.354	ng/ul	0.00
73) Anthracene-d10	17.428	188	1868991	37.054	ng/ul	0.00
81) Pyrene-d10	19.663	212	2320932	37.831	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	2532968	35.653	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.333	149	103194	2.345	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007676.D
Acq On : 26 Oct 2021 11:47
Operator : CG/JU
Sample : M4291-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P045-TW001-01

Quant Time: Oct 26 12:24:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 25 16:57:16 2021
Response via : Initial Calibration

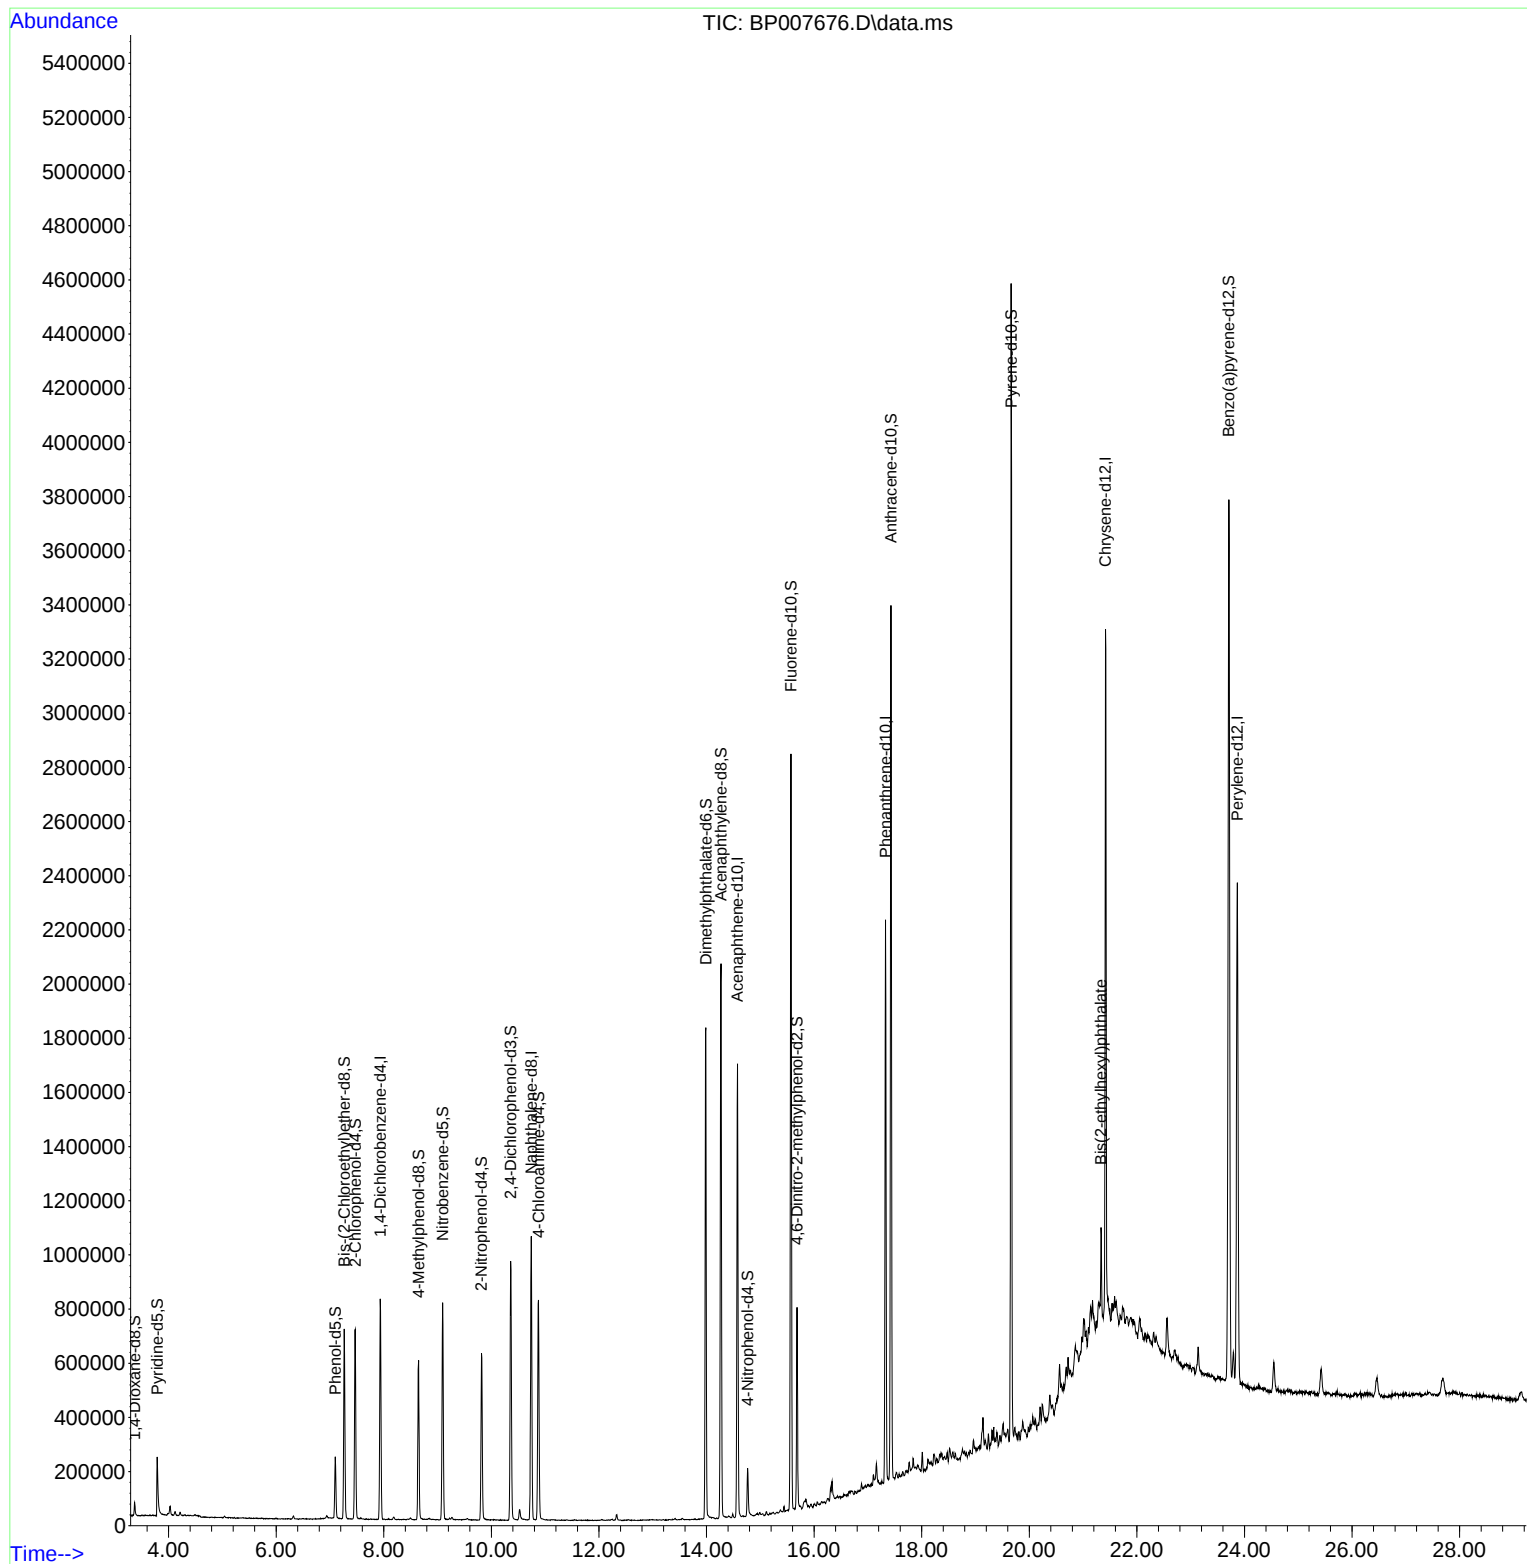

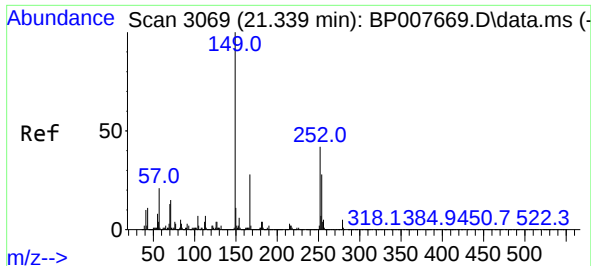

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.345 ng/ul
RT: 21.333 min Scan# 3068
Delta R.T. -0.006 min
Lab File: BP007676.D
Acq: 26 Oct 2021 11:47

Instrument :
BNA_P
ClientSampleId :
P045-TW001-01

Tgt Ion:149 Resp: 103194
Ion Ratio Lower Upper
149 100
167 28.5 22.6 33.8
279 4.0 3.3 4.9

