

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007723.D
 Acq On : 27 Oct 2021 17:13
 Operator : CG/JU
 Sample : PB140206BS
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS206

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:12:13 AM

Quant Time: Oct 27 17:38:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	221692	20.000	ng/u1	0.00
20) Naphthalene-d8	10.740	136	888527	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.569	164	563570	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1205203	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	1235303	20.000	ng/u1	0.00
88) Perylene-d12	23.863	264	1328251	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	32331	6.625	ng/uL	0.00
4) Pyridine-d5	3.781	84	486747	32.981	ng/u1	0.00
7) Phenol-d5	7.099	99	584061	34.686	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	333593	35.683	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	468613	35.782	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	462196	35.054	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	220348	36.391	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	238061	35.997	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	471195	35.004	ng/u1	0.00
31) 4-Chloroaniline-d4	10.869	131	573534	32.223	ng/u1	0.00
46) Dimethylphthalate-d6	13.981	166	1334626	34.961	ng/u1	0.00
49) Acenaphthylene-d8	14.263	160	1628588	34.807	ng/u1	0.00
54) 4-Nitrophenol-d4	14.763	143	248145	35.461	ng/u1	0.00
60) Fluorene-d10	15.563	176	1126724	35.010	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	208329	32.316	ng/u1	0.00
73) Anthracene-d10	17.428	188	1738213	35.095	ng/u1	0.00
81) Pyrene-d10	19.663	212	2156605	37.498	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.704	264	2227516	34.138	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	73224	13.421	ng/uL	89
5) Pyridine	3.799	79	508675	35.187	ng/u1	97
6) Benzaldehyde	7.069	77	377298	46.608	ng/u1	97
8) Phenol	7.122	94	636288	37.400	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.358	93	499549	37.245	ng/u1	99
12) 2-Chlorophenol	7.499	128	513493	38.676	ng/u1	98
13) 2-Methylphenol	8.375	108	474682	36.936	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.469	45	581210	38.152	ng/u1	97
16) Acetophenone	8.758	105	723760	36.779	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.746	70	353462	37.765	ng/u1	94
18) 4-Methylphenol	8.710	108	513205	37.447	ng/u1	96
19) Hexachloroethane	9.016	117	208051	38.289	ng/u1	94
22) Nitrobenzene	9.134	77	540951	37.862	ng/u1	96
23) Isophorone	9.663	82	1016511	37.192	ng/u1	98
25) 2-Nitrophenol	9.846	139	274730	38.596	ng/u1	96
26) 2,4-Dimethylphenol	9.910	107	544949	35.959	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.146	93	646977	36.925	ng/u1	99
29) 2,4-Dichlorophenol	10.381	162	487690	36.979	ng/u1	98
30) Naphthalene	10.787	128	1515276	36.123	ng/u1	99
32) 4-Chloroaniline	10.893	127	618024	34.113	ng/u1	98
33) Hexachlorobutadiene	11.081	225	346457	36.033	ng/u1	99
34) Caprolactam	11.669	113	154531m	35.736	ng/u1	
35) 4-Chloro-3-methylphenol	12.022	107	520722	38.139	ng/u1	98
36) 2-Methylnaphthalene	12.398	142	1050266	36.418	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007723.D
 Acq On : 27 Oct 2021 17:13
 Operator : CG/JU
 Sample : PB140206BS
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS206


Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:12:13 AM

Quant Time: Oct 27 17:38:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 27 15:37:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.616	142	1053542	36.181	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.769	216	619337	36.230	ng/ul#	96
40) Hexachlorocyclopentadiene	12.751	237	347443	31.341	ng/ul	100
41) 2,4,6-Trichlorophenol	13.004	196	398368	37.037	ng/ul	96
42) 2,4,5-Trichlorophenol	13.075	196	439076	37.913	ng/ul	97
43) 1,1'-Biphenyl	13.404	154	1407706	36.157	ng/ul	99
44) 2-Chloronaphthalene	13.445	162	1099072	36.428	ng/ul	98
45) 2-Nitroaniline	13.645	65	307222	40.362	ng/ul	95
47) Dimethylphthalate	14.028	163	1398898	37.074	ng/ul	99
48) 2,6-Dinitrotoluene	14.145	165	290726	40.340	ng/ul	91
50) Acenaphthylene	14.293	152	1734724	36.620	ng/ul	99
51) 3-Nitroaniline	14.469	138	295761	38.693	ng/ul#	96
52) Acenaphthene	14.634	153	1139517	36.474	ng/ul	99
53) 2,4-Dinitrophenol	14.675	184	147916	32.883	ng/ul	98
55) 4-Nitrophenol	14.781	109	225116	36.389	ng/ul	93
56) Dibenzofuran	14.969	168	1654560	36.228	ng/ul	99
57) 2,4-Dinitrotoluene	14.934	165	413460	39.946	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.198	232	360931	38.234	ng/ul	97
59) Diethylphthalate	15.398	149	1369866	37.017	ng/ul	98
61) Fluorene	15.622	166	1282168	36.016	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.616	204	669983	35.488	ng/ul	99
63) 4-Nitroaniline	15.634	138	290442	40.929	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.698	198	228996	35.290	ng/ul	99
67) N-Nitrosodiphenylamine	15.828	169	1155288	37.155	ng/ul	99
68) 4-Bromophenyl-phenylether	16.516	248	429592	36.556	ng/ul	95
69) Hexachlorobenzene	16.634	284	493144	36.238	ng/ul	95
70) Atrazine	16.786	200	455230	35.310	ng/ul	98
71) Pentachlorophenol	16.975	266	302101	35.746	ng/ul	99
72) Phenanthrene	17.369	178	2172668	37.298	ng/ul	100
74) Anthracene	17.463	178	2139483	36.925	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.369	216	615292	34.919	ng/ul	99
76) Pentachlorobenzene	14.892	250	591530	34.814	ng/ul	100
77) Carbazole	17.728	167	1989989	37.203	ng/ul	99
78) Di-n-butylphthalate	18.286	149	2334476	38.120	ng/ul	99
80) Fluoranthene	19.333	202	2716349	38.538	ng/ul	99
82) Pyrene	19.686	202	2716414	38.078	ng/ul	99
83) Butylbenzylphthalate	20.563	149	1095007	39.450	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.333	252	918992	40.141	ng/ul#	98
85) Benzo(a)anthracene	21.404	228	2763540	37.673	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.333	149	1581188	38.337	ng/ul	98
87) Chrysene	21.457	228	2664845	37.572	ng/ul	99
89) Di-n-octyl phthalate	22.274	149	2814764	38.043	ng/ul	100
90) Benzo(b)fluoranthene	23.116	252	2951983	37.718	ng/ul	99
91) Benzo(k)fluoranthene	23.169	252	2849837	38.911	ng/ul	99
93) Benzo(a)pyrene	23.757	252	2903136	38.285	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.421	276	3408474	37.736	ng/ul	100
95) Dibenzo(a,h)anthracene	26.433	278	2912784	37.631	ng/ul	99
96) Benzo(g,h,i)perylene	27.204	276	2937537	38.236	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

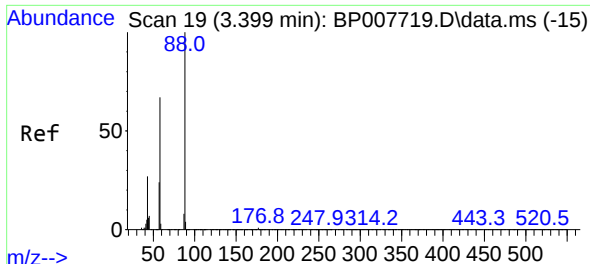





#2
1,4-Dioxane
Concen: 13.421 ng/uL
RT: 3.405 min Scan# 20
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion: 88 Resp: 73224
Ion Ratio Lower Upper
88 100
43 27.1 24.2 36.2
58 67.3 62.5 93.7

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

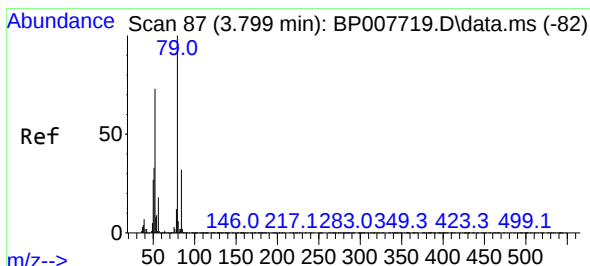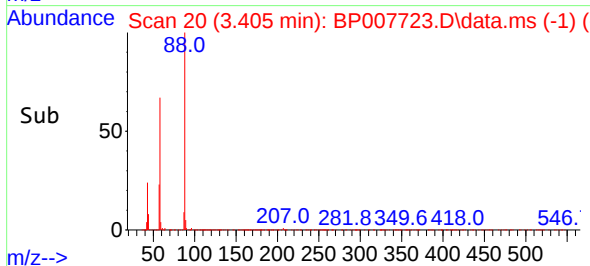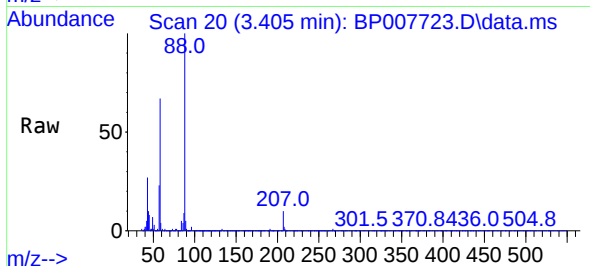

#5
Pyridine
Concen: 35.187 ng/uL
RT: 3.799 min Scan# 87
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion: 79 Resp: 508675
Ion Ratio Lower Upper
79 100
52 75.4 57.0 85.4
51 33.7 27.0 40.6

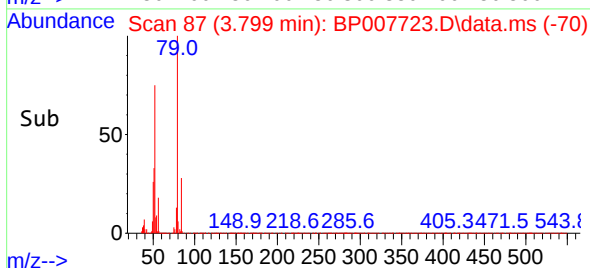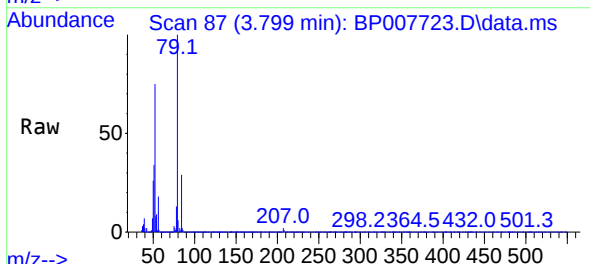



#6
Benzaldehyde
Concen: 46.608 ng/ul
RT: 7.069 min Scan# 643
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion: 77 Resp: 377298
Ion Ratio Lower Upper
77 100
105 100.6 78.2 117.4
106 97.2 74.6 112.0

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

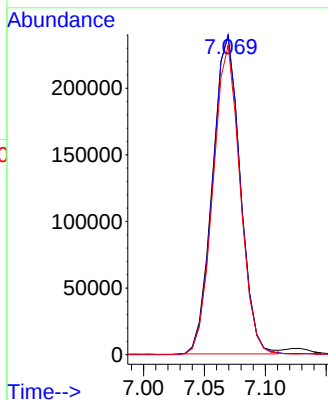


#8
Phenol
Concen: 37.400 ng/ul
RT: 7.122 min Scan# 652
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion: 94 Resp: 636288
Ion Ratio Lower Upper
94 100
65 27.0 21.9 32.9
66 39.3 29.9 44.9

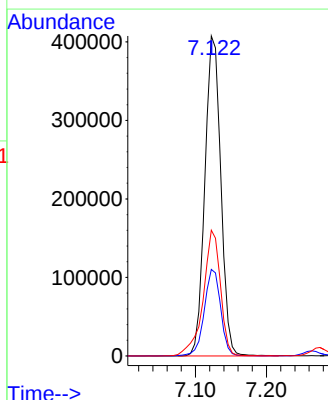



#10
Bis(2-Chloroethyl)ether
Concen: 37.245 ng/ul
RT: 7.358 min Scan# 692
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion: 93 Resp: 499549
Ion Ratio Lower Upper
93 100
63 72.6 59.0 88.4
95 32.8 26.4 39.6

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

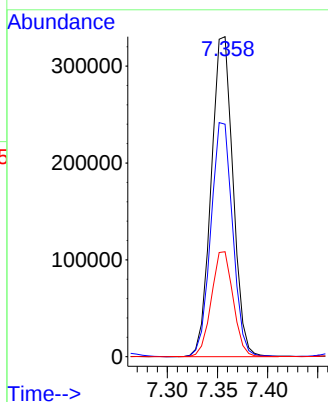


#12
2-Chlorophenol
Concen: 38.676 ng/ul
RT: 7.499 min Scan# 716
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13



Tgt Ion: 128 Resp: 513493
Ion Ratio Lower Upper
128 100
64 43.6 36.9 55.3
130 31.7 25.2 37.8

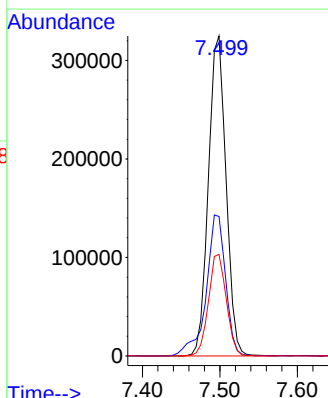







#13
2-Methylphenol
Concen: 36.936 ng/ul
RT: 8.375 min Scan# 865
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Instrument :
BNA_P
ClientSampleId :
SLCS206

Tgt Ion:108 Resp: 474682
Ion Ratio Lower Upper
108 100
107 89.5 72.2 108.2




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

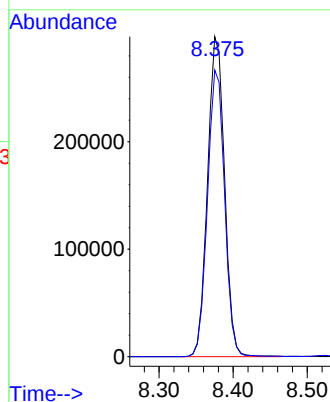

#14
2,2'-oxybis(1-Chloropropane)
Concen: 38.152 ng/ul
RT: 8.469 min Scan# 881
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion: 45 Resp: 581210
Ion Ratio Lower Upper
45 100
77 16.9 12.3 18.5
79 12.6 9.4 14.0





#16
Acetophenone
Concen: 36.779 ng/ul
RT: 8.758 min Scan# 930
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion: 105 Resp: 723760
Ion Ratio Lower Upper
105 100
77 76.7 61.8 92.6
51 25.0 20.8 31.2

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

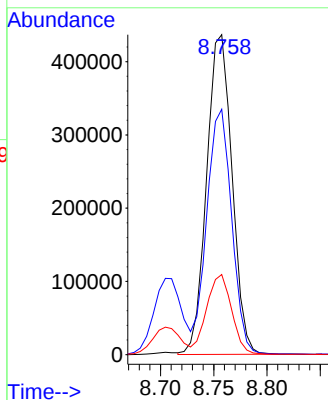


#17
N-Nitroso-di-n-propylamine
Concen: 37.765 ng/ul
RT: 8.746 min Scan# 928
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion: 70 Resp: 353462
Ion Ratio Lower Upper
70 100
42 53.2 46.3 69.5
101 10.0 7.4 11.0
130 22.4 16.2 24.2

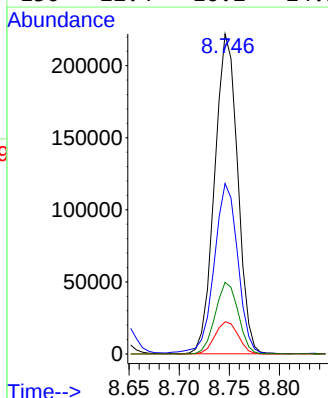



#18
4-Methylphenol
Concen: 37.447 ng/ul
RT: 8.710 min Scan# 922
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:108 Resp: 513205
Ion Ratio Lower Upper
108 100
107 109.8 90.9 136.3




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

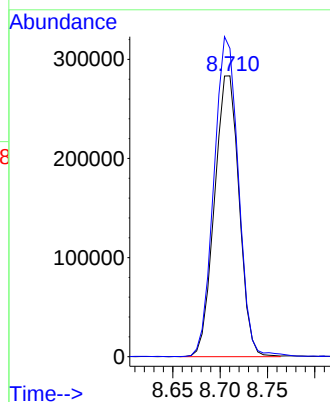

#19
Hexachloroethane
Concen: 38.289 ng/ul
RT: 9.016 min Scan# 974
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:117 Resp: 208051
Ion Ratio Lower Upper
117 100
201 109.7 82.3 123.5
199 68.3 51.8 77.6





#22
Nitrobenzene
Concen: 37.862 ng/ul
RT: 9.134 min Scan# 994
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion: 77 Resp: 540951
Ion Ratio Lower Upper
77 100
123 46.8 34.9 52.3
65 13.8 10.5 15.7

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#23
Isophorone
Concen: 37.192 ng/ul
RT: 9.663 min Scan# 1084
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion: 82 Resp: 1016511
Ion Ratio Lower Upper
82 100
95 7.7 5.6 8.4
138 17.4 13.4 20.0

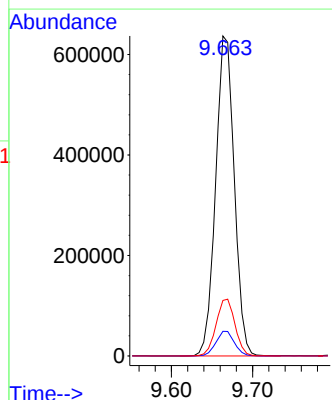

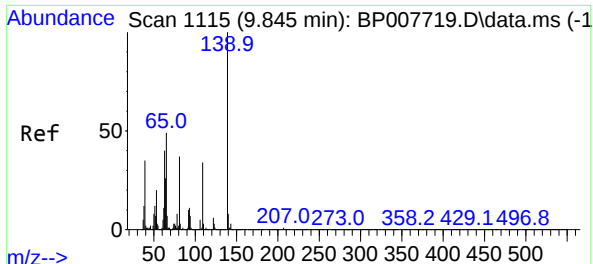

#25
2-Nitrophenol
Concen: 38.596 ng/ul
RT: 9.846 min Scan# 1115
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206

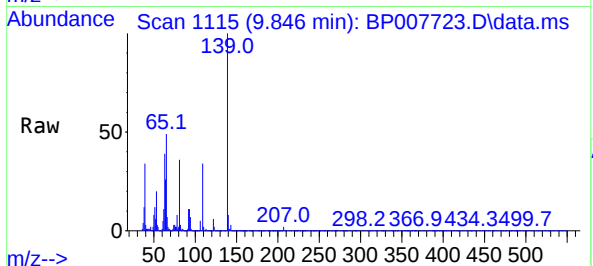

Tgt Ion:139 Resp: 274730
Ion Ratio Lower Upper
139 100
65 49.1 40.3 60.5
109 33.8 23.7 35.5




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

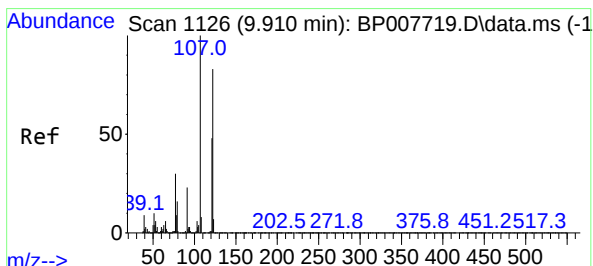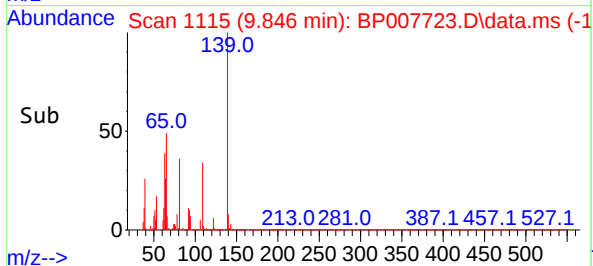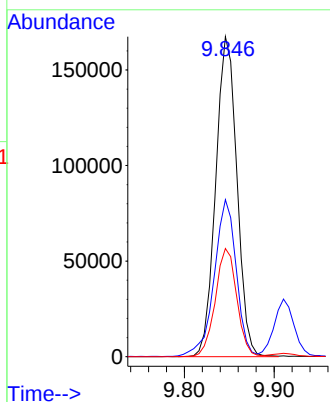

#26
2,4-Dimethylphenol
Concen: 35.959 ng/ul
RT: 9.910 min Scan# 1126
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:107 Resp: 544949
Ion Ratio Lower Upper
107 100
121 49.9 38.8 58.2
122 84.0 64.0 96.0

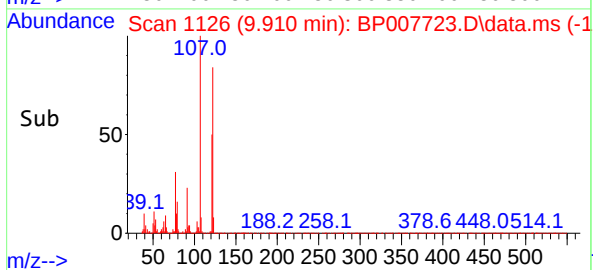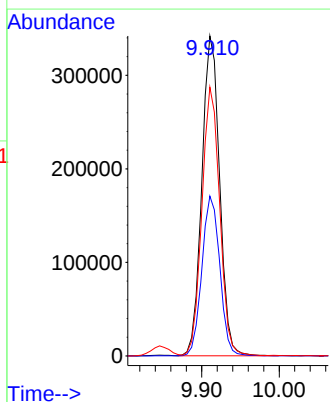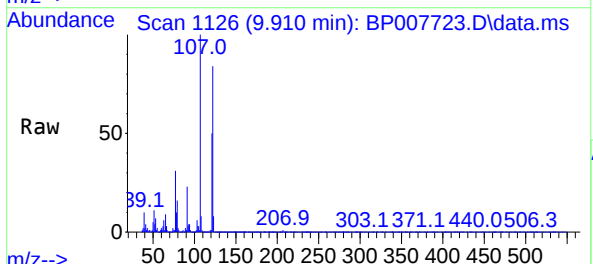



#27
Bis(2-Chloroethoxy)methane
Concen: 36.925 ng/ul
RT: 10.146 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion: 93 Resp: 646977
Ion Ratio Lower Upper
93 100
95 32.7 26.2 39.4
123 11.1 8.3 12.5

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#29
2,4-Dichlorophenol
Concen: 36.979 ng/ul
RT: 10.381 min Scan# 1206
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion: 162 Resp: 487690
Ion Ratio Lower Upper
162 100
164 66.5 52.9 79.3
98 35.7 30.6 45.8





#30
Naphthalene
Concen: 36.123 ng/ul
RT: 10.787 min Scan# 1275
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:128 Resp: 1515276
Ion Ratio Lower Upper
128 100
129 11.2 8.8 13.2
127 13.6 10.5 15.7

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

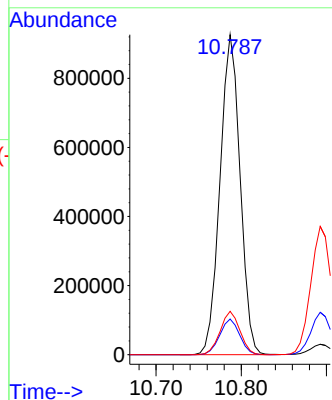


#32
4-Chloroaniline
Concen: 34.113 ng/ul
RT: 10.893 min Scan# 1293
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:127 Resp: 618024
Ion Ratio Lower Upper
127 100
129 33.1 25.8 38.6

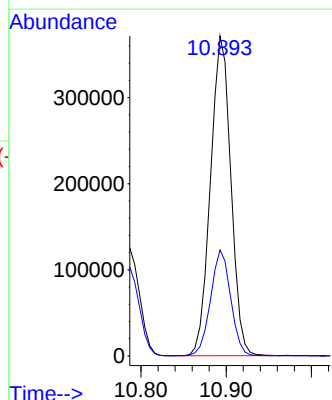



#33
Hexachlorobutadiene
Concen: 36.033 ng/ul
RT: 11.081 min Scan# 1325
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:225 Resp: 346457
Ion Ratio Lower Upper
225 100
223 61.7 50.6 76.0
227 64.4 51.0 76.6

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

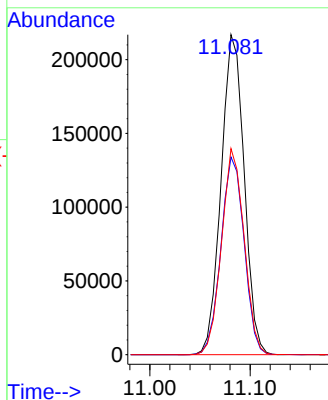


#34
Caprolactam
Concen: 35.736 ng/ul m
RT: 11.669 min Scan# 1425
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13



Tgt Ion:113 Resp: 154531
Ion Ratio Lower Upper
113 100
55 147.8 130.1 195.1
56 111.9 96.2 144.4

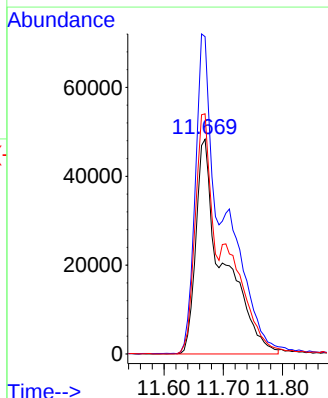







#35
4-Chloro-3-methylphenol
Concen: 38.139 ng/ul
RT: 12.022 min Scan# 1485
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:107 Resp: 520722
Ion Ratio Lower Upper
107 100
144 24.8 19.3 28.9
142 79.8 62.2 93.4

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#36
2-Methylnaphthalene
Concen: 36.418 ng/ul
RT: 12.398 min Scan# 1549
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:142 Resp: 1050266
Ion Ratio Lower Upper
142 100
141 88.8 71.8 107.6









#37
1-Methylnaphthalene
Concen: 36.181 ng/ul
RT: 12.616 min Scan# 1586
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:142 Resp: 1053542
Ion Ratio Lower Upper
142 100
141 91.9 73.5 110.3
116 4.0 3.1 4.7

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#39
1,2,4,5-Tetrachlorobenzene
Concen: 36.230 ng/ul
RT: 12.769 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:216 Resp: 619337
Ion Ratio Lower Upper
216 100
214 76.5 63.1 94.7
179 20.3 17.4 26.0
108 15.0 15.0 22.6#



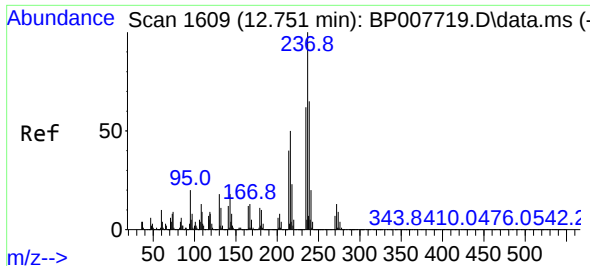





#40
Hexachlorocyclopentadiene
Concen: 31.341 ng/ul
RT: 12.751 min Scan# 1609
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:	237	Resp:	347443
Ion Ratio	Lower	Upper	
237	100		
235	61.9	49.4	74.2
272	12.0	9.8	14.6

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

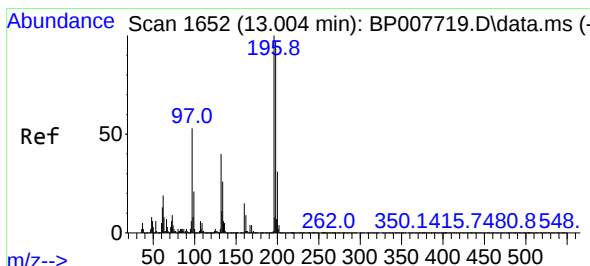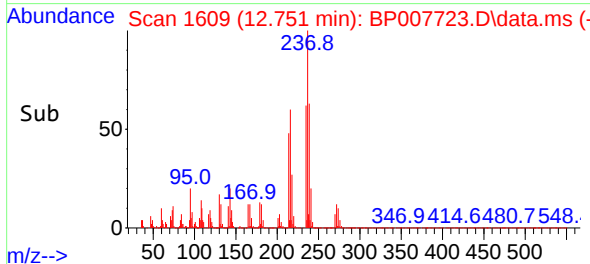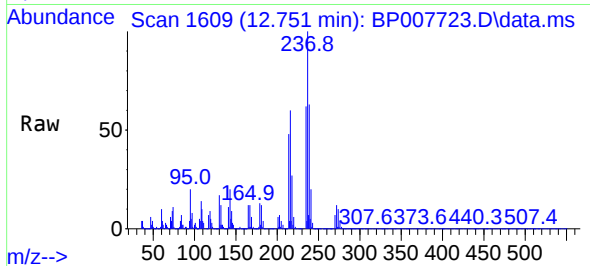

#41
2,4,6-Trichlorophenol
Concen: 37.037 ng/ul
RT: 13.004 min Scan# 1652
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:	196	Resp:	398368
Ion Ratio	Lower	Upper	
196	100		
198	98.0	75.8	113.6
200	31.2	23.0	34.4

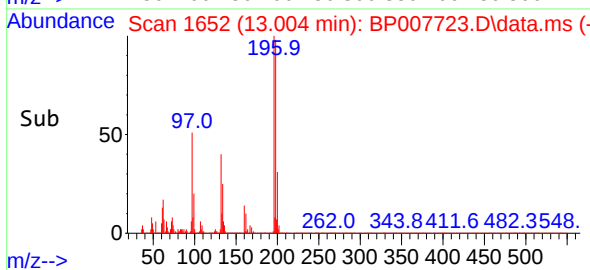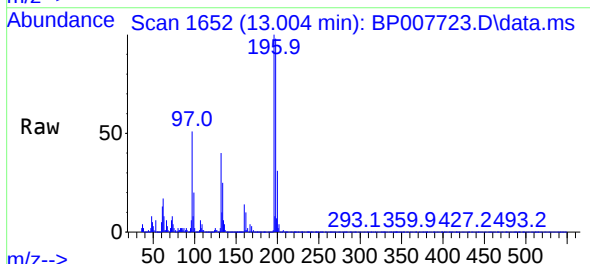



#42
2,4,5-Trichlorophenol
Concen: 37.913 ng/ul
RT: 13.075 min Scan# 1664
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:196 Resp: 439076
Ion Ratio Lower Upper
196 100
198 97.7 75.1 112.7
200 31.5 25.8 38.8

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

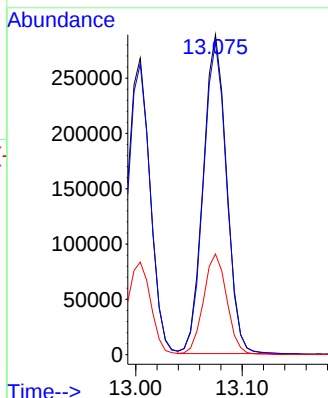


#43
1,1'-Biphenyl
Concen: 36.157 ng/ul
RT: 13.404 min Scan# 1720
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:154 Resp: 1407706
Ion Ratio Lower Upper
154 100
153 40.3 32.0 48.0
76 11.8 10.3 15.5

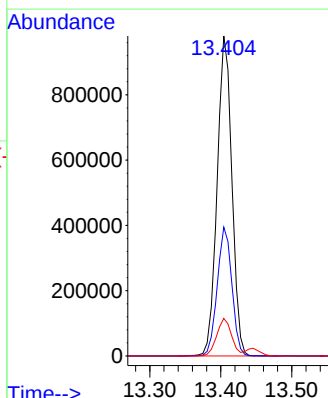



#44
2-Chloronaphthalene
Concen: 36.428 ng/ul
RT: 13.445 min Scan# 1727
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:162 Resp: 1099072
Ion Ratio Lower Upper
162 100
164 32.7 26.5 39.7
127 37.7 31.8 47.6

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

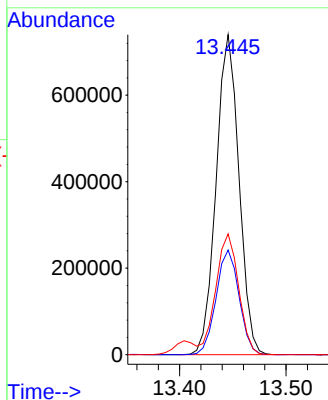


#45
2-Nitroaniline
Concen: 40.362 ng/ul
RT: 13.645 min Scan# 1761
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13



Tgt Ion: 65 Resp: 307222
Ion Ratio Lower Upper
65 100
92 72.3 55.9 83.9
138 110.9 83.4 125.2

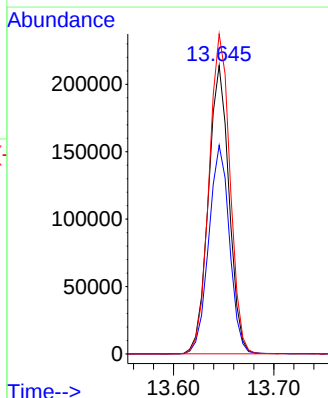




#47
Dimethylphthalate
Concen: 37.074 ng/ul
RT: 14.028 min Scan# 1826
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206

Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:13 AM







Tgt Ion:163 Resp: 1398898
Ion Ratio Lower Upper
163 100
194 4.1 3.2 4.8
164 10.3 7.9 11.9

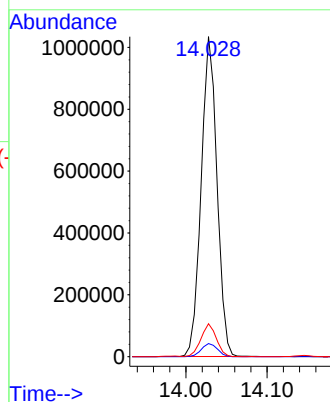

#48
2,6-Dinitrotoluene
Concen: 40.340 ng/ul
RT: 14.145 min Scan# 1846
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:165 Resp: 290726
Ion Ratio Lower Upper
165 100
89 54.2 49.0 73.4
121 19.3 18.4 27.6





#50
Acenaphthylene
Concen: 36.620 ng/ul
RT: 14.293 min Scan# 1871
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:152 Resp: 1734724
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.8
153 13.3 10.6 15.8




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#51
3-Nitroaniline
Concen: 38.693 ng/ul
RT: 14.469 min Scan# 1901
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:138 Resp: 295761
Ion Ratio Lower Upper
138 100
108 11.8 13.0 19.4#
92 115.7 95.7 143.5

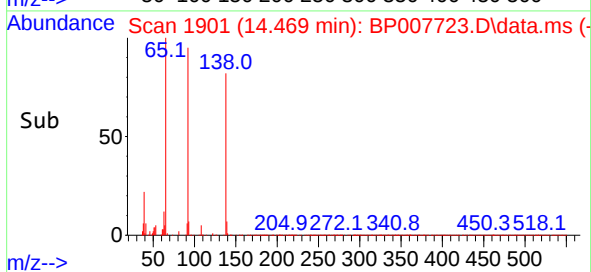







#52
Acenaphthene
Concen: 36.474 ng/ul
RT: 14.634 min Scan# 1929
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:153 Resp: 1139517
Ion Ratio Lower Upper
153 100
152 47.2 37.9 56.9
154 88.9 70.1 105.1

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#53
2,4-Dinitrophenol
Concen: 32.883 ng/ul
RT: 14.675 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:184 Resp: 147916
Ion Ratio Lower Upper
184 100
63 58.8 48.8 73.2
154 68.8 56.2 84.4





#55
4-Nitrophenol
Concen: 36.389 ng/ul
RT: 14.781 min Scan# 1954
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:109 Resp: 225116
Ion Ratio Lower Upper
109 100
139 121.9 100.2 150.2
65 110.6 98.8 148.2




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#56
Dibenzofuran
Concen: 36.228 ng/ul
RT: 14.969 min Scan# 1986
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:168 Resp: 1654560
Ion Ratio Lower Upper
168 100
139 38.3 30.1 45.1

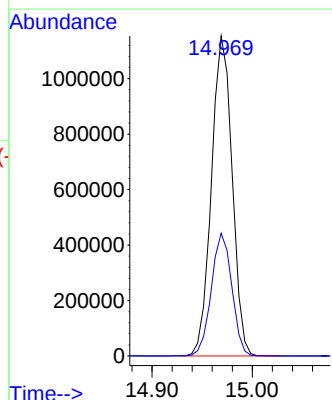



#57
2,4-Dinitrotoluene
Concen: 39.946 ng/ul
RT: 14.934 min Scan# 1980
Delta R.T. 0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:165 Resp: 413460
Ion Ratio Lower Upper
165 100
63 37.2 35.0 52.6
182 2.8 2.3 3.5

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#58
2,3,4,6-Tetrachlorophenol
Concen: 38.234 ng/ul
RT: 15.198 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:232 Resp: 360931
Ion Ratio Lower Upper
232 100
131 42.2 35.1 52.7
130 2.2 2.0 3.0
166 30.0 25.8 38.8

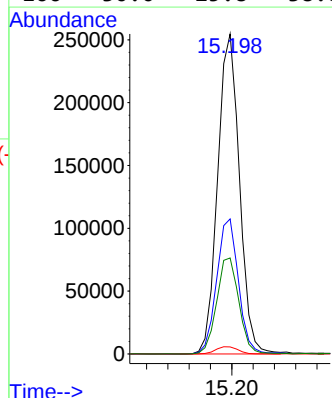



#59
Diethylphthalate
Concen: 37.017 ng/ul
RT: 15.398 min Scan# 2059
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampled :
SLCS206



Tgt Ion:149 Resp: 1369866
Ion Ratio Lower Upper
149 100
177 23.0 17.4 26.2
150 12.5 10.0 15.0




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM

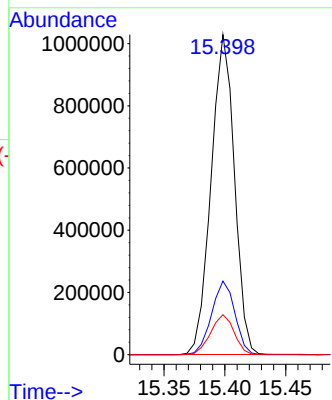

#61
Fluorene
Concen: 36.016 ng/ul
RT: 15.622 min Scan# 2097
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:166 Resp: 1282168
Ion Ratio Lower Upper
166 100
165 98.0 78.4 117.6
167 13.5 10.9 16.3

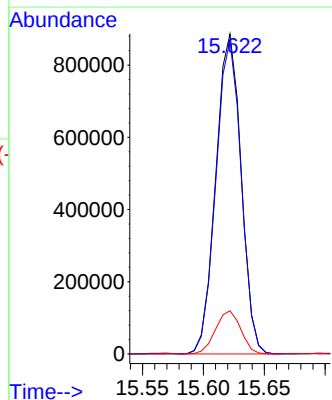







#62
4-Chlorophenyl-phenylether
Concen: 35.488 ng/ul
RT: 15.616 min Scan# 2096
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:204 Resp: 669983
Ion Ratio Lower Upper
204 100
206 33.0 26.5 39.7
141 58.0 47.4 71.0

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#63
4-Nitroaniline
Concen: 40.929 ng/ul
RT: 15.634 min Scan# 2099
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:138 Resp: 290442
Ion Ratio Lower Upper
138 100
92 50.1 42.1 63.1
108 84.9 70.3 105.5









#66
4,6-Dinitro-2-methylphenol
Concen: 35.290 ng/ul
RT: 15.698 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:198 Resp: 228996
Ion Ratio Lower Upper
198 100
182 4.0 3.3 4.9
77 22.3 18.4 27.6

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#67
N-Nitrosodiphenylamine
Concen: 37.155 ng/ul
RT: 15.828 min Scan# 2132
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:169 Resp: 1155288
Ion Ratio Lower Upper
169 100
168 66.6 52.5 78.7
167 36.0 28.4 42.6



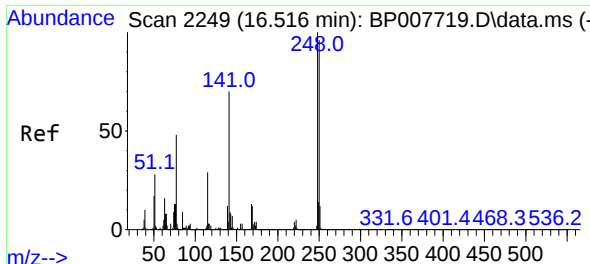

#68
4-Bromophenyl-phenylether
Concen: 36.556 ng/ul
RT: 16.516 min Scan# 2249
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206

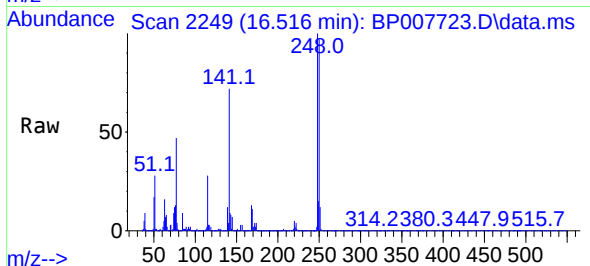


Tgt Ion:248 Resp: 429592
Ion Ratio Lower Upper
248 100
250 96.6 78.9 118.3
141 72.2 64.3 96.5

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM

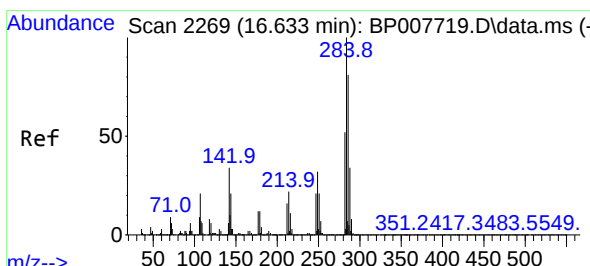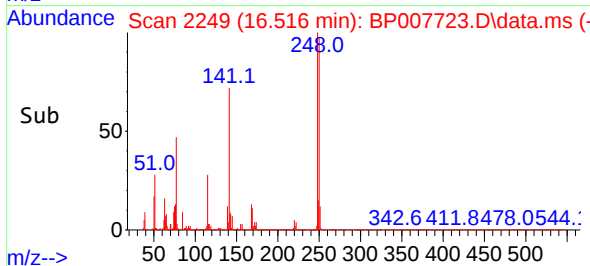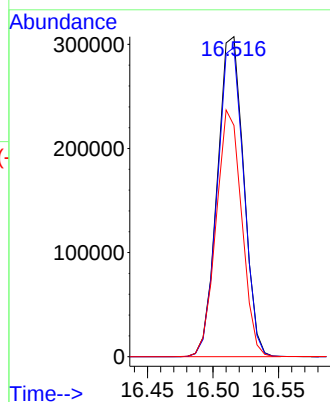


#69
Hexachlorobenzene
Concen: 36.238 ng/ul
RT: 16.634 min Scan# 2269
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

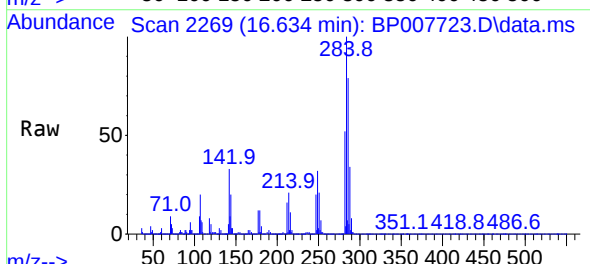


Tgt Ion:284 Resp: 493144
Ion Ratio Lower Upper
284 100
142 32.6 29.8 44.8
249 31.9 26.6 39.8

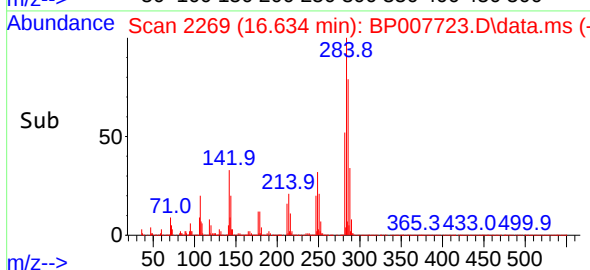



#70
Atrazine
Concen: 35.310 ng/ul
RT: 16.786 min Scan# 2295
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampled :
SLCS206




Tgt Ion:200 Resp: 455230
Ion Ratio Lower Upper
200 100
173 25.5 20.9 31.3
215 48.8 38.1 57.1

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#71
Pentachlorophenol
Concen: 35.746 ng/ul
RT: 16.975 min Scan# 2327
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:266 Resp: 302101
Ion Ratio Lower Upper
266 100
264 62.5 50.6 75.8
268 62.6 51.3 76.9





#72
Phenanthrene
Concen: 37.298 ng/u1
RT: 17.369 min Scan# 2394
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:178 Resp: 2172668
Ion Ratio Lower Upper
178 100
179 15.2 12.1 18.1
176 19.2 15.2 22.8

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#74
Anthracene
Concen: 36.925 ng/u1
RT: 17.463 min Scan# 2410
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13



Tgt Ion:178 Resp: 2139483
Ion Ratio Lower Upper
178 100
179 15.2 12.2 18.4
176 18.6 14.6 22.0









#75
1,2,3,4-Tetrachlorobenzene
Concen: 34.919 ng/uL
RT: 13.369 min Scan# 1714
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:216 Resp: 615292
Ion Ratio Lower Upper
216 100
214 77.6 62.0 93.0
218 48.0 37.6 56.4

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#76
Pentachlorobenzene
Concen: 34.814 ng/uL
RT: 14.892 min Scan# 1973
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:250 Resp: 591530
Ion Ratio Lower Upper
250 100
248 62.6 50.1 75.1
252 63.5 50.6 76.0





#77
 Carbazole
 Concen: 37.203 ng/ul
 RT: 17.728 min Scan# 2455
 Delta R.T. 0.000 min
 Lab File: BP007723.D
 Acq: 27 Oct 2021 17:13

Instrument :
 BNA_P
 ClientSampleId :
 SLCS206






Tgt Ion:167 Resp: 1989989

Ion	Ratio	Lower	Upper
167	100		
166	21.9	17.3	25.9
139	12.9	10.4	15.6

Manual Integrations
 APPROVED




mohammad
 10/28/2021 11:12:13 AM




#78
 Di-n-butylphthalate
 Concen: 38.120 ng/ul
 RT: 18.286 min Scan# 2550
 Delta R.T. -0.006 min
 Lab File: BP007723.D
 Acq: 27 Oct 2021 17:13

Tgt Ion:149 Resp: 2334476

Ion	Ratio	Lower	Upper
149	100		
150	9.3	7.3	10.9
104	5.1	4.2	6.4

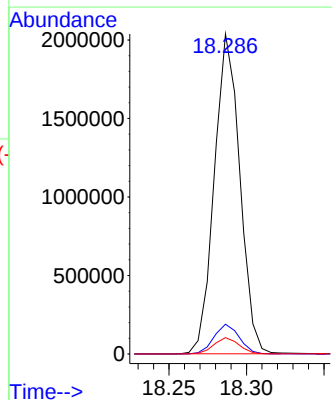




#80
Fluoranthene
Concen: 38.538 ng/u1
RT: 19.333 min Scan# 2728
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Instrument :
BNA_P
ClientSampleId :
SLCS206




Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:13 AM



Tgt Ion:202 Resp: 2716349




Ion	Ratio	Lower	Upper
202	100		
101	10.0	8.4	12.6
100	7.5	6.3	9.5

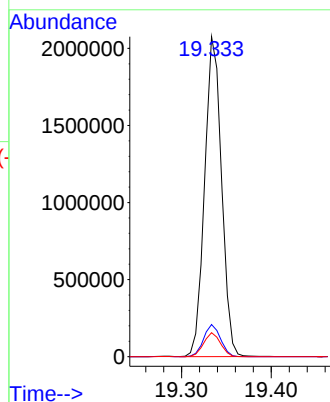


#82
Pyrene
Concen: 38.078 ng/u1
RT: 19.686 min Scan# 2788
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13

Tgt Ion:202 Resp: 2716414


Ion	Ratio	Lower	Upper
202	100		
101	11.7	9.9	14.9
100	9.6	7.9	11.9





#83
Butylbenzylphthalate
Concen: 39.450 ng/ul
RT: 20.563 min Scan# 2937
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampled :
SLCS206




Tgt Ion:149 Resp: 1095007
Ion Ratio Lower Upper
149 100
91 69.6 55.9 83.9
206 21.5 17.4 26.0

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#84
3,3'-Dichlorobenzidine
Concen: 40.141 ng/ul
RT: 21.333 min Scan# 3068
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:252 Resp: 918992
Ion Ratio Lower Upper
252 100
254 64.1 51.1 76.7
126 9.1 10.0 15.0#





#85
Benzo(a)anthracene
Concen: 37.673 ng/ul
RT: 21.404 min Scan# 3080
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:228 Resp: 2763540
Ion Ratio Lower Upper
228 100
229 19.6 15.7 23.5
226 27.3 21.4 32.0




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#86
Bis(2-ethylhexyl)phthalate
Concen: 38.337 ng/ul
RT: 21.333 min Scan# 3068
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:149 Resp: 1581188
Ion Ratio Lower Upper
149 100
167 27.4 22.6 33.8
279 4.6 3.3 4.9

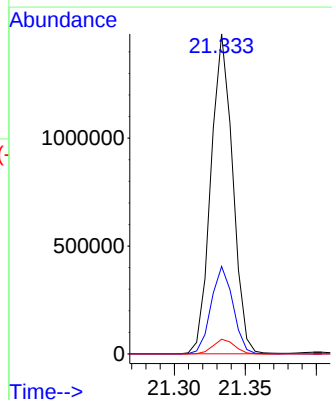



#87
Chrysene
Concen: 37.572 ng/ul
RT: 21.457 min Scan# 3089
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:228 Resp: 2664845
Ion Ratio Lower Upper
228 100
226 30.3 23.7 35.5
229 19.6 16.0 24.0




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#89
Di-n-octyl phthalate
Concen: 38.043 ng/ul
RT: 22.274 min Scan# 3228
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:149 Resp: 2814764





#90
Benzo(b)fluoranthene
Concen: 37.718 ng/ul
RT: 23.116 min Scan# 3371
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206



Tgt Ion:252 Resp: 2951983
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 8.8 7.8 11.6




Manual Integrations
APPROVED


mohammad
10/28/2021 11:12:13 AM



#91
Benzo(k)fluoranthene
Concen: 38.911 ng/ul
RT: 23.169 min Scan# 3380
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13


Tgt Ion:252 Resp: 2849837
Ion Ratio Lower Upper
252 100
253 21.8 17.6 26.4
125 8.6 8.0 12.0





#93
Benzo(a)pyrene
Concen: 38.285 ng/ul
RT: 23.757 min Scan# 3480
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampled :
SLCS206




Tgt Ion:252 Resp: 2903136
Ion Ratio Lower Upper
252 100
253 21.6 17.3 25.9
125 9.8 8.3 12.5

Manual Integrations
APPROVED



mohammad
10/28/2021 11:12:13 AM




#94
Indeno(1,2,3-cd)pyrene
Concen: 37.736 ng/ul
RT: 26.421 min Scan# 3933
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Tgt Ion:276 Resp: 3408474
Ion Ratio Lower Upper
276 100
138 22.4 17.8 26.8
277 24.9 19.8 29.6

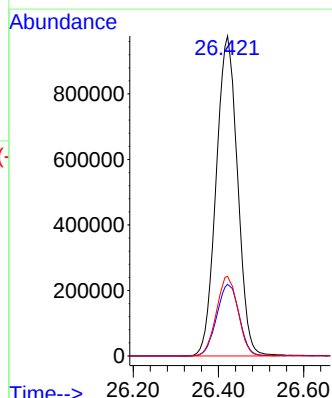



#95
Dibenzo(a,h)anthracene
Concen: 37.631 ng/ul
RT: 26.433 min Scan# 3935
Delta R.T. -0.006 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13




Instrument :
BNA_P
ClientSampleId :
SLCS206




Tgt Ion:278 Resp: 2912784
Ion Ratio Lower Upper
278 100
139 14.8 12.8 19.2
279 23.7 19.1 28.7

Manual Integrations
APPROVED

mohammad
10/28/2021 11:12:13 AM



#96
Benzo(g,h,i)perylene
Concen: 38.236 ng/ul
RT: 27.204 min Scan# 4066
Delta R.T. 0.000 min
Lab File: BP007723.D
Acq: 27 Oct 2021 17:13



Tgt Ion:276 Resp: 2937537
Ion Ratio Lower Upper
276 100
138 20.4 17.5 26.3
277 23.5 18.5 27.7

