

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007653.D
 Acq On : 25 Oct 2021 22:13
 Operator : CG/JU
 Sample : PB140162BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	21	rBV	51716	70875	1.25%	0.137%
2	3.787	82	85	106	rBV	748242	1164985	20.58%	2.246%
3	4.122	138	142	145	rVB2	11569	13987	0.25%	0.027%
4	7.105	641	649	661	rBV	813734	1308253	23.11%	2.523%
5	7.269	670	677	687	rVB	633953	1029268	18.19%	1.985%
6	7.469	703	711	722	rBV	834985	1322020	23.36%	2.549%
7	7.940	783	791	802	rVB	620286	974149	17.21%	1.878%
8	8.646	904	911	924	rBV	1038735	1612281	28.49%	3.109%
9	9.093	979	987	998	rBV	742313	1241640	21.94%	2.394%
10	9.822	1104	1111	1124	rBV	590194	990562	17.50%	1.910%
11	10.363	1193	1203	1219	rBV	976762	1660845	29.34%	3.202%
12	10.740	1259	1267	1276	rBV	785817	1375787	24.31%	2.653%
13	10.875	1281	1290	1304	rBV	996851	1676476	29.62%	3.233%
14	12.328	1531	1537	1543	rBV	19319	34219	0.60%	0.066%
15	13.987	1812	1819	1829	rBV	1809626	2563202	45.29%	4.942%
16	14.269	1853	1867	1882	rBV	1962972	2960651	52.31%	5.709%
17	14.575	1912	1919	1927	rBV	1343190	1919155	33.91%	3.701%
18	14.763	1943	1951	1966	rBV	842460	1269100	22.42%	2.447%
19	15.569	2081	2088	2101	rBV	2676991	3793443	67.02%	7.315%
20	15.681	2101	2107	2119	rBV	687179	985458	17.41%	1.900%
21	15.810	2125	2129	2135	rVB2	19518	28967	0.51%	0.056%
22	16.239	2198	2202	2207	rVB7	4168	7515	0.13%	0.014%
23	17.004	2328	2332	2337	rBV8	4321	7402	0.13%	0.014%
24	17.110	2346	2350	2357	rVB2	8216	12171	0.22%	0.023%
25	17.328	2380	2387	2396	rBV	1694839	2390317	42.23%	4.609%
26	17.428	2397	2404	2418	rBV	2959029	4199895	74.21%	8.098%
27	17.704	2447	2451	2454	rBV6	4875	8662	0.15%	0.017%
28	17.875	2474	2480	2482	rBV6	3633	7317	0.13%	0.014%
29	19.239	2707	2712	2716	rBV3	42925	61394	1.08%	0.118%
30	19.304	2719	2723	2728	rBV	40569	59996	1.06%	0.116%
31	19.663	2778	2784	2796	rBV	3767136	5143275	90.87%	9.917%
32	21.192	3041	3044	3050	rBV	199856	257489	4.55%	0.496%
33	21.416	3077	3082	3095	rBV	2264998	2970071	52.48%	5.727%
34	23.704	3463	3471	3480	rBV2	2755682	5659803	100.00%	10.913%
35	23.857	3491	3497	3507	rVB2	1471470	3081145	54.44%	5.941%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007653.D
Acq On : 25 Oct 2021 22:13
Operator : CG/JU
Sample : PB140162BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK162

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION


Sum of corrected areas: 51861775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007653.D
Acq On : 25 Oct 2021 22:13
Operator : CG/JU
Sample : PB140162BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK162

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

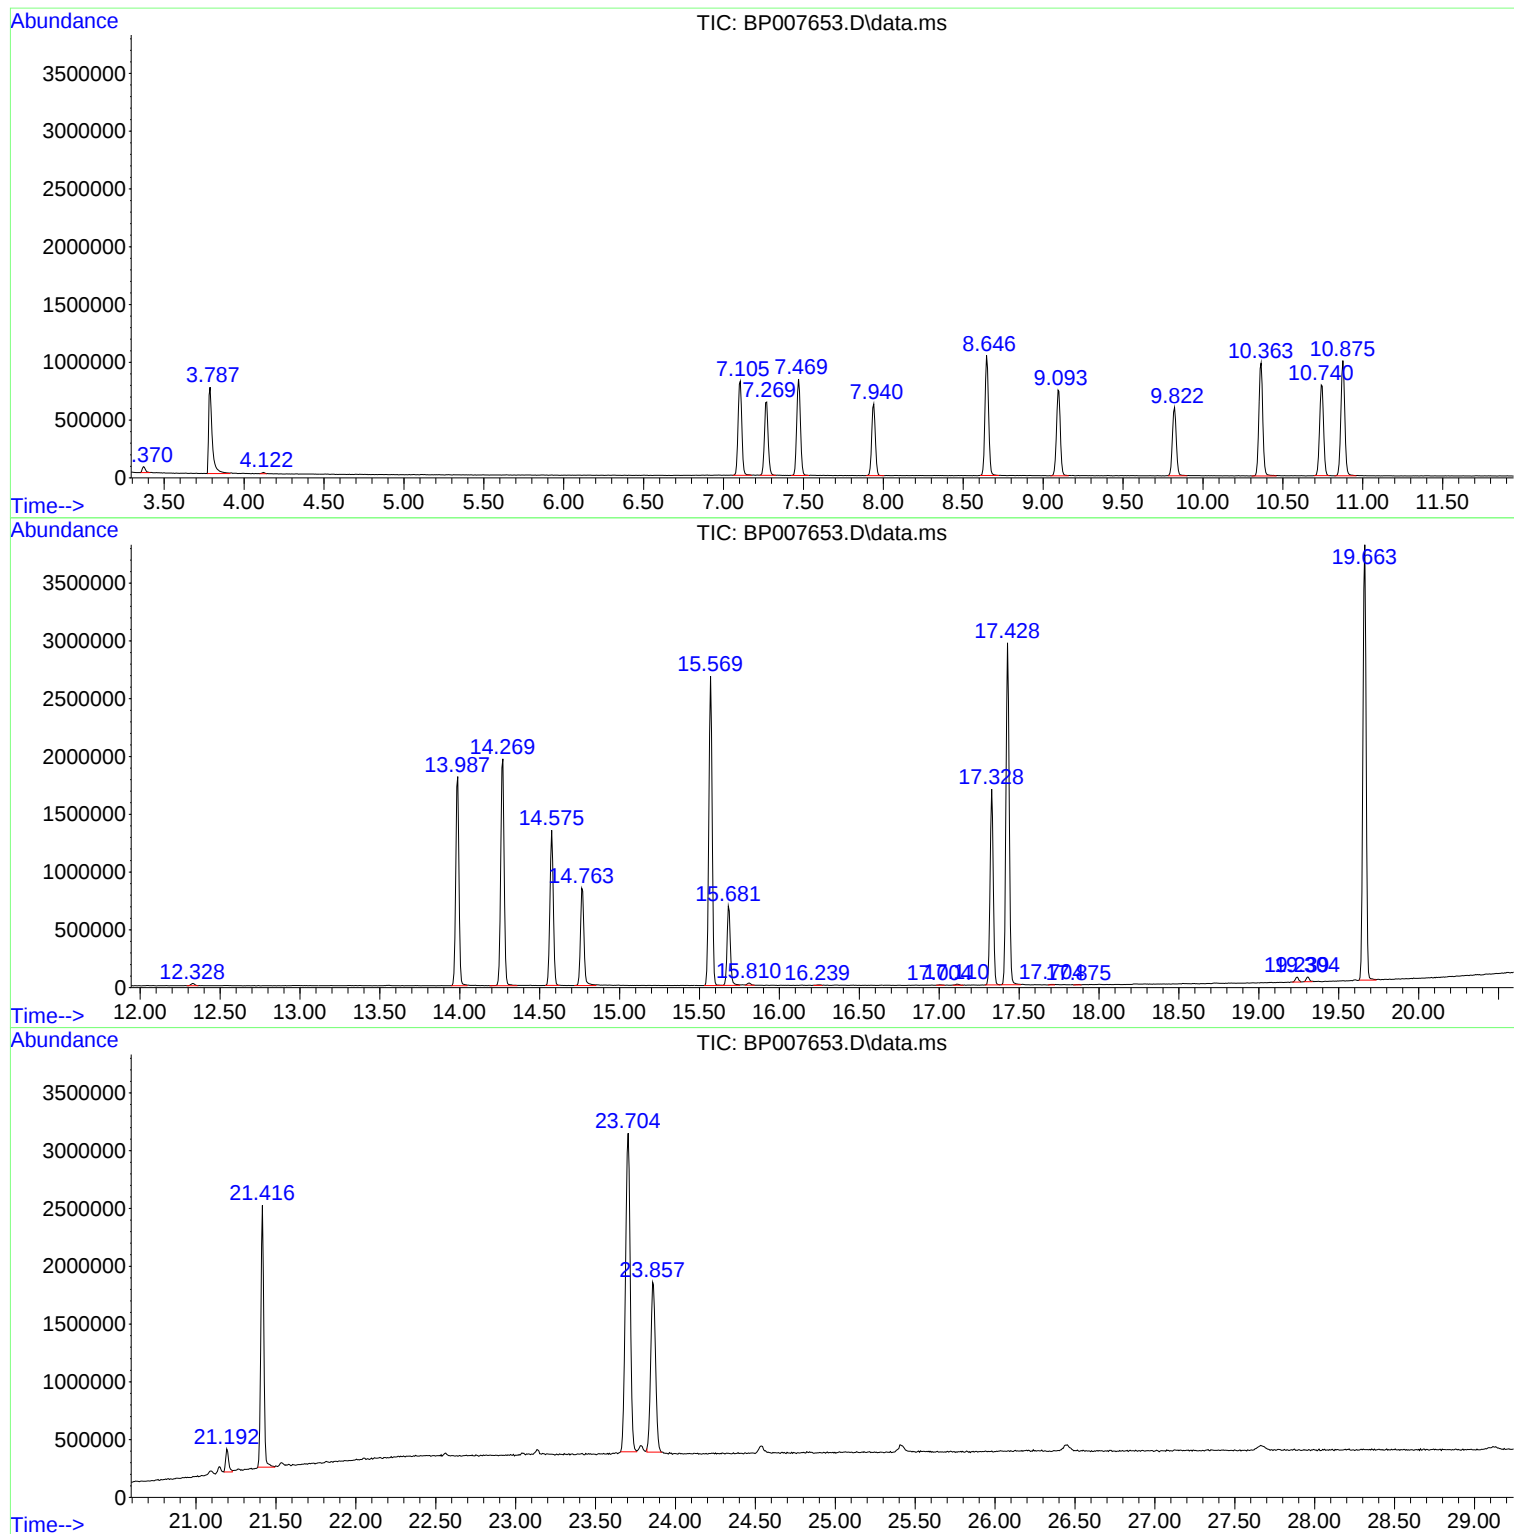

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007653.D
Acq On : 25 Oct 2021 22:13
Operator : CG/JU
Sample : PB140162BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK162

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007653.D
Acq On : 25 Oct 2021 22:13
Operator : CG/JU
Sample : PB140162BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK162

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
