

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007656.D
 Acq On : 25 Oct 2021 23:55
 Operator : CG/JU
 Sample : M4303-21
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P055-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rBV	46361	58613	1.01%	0.123%
2	3.787	83	85	100	rBV	204110	327589	5.65%	0.687%
3	3.993	116	120	121	rBV4	5023	6967	0.12%	0.015%
4	4.028	121	126	130	rVB2	28160	44072	0.76%	0.092%
5	4.123	138	142	147	rVB	9996	14692	0.25%	0.031%
6	4.217	153	158	164	rVB4	13137	19440	0.34%	0.041%
7	5.046	295	299	304	rVB5	10459	17927	0.31%	0.038%
8	6.322	511	516	521	rBV	11752	17488	0.30%	0.037%
9	7.099	641	648	659	rVB	172864	285890	4.93%	0.600%
10	7.264	668	676	688	rBV	598041	972434	16.76%	2.039%
11	7.469	703	711	719	rBV	646843	996705	17.18%	2.090%
12	7.569	726	728	735	rVB8	4843	6954	0.12%	0.015%
13	7.940	783	791	799	rBV	611916	988800	17.04%	2.074%
14	8.646	902	911	924	rBV	496944	801348	13.81%	1.680%
15	9.093	978	987	1002	rBV	728838	1176998	20.28%	2.468%
16	9.822	1100	1111	1127	rBV	542956	914842	15.77%	1.918%
17	10.363	1194	1203	1212	rBV	854661	1421915	24.51%	2.982%
18	10.534	1228	1232	1239	rBV5	7834	13307	0.23%	0.028%
19	10.740	1259	1267	1280	rVB	832400	1418455	24.45%	2.975%
20	10.875	1280	1290	1301	rBV	753695	1306486	22.52%	2.740%
21	12.328	1531	1537	1545	rVB2	18461	33457	0.58%	0.070%
22	13.551	1737	1745	1751	rVB10	4361	10149	0.17%	0.021%
23	13.987	1812	1819	1832	rBV	1743777	2466791	42.51%	5.173%
24	14.269	1855	1867	1876	rBV	1881494	2834307	48.85%	5.944%
25	14.575	1910	1919	1929	rBV	1309181	1964326	33.85%	4.119%
26	14.763	1945	1951	1965	rBV2	148198	241886	4.17%	0.507%
27	14.993	1985	1990	1995	rBV8	12814	19992	0.34%	0.042%
28	15.569	2080	2088	2096	rBV	2582943	3777830	65.11%	7.922%
29	15.681	2101	2107	2121	rVV	731883	1003010	17.29%	2.103%
30	15.804	2124	2128	2135	rVB2	19084	31955	0.55%	0.067%
31	16.245	2198	2203	2204	rBV5	6447	8551	0.15%	0.018%
32	16.263	2204	2206	2211	rVB6	7024	8075	0.14%	0.017%
33	16.357	2219	2222	2227	rVB6	5737	7977	0.14%	0.017%
34	17.110	2345	2350	2353	rBV2	8883	14426	0.25%	0.030%
35	17.328	2380	2387	2396	rBV	1749369	2410161	41.54%	5.054%
36	17.428	2397	2404	2417	rVV	3100124	4344637	74.87%	9.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007656.D
 Acq On : 25 Oct 2021 23:55
 Operator : CG/JU
 Sample : M4303-21
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P055-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.522	2418	2420	2426	rVB6	9088	11709	0.20%	0.025%
38	18.004	2499	2502	2507	rVB6	6013	9576	0.17%	0.020%
39	18.222	2535	2539	2547	rBV9	20649	35964	0.62%	0.075%
40	18.292	2547	2551	2555	rVB3	5504	9771	0.17%	0.020%
41	19.239	2707	2712	2718	rBV3	42264	65377	1.13%	0.137%
42	19.304	2719	2723	2731	rVV	47403	71738	1.24%	0.150%
43	19.604	2771	2774	2776	rBV3	13408	14264	0.25%	0.030%
44	19.663	2777	2784	2791	rBV	3876839	5361087	92.39%	11.242%
45	20.975	3005	3007	3010	rBV3	32813	26969	0.46%	0.057%
46	21.192	3041	3044	3049	rBV	159440	183262	3.16%	0.384%
47	21.416	3076	3082	3087	rBV	2254098	2978407	51.33%	6.246%
48	23.698	3463	3470	3480	rBV2	2833618	5802540	100.00%	12.168%
49	23.857	3491	3497	3508	rVB2	1513151	3127529	53.90%	6.559%


Sum of corrected areas: 47686645

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007656.D
Acq On : 25 Oct 2021 23:55
Operator : CG/JU
Sample : M4303-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P055-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

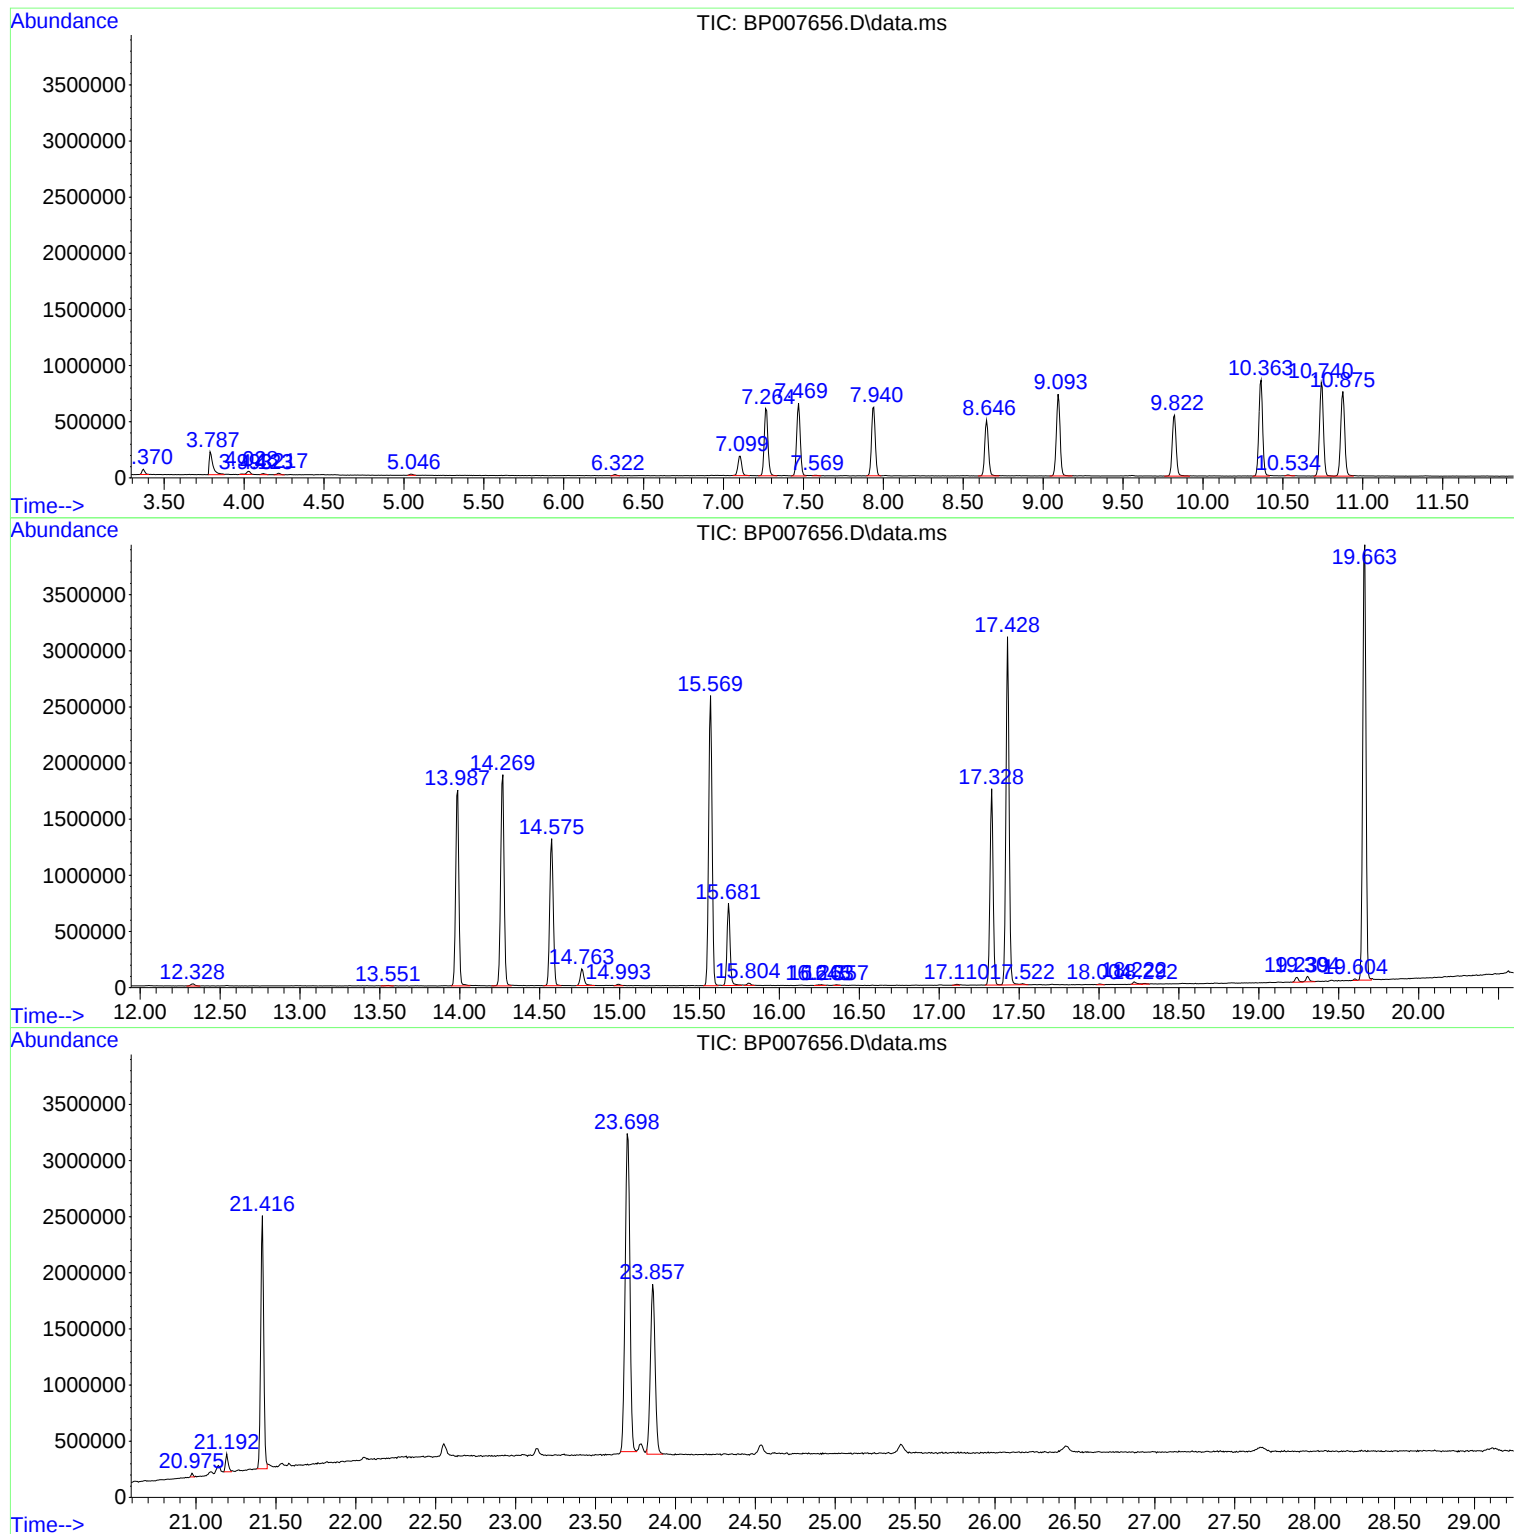

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007656.D
Acq On : 25 Oct 2021 23:55
Operator : CG/JU
Sample : M4303-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P055-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007656.D
Acq On : 25 Oct 2021 23:55
Operator : CG/JU
Sample : M4303-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P055-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
