

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007657.D
 Acq On : 26 Oct 2021 00:29
 Operator : CG/JU
 Sample : M4304-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P056-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	25	rVB	43578	63631	0.97%	0.120%
2	3.793	84	86	100	rBV	80680	125627	1.92%	0.238%
3	4.028	121	126	132	rVB	30847	48081	0.73%	0.091%
4	4.122	138	142	146	rVB2	13092	17024	0.26%	0.032%
5	4.216	154	158	162	rBV5	11155	16530	0.25%	0.031%
6	5.046	295	299	303	rVB4	5818	8712	0.13%	0.016%
7	6.322	509	516	522	rVB2	10983	20917	0.32%	0.040%
8	7.099	642	648	659	rBV	207534	332971	5.08%	0.630%
9	7.263	670	676	688	rVB	678688	1090024	16.62%	2.064%
10	7.469	702	711	718	rBV	736056	1135850	17.32%	2.151%
11	7.940	783	791	798	rBV	673402	1063329	16.21%	2.013%
12	8.646	902	911	922	rBV	572622	908890	13.86%	1.721%
13	9.093	978	987	997	rBV	792276	1328068	20.25%	2.515%
14	9.557	1059	1066	1072	rBV10	4328	8898	0.14%	0.017%
15	9.822	1103	1111	1122	rBV	623307	1024767	15.63%	1.940%
16	10.363	1195	1203	1212	rBV	960471	1593082	24.29%	3.016%
17	10.528	1225	1231	1242	rBV	40143	75415	1.15%	0.143%
18	10.740	1259	1267	1277	rBV	888737	1490748	22.73%	2.823%
19	10.875	1279	1290	1302	rBV	768985	1336051	20.37%	2.530%
20	12.328	1530	1537	1545	rBV3	20695	37110	0.57%	0.070%
21	13.192	1680	1684	1690	rVB7	6232	8694	0.13%	0.016%
22	13.310	1697	1704	1709	rVB7	3287	7926	0.12%	0.015%
23	13.487	1731	1734	1737	rVV5	4252	6559	0.10%	0.012%
24	13.545	1739	1744	1750	rVB8	5634	10907	0.17%	0.021%
25	13.987	1812	1819	1833	rBV	1916172	2748669	41.91%	5.204%
26	14.263	1853	1866	1878	rBV	2051340	3108144	47.39%	5.885%
27	14.575	1910	1919	1929	rBV	1394124	2097651	31.99%	3.972%
28	14.763	1943	1951	1967	rBV	192109	314776	4.80%	0.596%
29	14.992	1984	1990	1995	rBV6	13755	19404	0.30%	0.037%
30	15.386	2053	2057	2062	rBV7	5014	8984	0.14%	0.017%
31	15.569	2081	2088	2096	rBV	2859672	4106451	62.62%	7.775%
32	15.681	2101	2107	2122	rVV	825355	1168487	17.82%	2.212%
33	15.810	2124	2129	2134	rVV	21647	37187	0.57%	0.070%
34	16.263	2198	2206	2212	rBV	36462	63618	0.97%	0.120%
35	16.333	2214	2218	2221	rBV5	6267	8812	0.13%	0.017%
36	16.998	2329	2331	2336	rVB6	5340	7063	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007657.D
 Acq On : 26 Oct 2021 00:29
 Operator : CG/JU
 Sample : M4304-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P056-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.110	2346	2350	2354	rBV3	10881	17671	0.27%	0.033%
38	17.263	2370	2376	2379	rBV8	4479	7289	0.11%	0.014%
39	17.328	2380	2387	2397	rBV	1796854	2589223	39.48%	4.902%
40	17.428	2397	2404	2417	rBV	3483787	4961632	75.66%	9.394%
41	17.704	2446	2451	2455	rBV6	5529	11875	0.18%	0.022%
42	18.004	2499	2502	2506	rBV2	18990	23912	0.36%	0.045%
43	18.222	2535	2539	2547	rBV7	30001	47704	0.73%	0.090%
44	18.522	2587	2590	2595	rBV7	8927	13277	0.20%	0.025%
45	19.233	2707	2711	2718	rBV	50608	75825	1.16%	0.144%
46	19.304	2719	2723	2732	rVB	56216	84303	1.29%	0.160%
47	19.451	2746	2748	2752	rBV4	12075	17600	0.27%	0.033%
48	19.598	2771	2773	2777	rBV5	12420	13110	0.20%	0.025%
49	19.663	2777	2784	2797	rBV	4301044	6110346	93.17%	11.569%
50	21.133	3031	3034	3040	rBV3	92565	155641	2.37%	0.295%
51	21.192	3041	3044	3051	rVV	136532	178976	2.73%	0.339%
52	21.416	3077	3082	3093	rBV	2468630	3180618	48.50%	6.022%
53	23.704	3463	3471	3480	rBV2	3219063	6558112	100.00%	12.417%
54	23.857	3491	3497	3508	rVB2	1591900	3319277	50.61%	6.285%


Sum of corrected areas: 52815448

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007657.D
Acq On : 26 Oct 2021 00:29
Operator : CG/JU
Sample : M4304-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P056-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

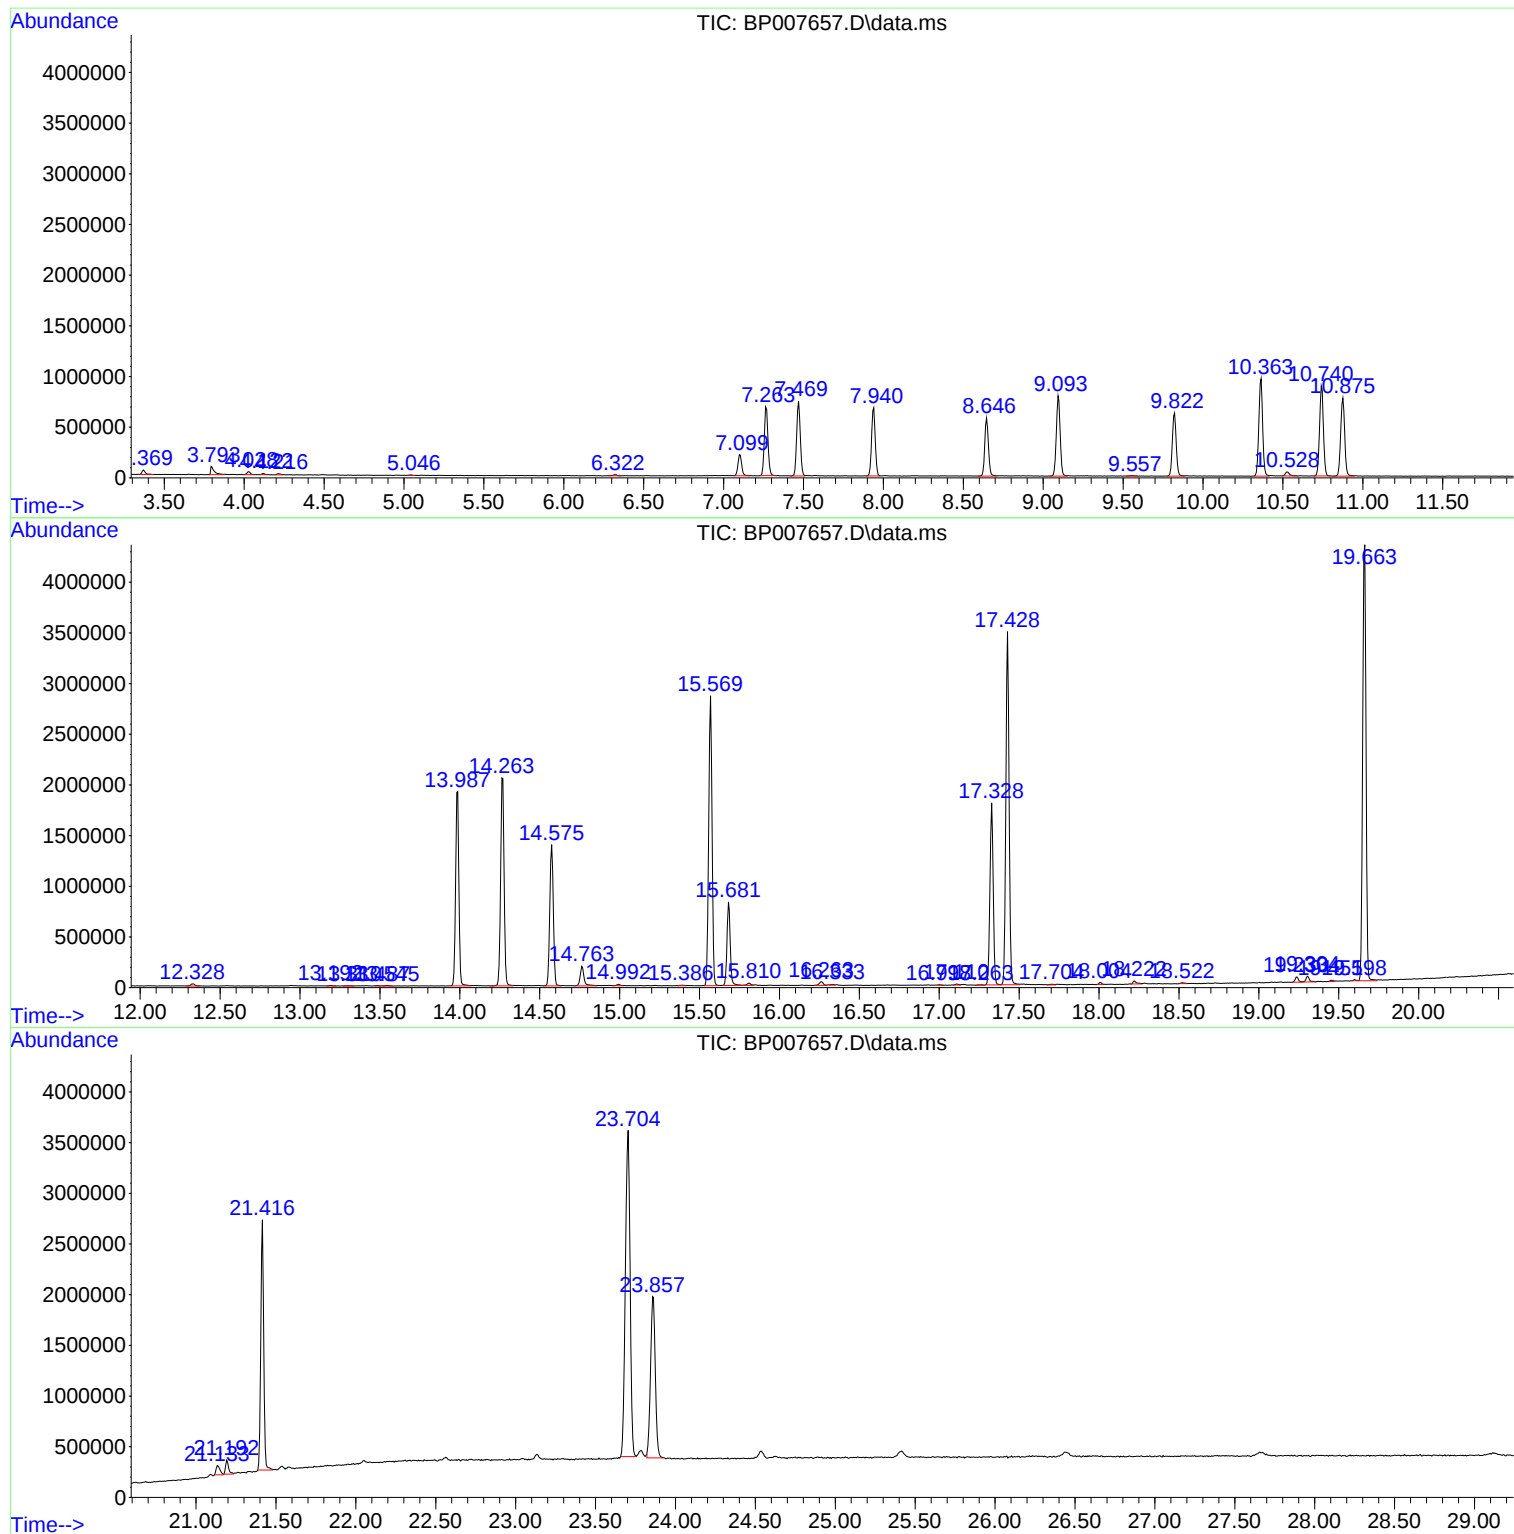

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007657.D
Acq On : 26 Oct 2021 00:29
Operator : CG/JU
Sample : M4304-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P056-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007657.D
Acq On : 26 Oct 2021 00:29
Operator : CG/JU
Sample : M4304-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P056-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
