

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007658.D
 Acq On : 26 Oct 2021 01:03
 Operator : CG/JU
 Sample : M4304-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P064-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	11	14	22	rVB	50699	64202	1.06%	0.128%
2	3.658	59	63	66	rBV6	4630	6825	0.11%	0.014%
3	3.793	84	86	99	rBV	78879	114897	1.89%	0.229%
4	4.028	121	126	132	rVB	28833	43093	0.71%	0.086%
5	4.122	138	142	151	rVB2	12526	22347	0.37%	0.045%
6	4.216	154	158	163	rVB4	13972	20507	0.34%	0.041%
7	5.040	294	298	304	rVB6	7226	12182	0.20%	0.024%
8	6.316	509	515	522	rBV3	10795	19882	0.33%	0.040%
9	7.099	642	648	656	rBV	190321	300941	4.96%	0.601%
10	7.263	670	676	690	rVB	672284	1073664	17.70%	2.143%
11	7.469	704	711	719	rBV	687155	1074668	17.71%	2.145%
12	7.575	722	729	733	rVB10	5283	10866	0.18%	0.022%
13	7.934	784	790	799	rBV	684967	1125447	18.55%	2.246%
14	8.010	799	803	806	rVB6	5339	7009	0.12%	0.014%
15	8.193	827	834	837	rBV9	3145	6860	0.11%	0.014%
16	8.646	901	911	925	rBV	534692	863014	14.23%	1.723%
17	8.757	926	930	934	rVB7	3874	6514	0.11%	0.013%
18	9.093	980	987	996	rBV	791102	1279417	21.09%	2.554%
19	9.557	1061	1066	1072	rBV6	5340	10076	0.17%	0.020%
20	9.816	1102	1110	1118	rBV	583656	982337	16.19%	1.961%
21	10.363	1192	1203	1220	rBV	928777	1574426	25.95%	3.143%
22	10.522	1224	1230	1239	rBV	86570	157204	2.59%	0.314%
23	10.740	1258	1267	1282	rBV	920715	1585584	26.14%	3.165%
24	10.875	1282	1290	1301	rBV	188133	328345	5.41%	0.655%
25	12.328	1533	1537	1541	rBV2	20028	32127	0.53%	0.064%
26	12.369	1541	1544	1548	rVB5	7018	9692	0.16%	0.019%
27	13.416	1718	1722	1727	rVB8	4552	6640	0.11%	0.013%
28	13.487	1727	1734	1737	rBV7	5763	9673	0.16%	0.019%
29	13.551	1740	1745	1752	rBV8	5787	12703	0.21%	0.025%
30	13.987	1812	1819	1825	rBV	1772434	2547401	41.99%	5.085%
31	14.269	1856	1867	1880	rBV	2027605	3044836	50.19%	6.077%
32	14.487	1900	1904	1907	rVB6	5202	6733	0.11%	0.013%
33	14.575	1910	1919	1932	rBV	1461702	2199185	36.25%	4.390%
34	14.763	1946	1951	1963	rBV	156588	250407	4.13%	0.500%
35	15.298	2038	2042	2048	rBV9	3645	6896	0.11%	0.014%
36	15.569	2081	2088	2098	rBV	2774205	3910374	64.46%	7.805%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007658.D
 Acq On : 26 Oct 2021 01:03
 Operator : CG/JU
 Sample : M4304-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P064-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.681	2101	2107	2118	rBV	725994	1007345	16.61%	2.011%
38	15.810	2124	2129	2134	rVV3	19454	30492	0.50%	0.061%
39	16.139	2180	2185	2189	rBV8	5059	9728	0.16%	0.019%
40	16.251	2198	2204	2210	rBV8	6576	15600	0.26%	0.031%
41	17.010	2329	2333	2337	rVB6	6107	8598	0.14%	0.017%
42	17.110	2346	2350	2354	rBV2	9173	14615	0.24%	0.029%
43	17.328	2380	2387	2397	rBV	1902903	2700878	44.52%	5.391%
44	17.428	2397	2404	2417	rVV	3196307	4523770	74.57%	9.029%
45	17.698	2448	2450	2455	rBV6	5349	8466	0.14%	0.017%
46	18.010	2499	2503	2508	rBV	19196	26008	0.43%	0.052%
47	18.222	2535	2539	2545	rBV4	32858	49793	0.82%	0.099%
48	18.522	2586	2590	2597	rBV8	10014	19228	0.32%	0.038%
49	19.239	2707	2712	2716	rBV2	47856	67606	1.11%	0.135%
50	19.304	2719	2723	2728	rVV	48644	67211	1.11%	0.134%
51	19.604	2771	2774	2777	rBV4	13187	15938	0.26%	0.032%
52	19.657	2778	2783	2794	rVV	4048576	5533004	91.21%	11.044%
53	21.139	3031	3035	3041	rBV4	87076	159684	2.63%	0.319%
54	21.192	3041	3044	3050	rVV	143724	169076	2.79%	0.337%
55	21.416	3077	3082	3087	rBV	2545661	3300252	54.40%	6.587%
56	23.704	3463	3471	3480	rBV2	2983989	6066458	100.00%	12.109%
57	23.857	3490	3497	3511	rVB2	1681659	3579675	59.01%	7.145%




Sum of corrected areas: 50100399

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007658.D
Acq On : 26 Oct 2021 01:03
Operator : CG/JU
Sample : M4304-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P064-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

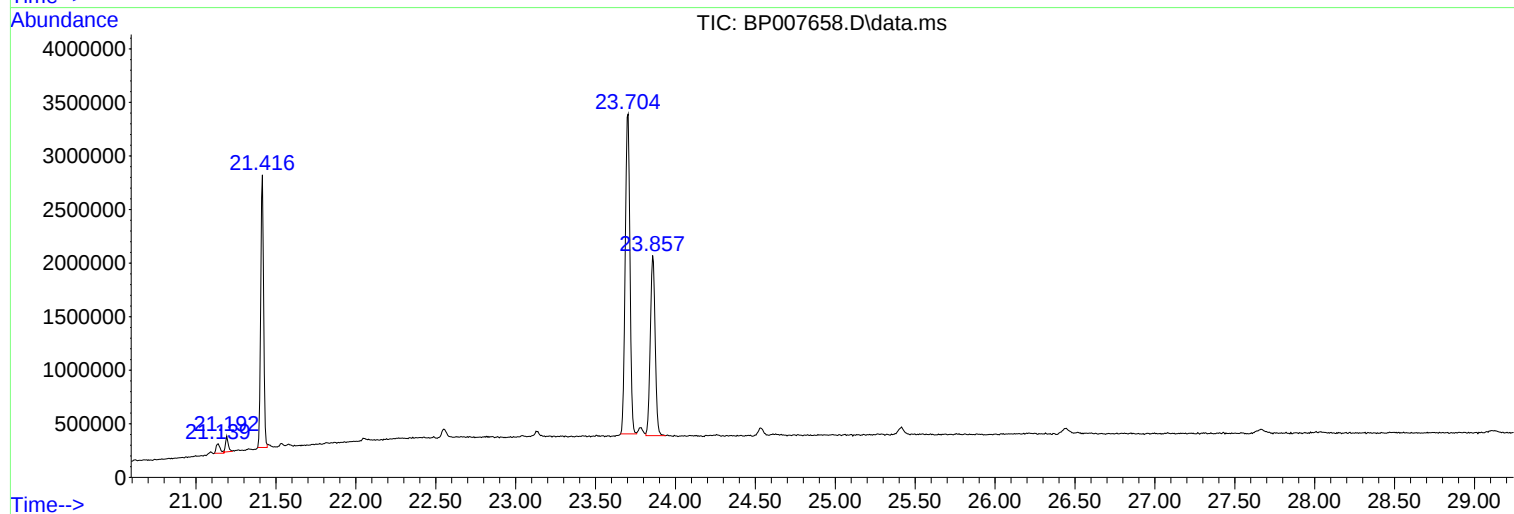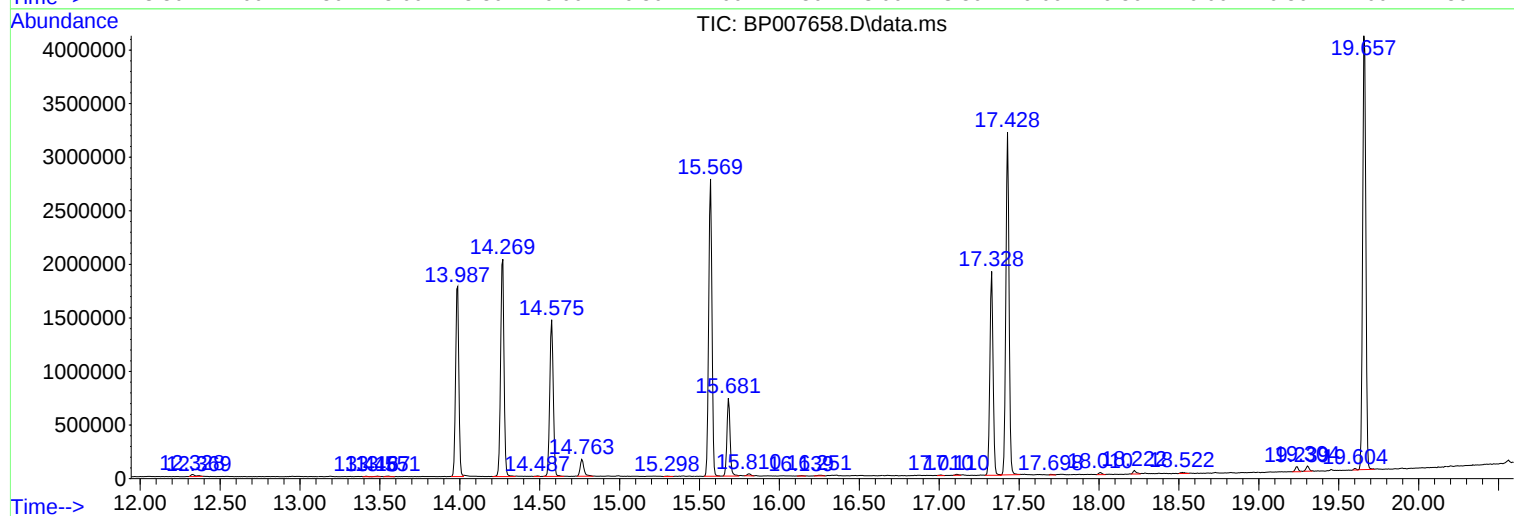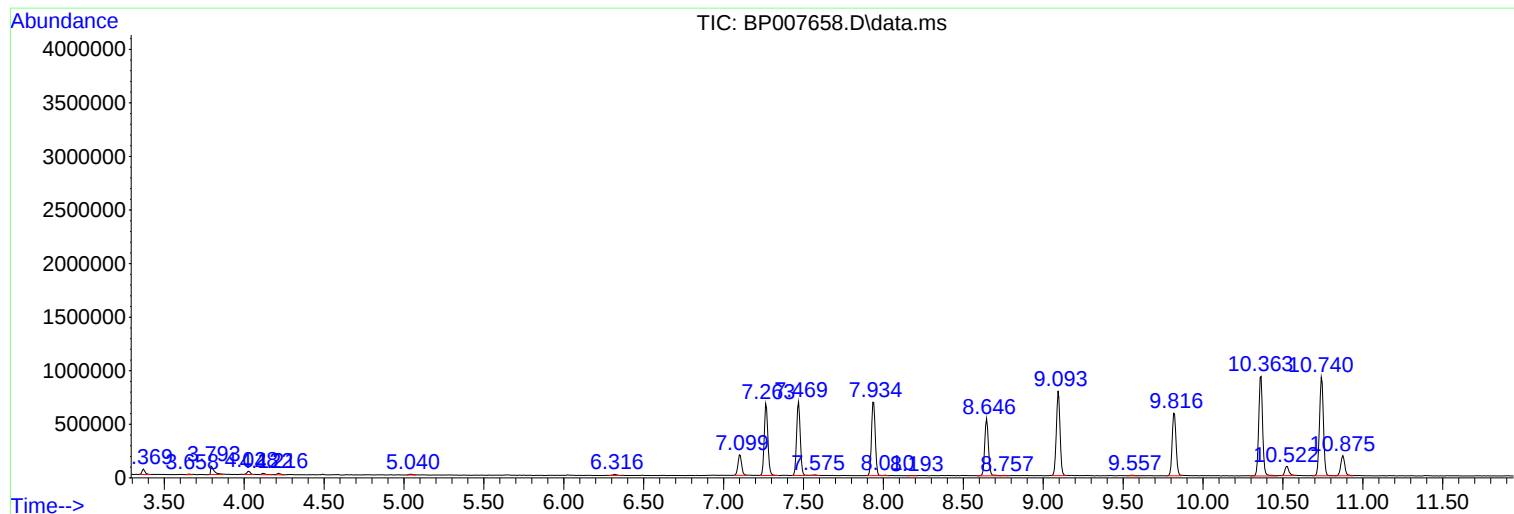

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007658.D
Acq On : 26 Oct 2021 01:03
Operator : CG/JU
Sample : M4304-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P064-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007658.D
Acq On : 26 Oct 2021 01:03
Operator : CG/JU
Sample : M4304-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P064-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
