

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007659.D
 Acq On : 26 Oct 2021 01:36
 Operator : CG/JU
 Sample : M4304-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P061-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	19	rVB	48438	58076	0.85%	0.110%
2	3.787	83	85	96	rBV	177671	286870	4.18%	0.545%
3	4.028	121	126	131	rVB	31412	44025	0.64%	0.084%
4	4.117	138	141	150	rVB	13796	20137	0.29%	0.038%
5	4.217	154	158	162	rVB5	13701	20095	0.29%	0.038%
6	5.040	294	298	304	rVB4	10771	18766	0.27%	0.036%
7	6.322	511	516	523	rVB5	12684	21462	0.31%	0.041%
8	7.099	642	648	656	rVB	191792	307638	4.48%	0.585%
9	7.263	670	676	687	rVB	715403	1123805	16.37%	2.137%
10	7.469	704	711	721	rBV	719197	1135206	16.54%	2.159%
11	7.934	783	790	798	rBV	594023	968184	14.10%	1.841%
12	8.646	904	911	922	rBV	554932	891438	12.99%	1.695%
13	9.093	979	987	998	rBV	826332	1369080	19.94%	2.603%
14	9.816	1102	1110	1126	rBV	644418	1064015	15.50%	2.023%
15	10.357	1195	1202	1216	rBV	955537	1639318	23.88%	3.117%
16	10.534	1226	1232	1239	rBV6	6962	13131	0.19%	0.025%
17	10.740	1259	1267	1276	rBV	821610	1361309	19.83%	2.589%
18	10.875	1281	1290	1300	rBV	893137	1528366	22.26%	2.906%
19	12.328	1531	1537	1542	rBV2	22581	36294	0.53%	0.069%
20	13.540	1737	1743	1749	rBV10	4369	7885	0.11%	0.015%
21	13.987	1812	1819	1826	rBV	1943842	2781147	40.51%	5.288%
22	14.263	1856	1866	1877	rBV	2107549	3224882	46.98%	6.132%
23	14.575	1912	1919	1928	rBV	1285651	1871057	27.26%	3.558%
24	14.763	1945	1951	1958	rBV	184374	268444	3.91%	0.510%
25	14.992	1986	1990	1997	rVB3	18000	24702	0.36%	0.047%
26	15.398	2054	2059	2062	rBV6	5494	7636	0.11%	0.015%
27	15.569	2080	2088	2101	rBV	2981991	4314059	62.84%	8.203%
28	15.681	2101	2107	2119	rBV	883694	1220101	17.77%	2.320%
29	15.810	2124	2129	2135	rVB2	23274	36491	0.53%	0.069%
30	16.245	2198	2203	2204	rBV5	7327	9177	0.13%	0.017%
31	16.351	2218	2221	2228	rVB8	5820	10214	0.15%	0.019%
32	17.004	2329	2332	2337	rVB7	4880	7061	0.10%	0.013%
33	17.110	2345	2350	2356	rBV4	10461	18689	0.27%	0.036%
34	17.328	2380	2387	2395	rBV	1658147	2302322	33.54%	4.378%
35	17.428	2397	2404	2414	rBV2	3626216	5172050	75.34%	9.835%
36	18.004	2498	2502	2506	rBV6	6736	10825	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007659.D
Acq On : 26 Oct 2021 01:36
Operator : CG/JU
Sample : M4304-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P061-TW001-01

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	18.216	2535	2538	2541	rBV3	10022	13504	0.20%	0.026%
38	19.239	2708	2712	2716	rBV2	52028	73511	1.07%	0.140%
39	19.304	2719	2723	2729	rVV2	54151	74712	1.09%	0.142%
40	19.663	2778	2784	2795	rBV	4486928	6322820	92.11%	12.023%
41	21.192	3041	3044	3051	rBV	104959	136865	1.99%	0.260%
42	21.416	3076	3082	3093	rBV	2153961	2924334	42.60%	5.561%
43	23.704	3463	3471	3480	rVB2	3415030	6864789	100.00%	13.053%
44	23.857	3490	3497	3511	rVB2	1393003	2985298	43.49%	5.677%


Sum of corrected areas: 52589790

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007659.D
Acq On : 26 Oct 2021 01:36
Operator : CG/JU
Sample : M4304-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P061-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

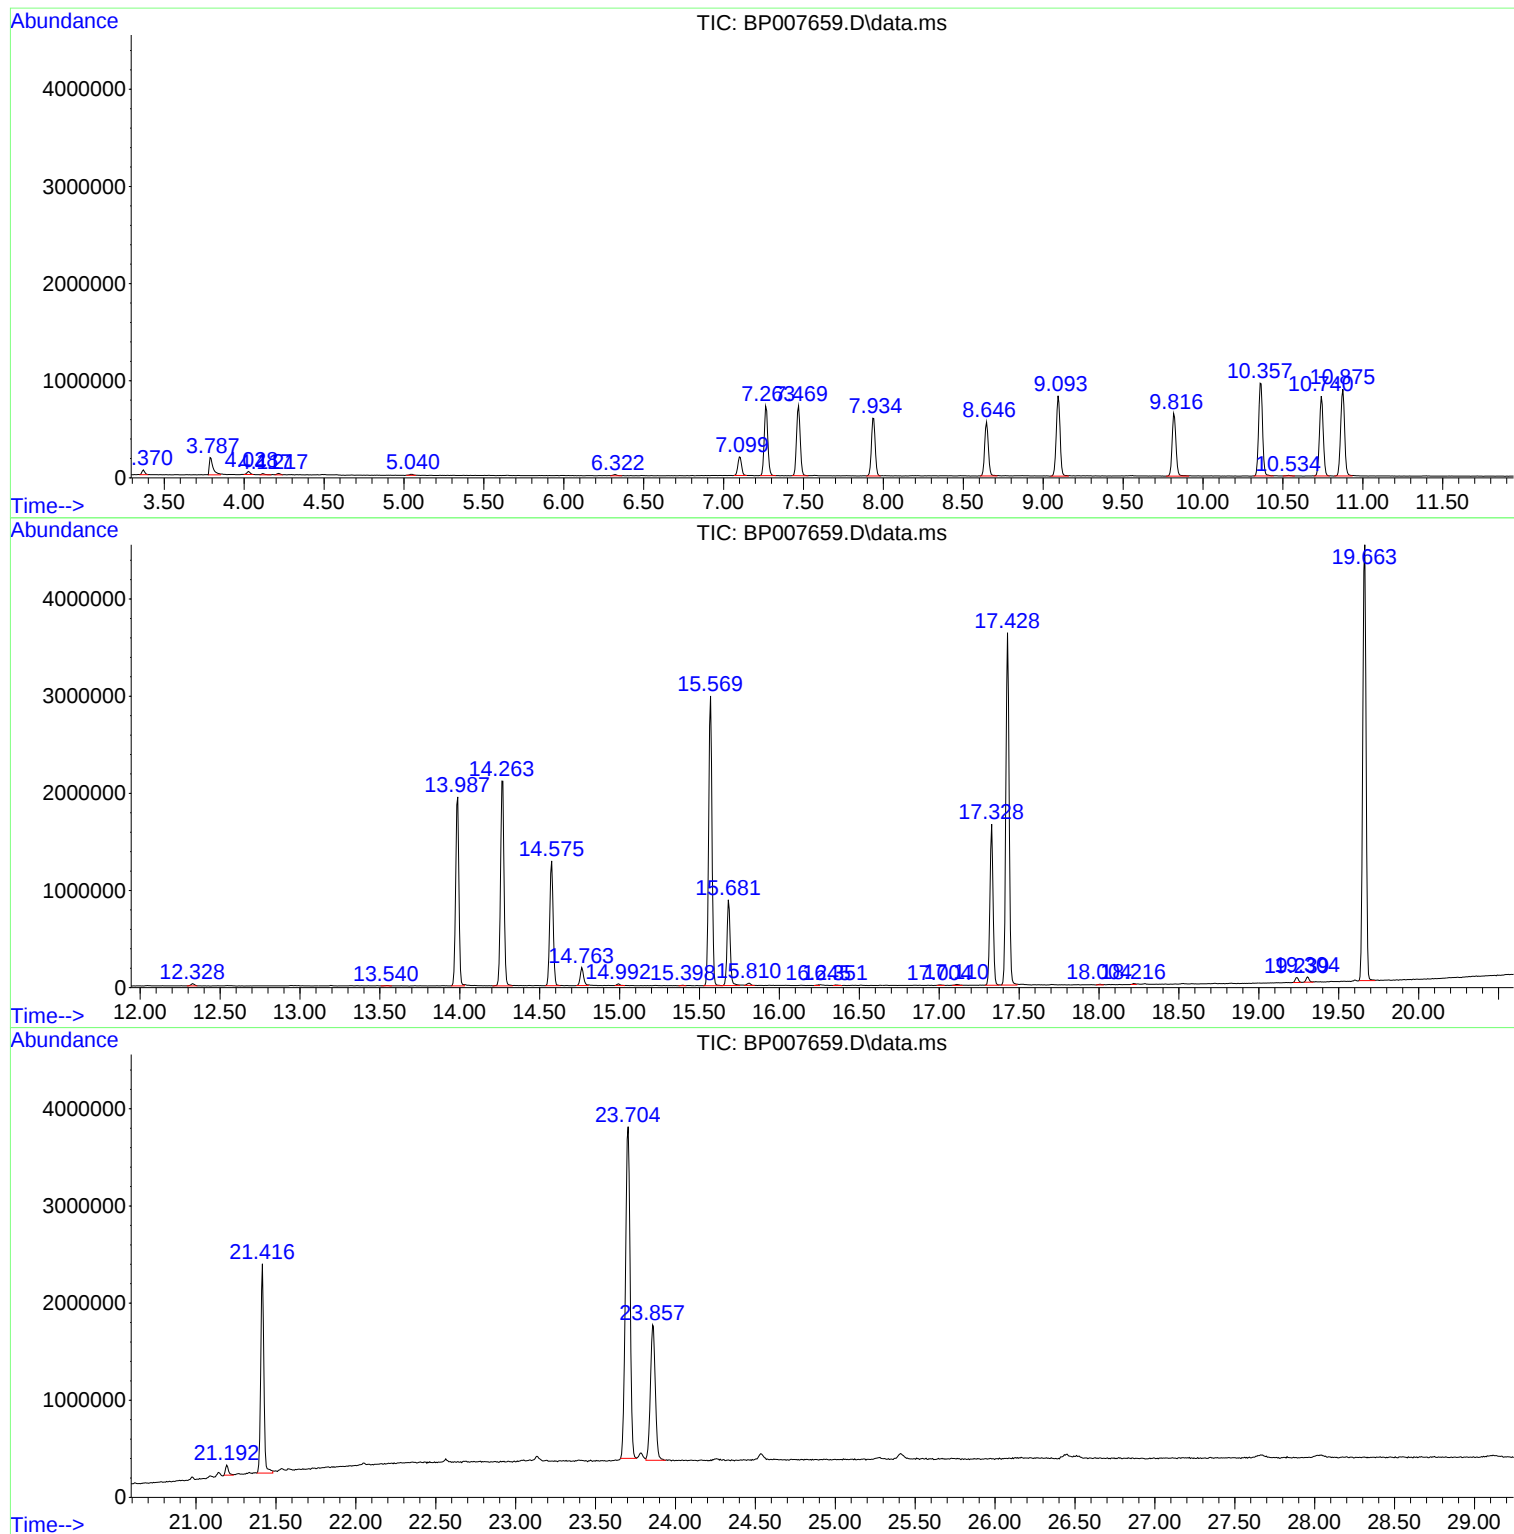

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007659.D
Acq On : 26 Oct 2021 01:36
Operator : CG/JU
Sample : M4304-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P061-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007659.D
Acq On : 26 Oct 2021 01:36
Operator : CG/JU
Sample : M4304-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P061-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
