

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007660.D
 Acq On : 26 Oct 2021 02:10
 Operator : CG/JU
 Sample : M4304-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P063-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	20	rVB	47804	59375	0.86%	0.106%
2	3.793	84	86	99	rBV	149112	239028	3.47%	0.428%
3	4.028	121	126	135	rVB2	36588	59280	0.86%	0.106%
4	4.116	137	141	146	rVB2	14257	20991	0.30%	0.038%
5	4.216	154	158	162	rVB5	13915	19402	0.28%	0.035%
6	5.034	294	297	305	rVB3	7349	14410	0.21%	0.026%
7	6.322	510	516	522	rVB3	14017	22882	0.33%	0.041%
8	7.098	642	648	657	rVB	238674	372385	5.41%	0.667%
9	7.263	670	676	687	rVB	711461	1129217	16.40%	2.023%
10	7.469	703	711	719	rBV	746851	1181976	17.17%	2.117%
11	7.575	725	729	736	rVB8	4945	9650	0.14%	0.017%
12	7.940	783	791	800	rBV	706392	1134000	16.47%	2.031%
13	8.004	800	802	808	rVB5	5817	8628	0.13%	0.015%
14	8.645	902	911	924	rBV	633579	1009454	14.66%	1.808%
15	9.092	980	987	996	rBV	839463	1363684	19.81%	2.443%
16	9.551	1060	1065	1074	rVB9	6819	15174	0.22%	0.027%
17	9.822	1102	1111	1120	rBV	619391	1051417	15.27%	1.883%
18	10.363	1194	1203	1219	rBV	991492	1682545	24.44%	3.014%
19	10.522	1223	1230	1241	rBV	60049	108875	1.58%	0.195%
20	10.739	1259	1267	1277	rBV	942742	1605760	23.33%	2.876%
21	10.875	1282	1290	1298	rBV	894340	1506868	21.89%	2.699%
22	12.057	1485	1491	1494	rBV8	4361	8150	0.12%	0.015%
23	12.328	1532	1537	1544	rVB2	23644	34726	0.50%	0.062%
24	12.945	1638	1642	1649	rBV8	6697	16881	0.25%	0.030%
25	13.192	1678	1684	1690	rVB7	7490	12164	0.18%	0.022%
26	13.551	1739	1745	1748	rBV4	5623	11465	0.17%	0.021%
27	13.986	1811	1819	1832	rBV	1907869	2836639	41.21%	5.081%
28	14.269	1856	1867	1875	rBV	2191301	3253419	47.26%	5.828%
29	14.574	1912	1919	1933	rVB	1517404	2244974	32.61%	4.021%
30	14.763	1943	1951	1963	rBV	230714	360344	5.23%	0.645%
31	14.992	1986	1990	1995	rVB6	13501	19429	0.28%	0.035%
32	15.392	2051	2058	2062	rBV6	6422	12934	0.19%	0.023%
33	15.569	2079	2088	2097	rBV	2911566	4262451	61.92%	7.635%
34	15.680	2100	2107	2118	rBV	843379	1190322	17.29%	2.132%
35	15.810	2123	2129	2134	rVB3	22443	35448	0.51%	0.063%
36	16.251	2198	2204	2211	rBV3	8043	20694	0.30%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007660.D
 Acq On : 26 Oct 2021 02:10
 Operator : CG/JU
 Sample : M4304-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P063-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.363	2219	2223	2226	rVB5	5268	7372	0.11%	0.013%
38	16.463	2235	2240	2244	rBV7	3447	7713	0.11%	0.014%
39	16.516	2246	2249	2254	rVB7	4638	6977	0.10%	0.012%
40	17.010	2328	2333	2339	rVB10	6154	10225	0.15%	0.018%
41	17.115	2345	2351	2354	rBV3	9960	18044	0.26%	0.032%
42	17.327	2380	2387	2394	rBV	1879347	2751183	39.97%	4.928%
43	17.427	2397	2404	2418	rBV2	3638211	5143623	74.72%	9.213%
44	18.010	2498	2503	2508	rBV3	21663	30401	0.44%	0.054%
45	18.221	2534	2539	2545	rBV3	41992	69357	1.01%	0.124%
46	18.527	2587	2591	2596	rBV8	5870	10397	0.15%	0.019%
47	19.239	2707	2712	2717	rBV3	53580	77417	1.12%	0.139%
48	19.304	2719	2723	2731	rVV	57894	77356	1.12%	0.139%
49	19.451	2746	2748	2751	rBV4	9119	7818	0.11%	0.014%
50	19.598	2770	2773	2776	rBV5	14948	22353	0.32%	0.040%
51	19.662	2778	2784	2796	rVV	4632665	6302530	91.55%	11.289%
52	21.133	3030	3034	3040	rBV3	140984	241778	3.51%	0.433%
53	21.192	3041	3044	3049	rVV	117643	141600	2.06%	0.254%
54	21.415	3076	3082	3089	rBV	2596134	3455456	50.20%	6.189%
55	23.703	3463	3471	3480	rBV2	3469093	6883952	100.00%	12.331%
56	23.856	3490	3497	3510	rVB2	1735249	3628047	52.70%	6.499%


Sum of corrected areas: 55828640

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007660.D
Acq On : 26 Oct 2021 02:10
Operator : CG/JU
Sample : M4304-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P063-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

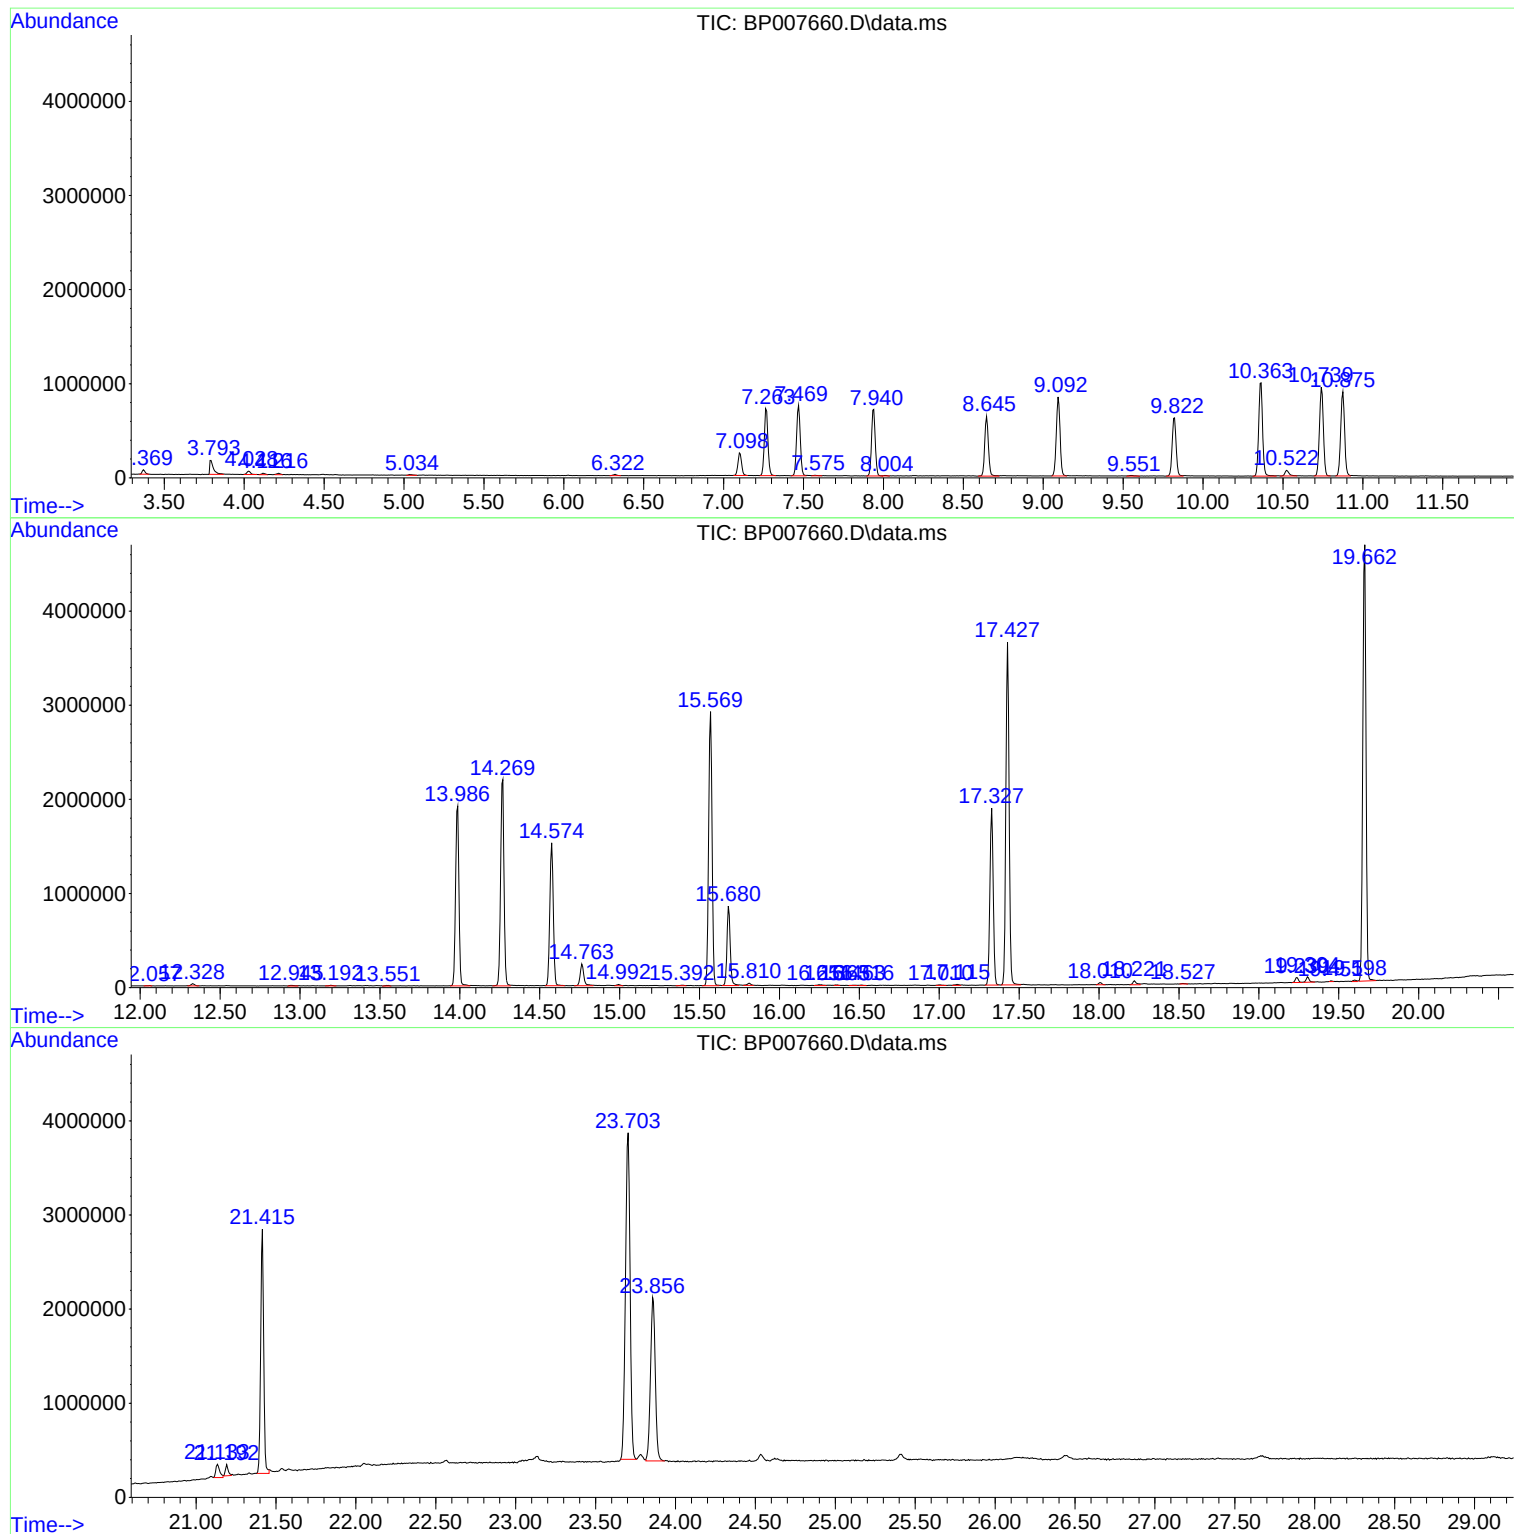

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007660.D
Acq On : 26 Oct 2021 02:10
Operator : CG/JU
Sample : M4304-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P063-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007660.D
Acq On : 26 Oct 2021 02:10
Operator : CG/JU
Sample : M4304-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P063-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
