

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007661.D
 Acq On : 26 Oct 2021 02:44
 Operator : CG/JU
 Sample : M4304-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P060-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rBV	52427	63298	0.86%	0.112%
2	3.793	84	86	97	rBV	86582	143994	1.95%	0.254%
3	4.028	121	126	130	rBV	29135	42028	0.57%	0.074%
4	4.122	137	142	147	rBV2	13383	21456	0.29%	0.038%
5	4.217	153	158	166	rVB4	13426	21399	0.29%	0.038%
6	5.052	294	300	308	rVB6	9026	20483	0.28%	0.036%
7	6.322	509	516	522	rBV	11561	19261	0.26%	0.034%
8	7.099	642	648	659	rVB	211071	340009	4.59%	0.600%
9	7.263	669	676	688	rVB	736313	1159836	15.67%	2.045%
10	7.469	703	711	723	rBV	755111	1181523	15.96%	2.083%
11	7.934	783	790	798	rBV	699632	1113957	15.05%	1.964%
12	8.646	904	911	921	rBV	593354	935169	12.63%	1.649%
13	9.093	979	987	997	rBV	879442	1412099	19.07%	2.490%
14	9.816	1101	1110	1128	rBV	660783	1087304	14.69%	1.917%
15	10.357	1195	1202	1215	rBV	1024001	1685072	22.76%	2.971%
16	10.528	1224	1231	1242	rBV	30255	54426	0.74%	0.096%
17	10.740	1258	1267	1278	rBV	930867	1576986	21.30%	2.781%
18	10.875	1282	1290	1301	rBV	781983	1370397	18.51%	2.416%
19	12.328	1532	1537	1543	rBV2	21773	35847	0.48%	0.063%
20	12.946	1635	1642	1646	rBV5	7066	13421	0.18%	0.024%
21	13.187	1679	1683	1690	rVB6	5852	9177	0.12%	0.016%
22	13.551	1738	1745	1754	rVB6	5144	13945	0.19%	0.025%
23	13.981	1812	1818	1825	rBV	2002095	2879282	38.89%	5.077%
24	14.263	1858	1866	1876	rBV	2196264	3330608	44.99%	5.873%
25	14.575	1911	1919	1930	rBV	1495735	2167686	29.28%	3.822%
26	14.763	1940	1951	1965	rBV	206553	330097	4.46%	0.582%
27	14.992	1986	1990	1998	rVB10	10203	18188	0.25%	0.032%
28	15.381	2052	2056	2061	rBV7	5418	10400	0.14%	0.018%
29	15.569	2081	2088	2096	rBV	2899505	4371243	59.05%	7.708%
30	15.681	2101	2107	2121	rVV	981373	1326727	17.92%	2.339%
31	15.804	2124	2128	2136	rVB	23179	40042	0.54%	0.071%
32	16.134	2179	2184	2188	rBV8	5317	9220	0.12%	0.016%
33	16.263	2195	2206	2211	rBV	39313	70489	0.95%	0.124%
34	16.357	2219	2222	2227	rVB7	5517	8439	0.11%	0.015%
35	17.110	2346	2350	2354	rBV3	10657	18350	0.25%	0.032%
36	17.328	2380	2387	2397	rBV	1901125	2671007	36.08%	4.710%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007661.D
 Acq On : 26 Oct 2021 02:44
 Operator : CG/JU
 Sample : M4304-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P060-TW001-01

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.428	2397	2404	2416	rBV	3789890	5540040	74.83%	9.769%
38	17.710	2447	2452	2456	rBV6	7035	14498	0.20%	0.026%
39	18.010	2498	2503	2509	rBV6	18157	26995	0.36%	0.048%
40	18.222	2534	2539	2546	rBV3	38672	61935	0.84%	0.109%
41	19.233	2707	2711	2718	rBV	56829	82391	1.11%	0.145%
42	19.304	2719	2723	2731	rVB	56772	84251	1.14%	0.149%
43	19.604	2770	2774	2776	rBV5	15506	19560	0.26%	0.034%
44	19.657	2777	2783	2790	rBV	4935576	6834835	92.32%	12.052%
45	21.133	3030	3034	3039	rBV4	100862	168505	2.28%	0.297%
46	21.192	3041	3044	3050	rVV	97425	127959	1.73%	0.226%
47	21.416	3076	3082	3094	rBV	2431142	3345421	45.19%	5.899%
48	23.704	3463	3471	3479	rVB2	3620691	7403041	100.00%	13.054%
49	23.857	3490	3497	3511	rVB2	1660099	3427897	46.30%	6.045%


Sum of corrected areas: 56710193

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007661.D
Acq On : 26 Oct 2021 02:44
Operator : CG/JU
Sample : M4304-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P060-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

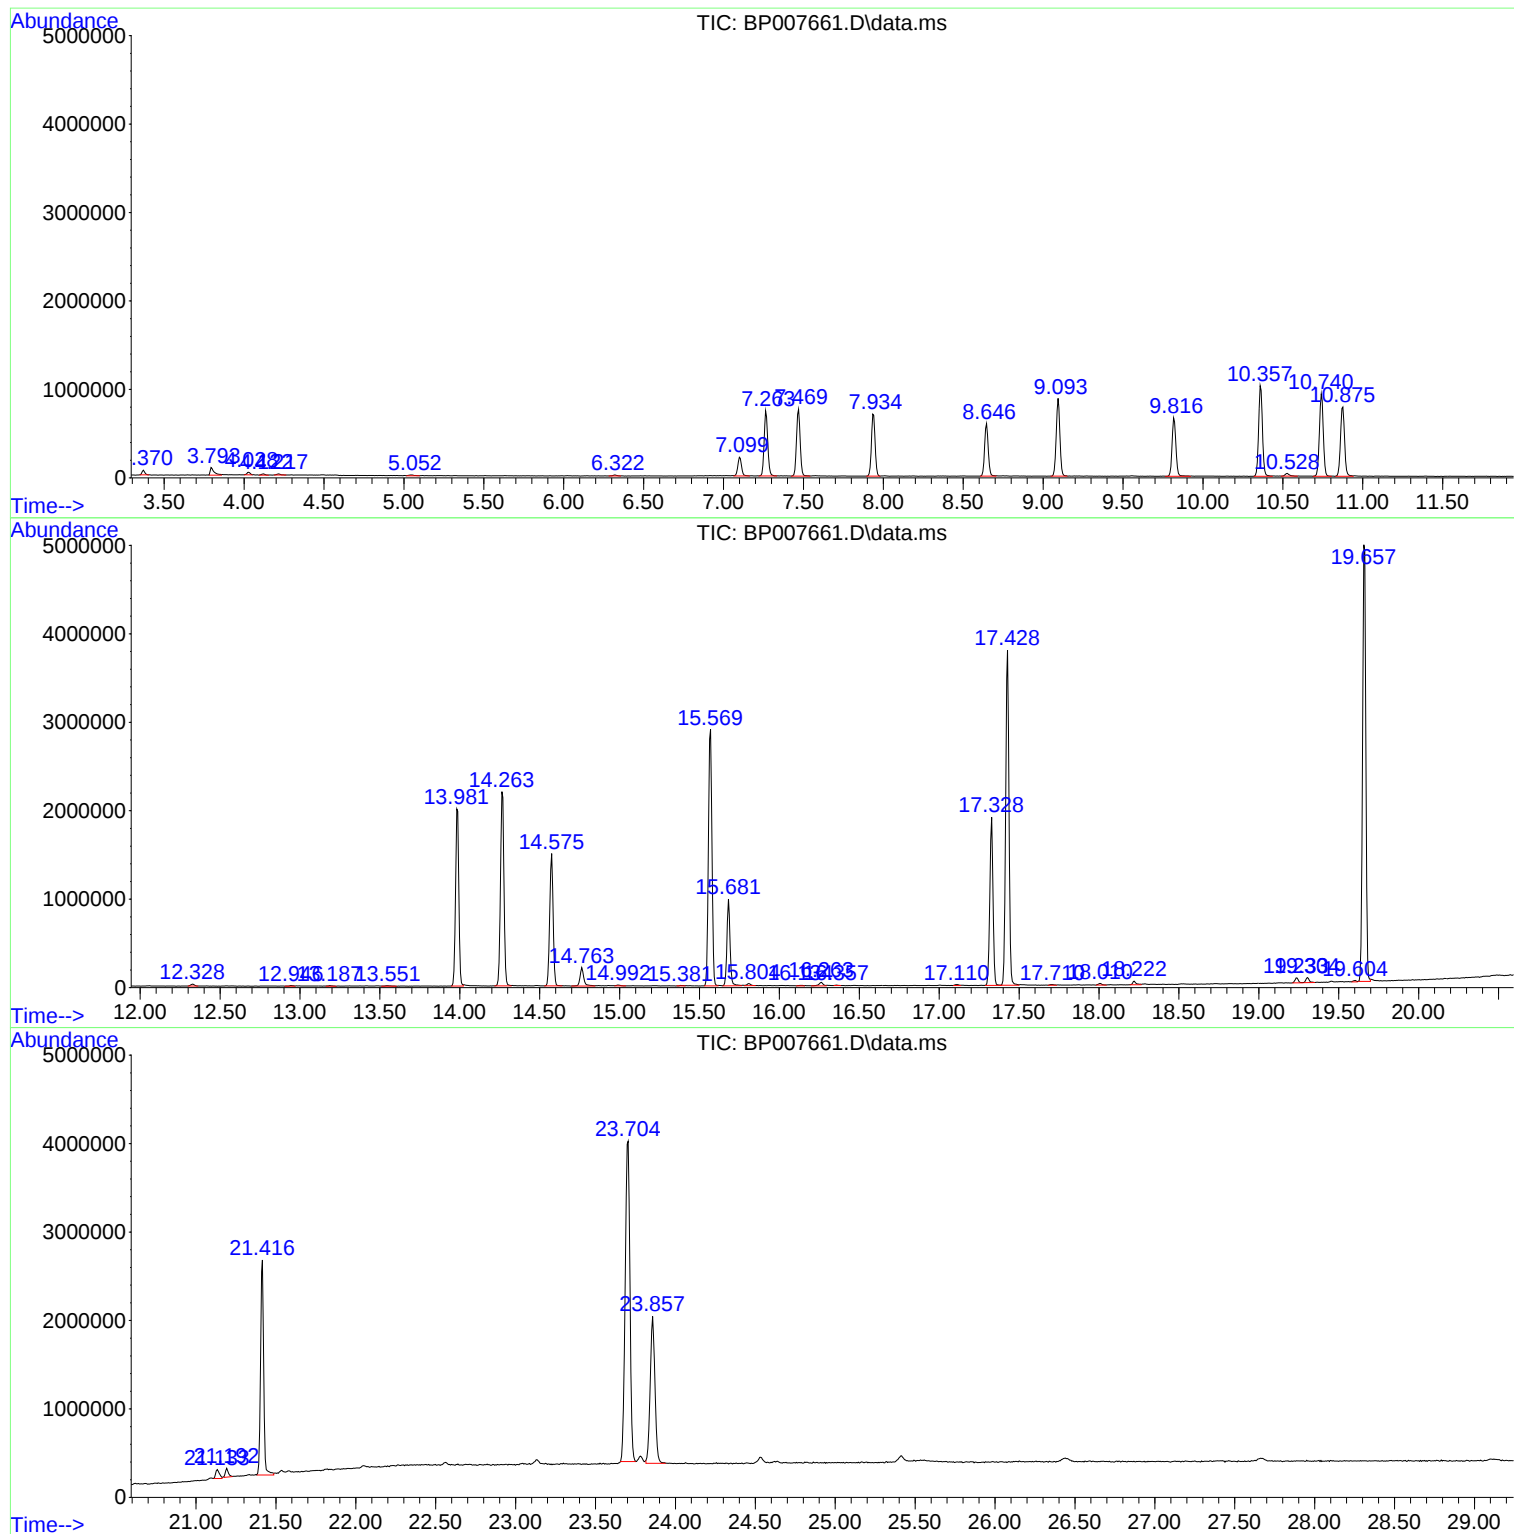

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007661.D
Acq On : 26 Oct 2021 02:44
Operator : CG/JU
Sample : M4304-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P060-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007661.D
Acq On : 26 Oct 2021 02:44
Operator : CG/JU
Sample : M4304-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P060-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
