

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007663.D
 Acq On : 26 Oct 2021 03:52
 Operator : CG/JU
 Sample : M4291-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P009-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	22	rVB	49899	61753	0.99%	0.123%
2	3.793	84	86	98	rBV	71369	117697	1.90%	0.235%
3	4.028	121	126	131	rVB	32433	49838	0.80%	0.100%
4	4.117	137	141	147	rVB	22522	32945	0.53%	0.066%
5	4.217	154	158	162	rVB4	13277	19670	0.32%	0.039%
6	4.487	202	204	209	rVB5	4990	6479	0.10%	0.013%
7	5.040	295	298	302	rVB2	5779	8577	0.14%	0.017%
8	6.322	509	516	523	rBV4	12838	23656	0.38%	0.047%
9	6.946	618	622	628	rVB6	5147	9068	0.15%	0.018%
10	7.099	642	648	658	rVB	190204	298151	4.80%	0.596%
11	7.264	669	676	690	rVB	643113	1024085	16.49%	2.048%
12	7.469	703	711	722	rBV	646361	1036284	16.69%	2.072%
13	7.575	722	729	735	rVB	4574	11288	0.18%	0.023%
14	7.934	784	790	799	rBV	660256	1067306	17.19%	2.134%
15	8.187	828	833	837	rBV6	8263	12741	0.21%	0.025%
16	8.499	882	886	889	rVB5	5361	7815	0.13%	0.016%
17	8.646	902	911	921	rBV	516118	845458	13.62%	1.691%
18	9.093	980	987	995	rBV	748765	1216371	19.59%	2.432%
19	9.552	1060	1065	1068	rBV7	3982	7429	0.12%	0.015%
20	9.816	1103	1110	1124	rBV	558996	935900	15.07%	1.872%
21	10.358	1193	1202	1215	rBV	891029	1495317	24.08%	2.990%
22	10.528	1226	1231	1238	rBV5	10117	18146	0.29%	0.036%
23	10.740	1254	1267	1276	rBV	894418	1505191	24.24%	3.010%
24	10.875	1280	1290	1304	rBV	669377	1172915	18.89%	2.346%
25	12.246	1516	1523	1527	rBV10	3660	6303	0.10%	0.013%
26	12.328	1527	1537	1541	rBV2	18821	34785	0.56%	0.070%
27	12.363	1541	1543	1547	rVB3	6188	7608	0.12%	0.015%
28	13.416	1717	1722	1726	rVV8	5871	8955	0.14%	0.018%
29	13.546	1738	1744	1750	rBV8	4908	7899	0.13%	0.016%
30	13.893	1796	1803	1808	rBV10	3668	6625	0.11%	0.013%
31	13.981	1810	1818	1825	rBV	1785056	2525364	40.68%	5.050%
32	14.116	1837	1841	1846	rVB8	4891	7029	0.11%	0.014%
33	14.263	1857	1866	1876	rBV	1964370	2898215	46.68%	5.796%
34	14.487	1900	1904	1909	rVB7	6428	8480	0.14%	0.017%
35	14.575	1909	1919	1931	rBV	1420546	2138801	34.45%	4.277%
36	14.763	1945	1951	1966	rBV	165421	275929	4.44%	0.552%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007663.D
 Acq On : 26 Oct 2021 03:52
 Operator : CG/JU
 Sample : M4291-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P009-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.993	1983	1990	1996	rVB	12592	24202	0.39%	0.048%
38	15.387	2055	2057	2062	rVB5	8030	10810	0.17%	0.022%
39	15.569	2079	2088	2100	rBV	2652457	3876146	62.43%	7.751%
40	15.681	2101	2107	2116	rBV	775635	1052615	16.95%	2.105%
41	15.810	2123	2129	2133	rBV2	19860	32583	0.52%	0.065%
42	16.145	2178	2186	2189	rBV10	5287	11009	0.18%	0.022%
43	16.251	2195	2204	2210	rBV10	7704	23970	0.39%	0.048%
44	16.328	2214	2217	2223	rVB7	6146	11919	0.19%	0.024%
45	16.857	2303	2307	2309	rBV4	5495	7466	0.12%	0.015%
46	17.110	2347	2350	2354	rBV3	9282	14768	0.24%	0.030%
47	17.157	2356	2358	2367	rVB10	8662	11456	0.18%	0.023%
48	17.328	2380	2387	2397	rBV	1786037	2616394	42.14%	5.232%
49	17.428	2397	2404	2416	rBV	3214147	4613812	74.31%	9.226%
50	18.004	2499	2502	2506	rVB6	7720	10285	0.17%	0.021%
51	18.222	2535	2539	2546	rBV4	42650	64123	1.03%	0.128%
52	19.234	2708	2711	2717	rVB2	45833	64569	1.04%	0.129%
53	19.304	2719	2723	2727	rBV	50816	69594	1.12%	0.139%
54	19.451	2745	2748	2753	rBV5	21407	30019	0.48%	0.060%
55	19.663	2777	2784	2794	rBV	4039161	5720509	92.14%	11.440%
56	21.192	3041	3044	3049	rBV	75306	88389	1.42%	0.177%
57	21.416	3077	3082	3087	rBV	2515465	3170543	51.07%	6.340%
58	23.704	3463	3471	3480	rBV2	2928350	6208537	100.00%	12.416%
59	23.857	3490	3497	3508	rVB2	1645429	3362361	54.16%	6.724%




Sum of corrected areas: 50006152

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007663.D
Acq On : 26 Oct 2021 03:52
Operator : CG/JU
Sample : M4291-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P009-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

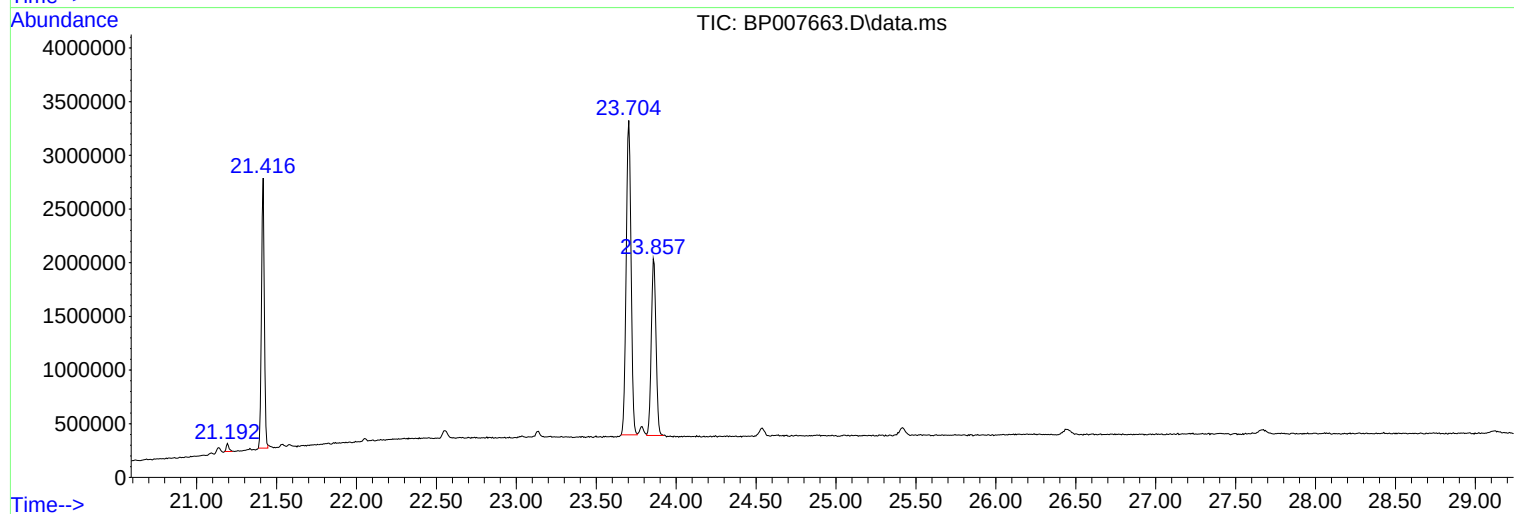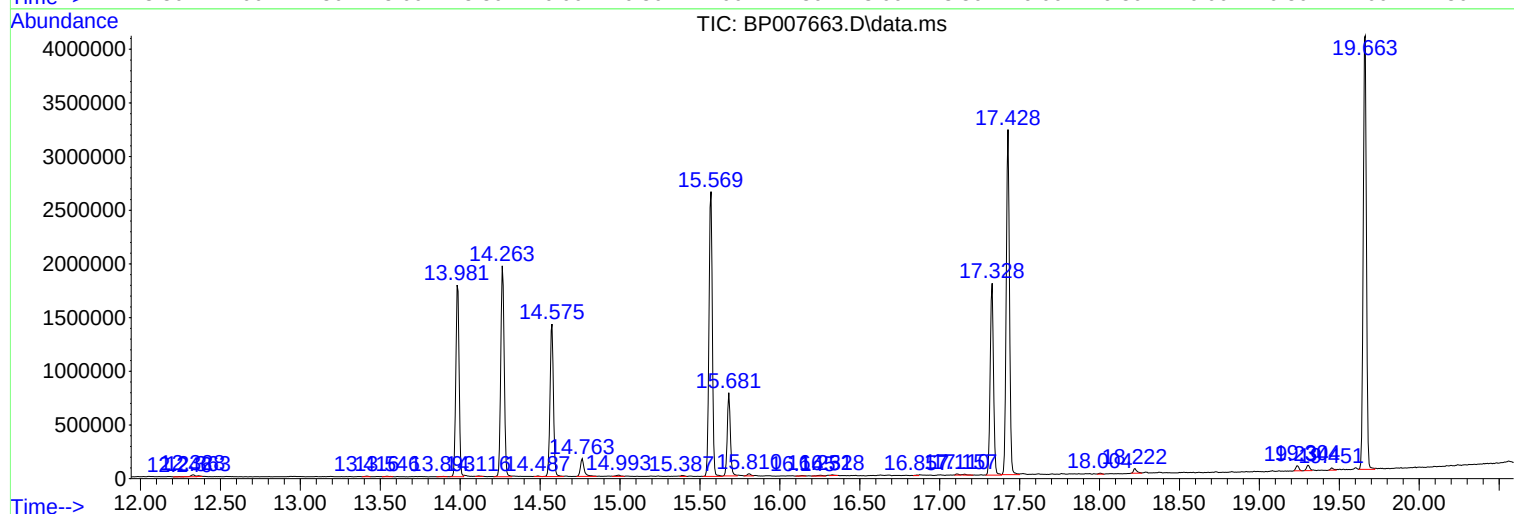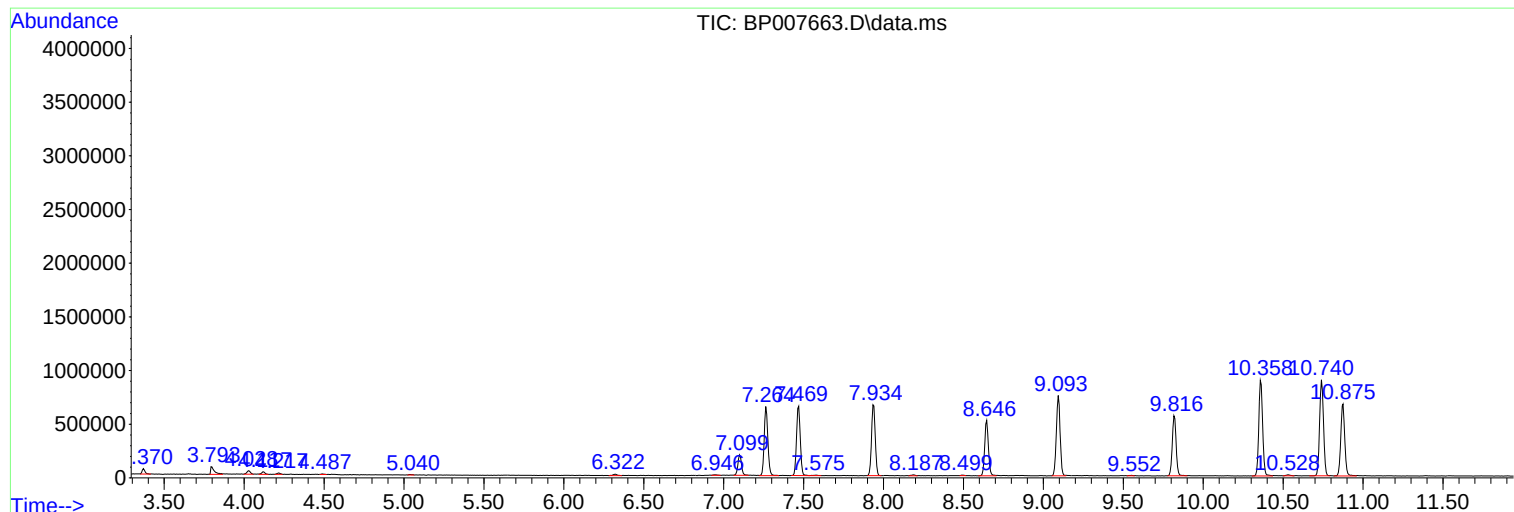

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007663.D
Acq On : 26 Oct 2021 03:52
Operator : CG/JU
Sample : M4291-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P009-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007663.D
Acq On : 26 Oct 2021 03:52
Operator : CG/JU
Sample : M4291-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P009-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
