

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007664.D
 Acq On : 26 Oct 2021 04:26
 Operator : CG/JU
 Sample : M4291-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P011-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	22	rVB	52602	69189	1.15%	0.136%
2	3.787	83	85	101	rBV	245900	388325	6.46%	0.765%
3	4.028	121	126	132	rBV	32153	46438	0.77%	0.091%
4	4.117	137	141	148	rVB	18188	26878	0.45%	0.053%
5	4.217	154	158	162	rVB3	11819	16463	0.27%	0.032%
6	5.046	294	299	302	rVB3	6603	10079	0.17%	0.020%
7	6.317	510	515	522	rVB5	12795	24472	0.41%	0.048%
8	6.952	615	623	626	rBV9	4881	9408	0.16%	0.019%
9	7.099	641	648	657	rVB	221221	347623	5.78%	0.685%
10	7.264	670	676	688	rBV	593197	934896	15.56%	1.841%
11	7.469	703	711	723	rBV	642169	1005670	16.74%	1.981%
12	7.569	725	728	732	rVB6	5013	6788	0.11%	0.013%
13	7.934	782	790	798	rBV	742947	1189545	19.80%	2.343%
14	8.011	798	803	809	rVB6	5346	11819	0.20%	0.023%
15	8.181	828	832	838	rBV6	7341	11803	0.20%	0.023%
16	8.487	880	884	890	rBV8	5873	12094	0.20%	0.024%
17	8.646	903	911	924	rBV	535110	887470	14.77%	1.748%
18	9.093	977	987	996	rBV	690377	1123524	18.70%	2.213%
19	9.228	1005	1010	1015	rBV	27432	42479	0.71%	0.084%
20	9.558	1057	1066	1070	rBV9	5163	10236	0.17%	0.020%
21	9.816	1103	1110	1121	rBV	523197	865128	14.40%	1.704%
22	10.358	1195	1202	1215	rBV	840518	1404444	23.37%	2.766%
23	10.528	1224	1231	1242	rBV2	24825	53471	0.89%	0.105%
24	10.740	1258	1267	1281	rVB	995311	1673154	27.84%	3.296%
25	10.869	1281	1289	1303	rBV	807052	1406585	23.41%	2.771%
26	12.328	1531	1537	1543	rBV3	19111	32970	0.55%	0.065%
27	12.546	1569	1574	1580	rBV10	3606	7410	0.12%	0.015%
28	12.946	1637	1642	1646	rBV7	5764	10506	0.17%	0.021%
29	13.193	1677	1684	1689	rBV10	5959	10693	0.18%	0.021%
30	13.487	1727	1734	1738	rBV4	17228	27118	0.45%	0.053%
31	13.546	1740	1744	1747	rVB6	4120	6318	0.11%	0.012%
32	13.981	1812	1818	1833	rVV	1654371	2312286	38.48%	4.554%
33	14.263	1856	1866	1883	rBV	1789122	2668899	44.41%	5.257%
34	14.575	1909	1919	1932	rBV	1581166	2361957	39.31%	4.652%
35	14.763	1945	1951	1962	rBV	203401	315633	5.25%	0.622%
36	14.993	1984	1990	1996	rBV10	10114	17140	0.29%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007664.D
 Acq On : 26 Oct 2021 04:26
 Operator : CG/JU
 Sample : M4291-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P011-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.387	2053	2057	2063	rBV6	5752	12059	0.20%	0.024%
38	15.569	2079	2088	2101	rBV	2471011	3587113	59.69%	7.065%
39	15.681	2101	2107	2118	rBV	732879	1008047	16.77%	1.986%
40	15.804	2125	2128	2137	rVB2	20330	32179	0.54%	0.063%
41	16.263	2200	2206	2211	rBV10	7303	14532	0.24%	0.029%
42	17.110	2345	2350	2354	rBV2	11011	16899	0.28%	0.033%
43	17.328	2380	2387	2397	rBV	2102599	2914291	48.50%	5.740%
44	17.428	2397	2404	2416	rVV	3078855	4451488	74.08%	8.768%
45	17.522	2416	2420	2425	rVB7	21811	31263	0.52%	0.062%
46	17.645	2438	2441	2447	rVB8	4304	8733	0.15%	0.017%
47	17.704	2447	2451	2453	rBV4	5457	7487	0.12%	0.015%
48	18.004	2498	2502	2506	rBV5	19657	26670	0.44%	0.053%
49	18.222	2534	2539	2545	rBV3	43321	66043	1.10%	0.130%
50	18.669	2613	2615	2621	rBV6	4521	9631	0.16%	0.019%
51	19.239	2708	2712	2718	rBV	43957	62508	1.04%	0.123%
52	19.304	2719	2723	2727	rBV	50562	63468	1.06%	0.125%
53	19.451	2746	2748	2756	rBV8	11917	17716	0.29%	0.035%
54	19.598	2771	2773	2777	rVB5	12253	14673	0.24%	0.029%
55	19.663	2777	2784	2796	rBV	3999866	5566419	92.63%	10.964%
56	21.133	3031	3034	3040	rBV4	64515	109661	1.82%	0.216%
57	21.192	3041	3044	3051	rVV	70128	104668	1.74%	0.206%
58	21.416	3077	3082	3094	rBV	2623081	3562805	59.29%	7.018%
59	23.704	3463	3471	3480	rBV2	2949009	6009227	100.00%	11.836%
60	23.863	3491	3498	3508	rVB2	1782047	3723416	61.96%	7.334%


Sum of corrected areas: 50769907

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007664.D
Acq On : 26 Oct 2021 04:26
Operator : CG/JU
Sample : M4291-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P011-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

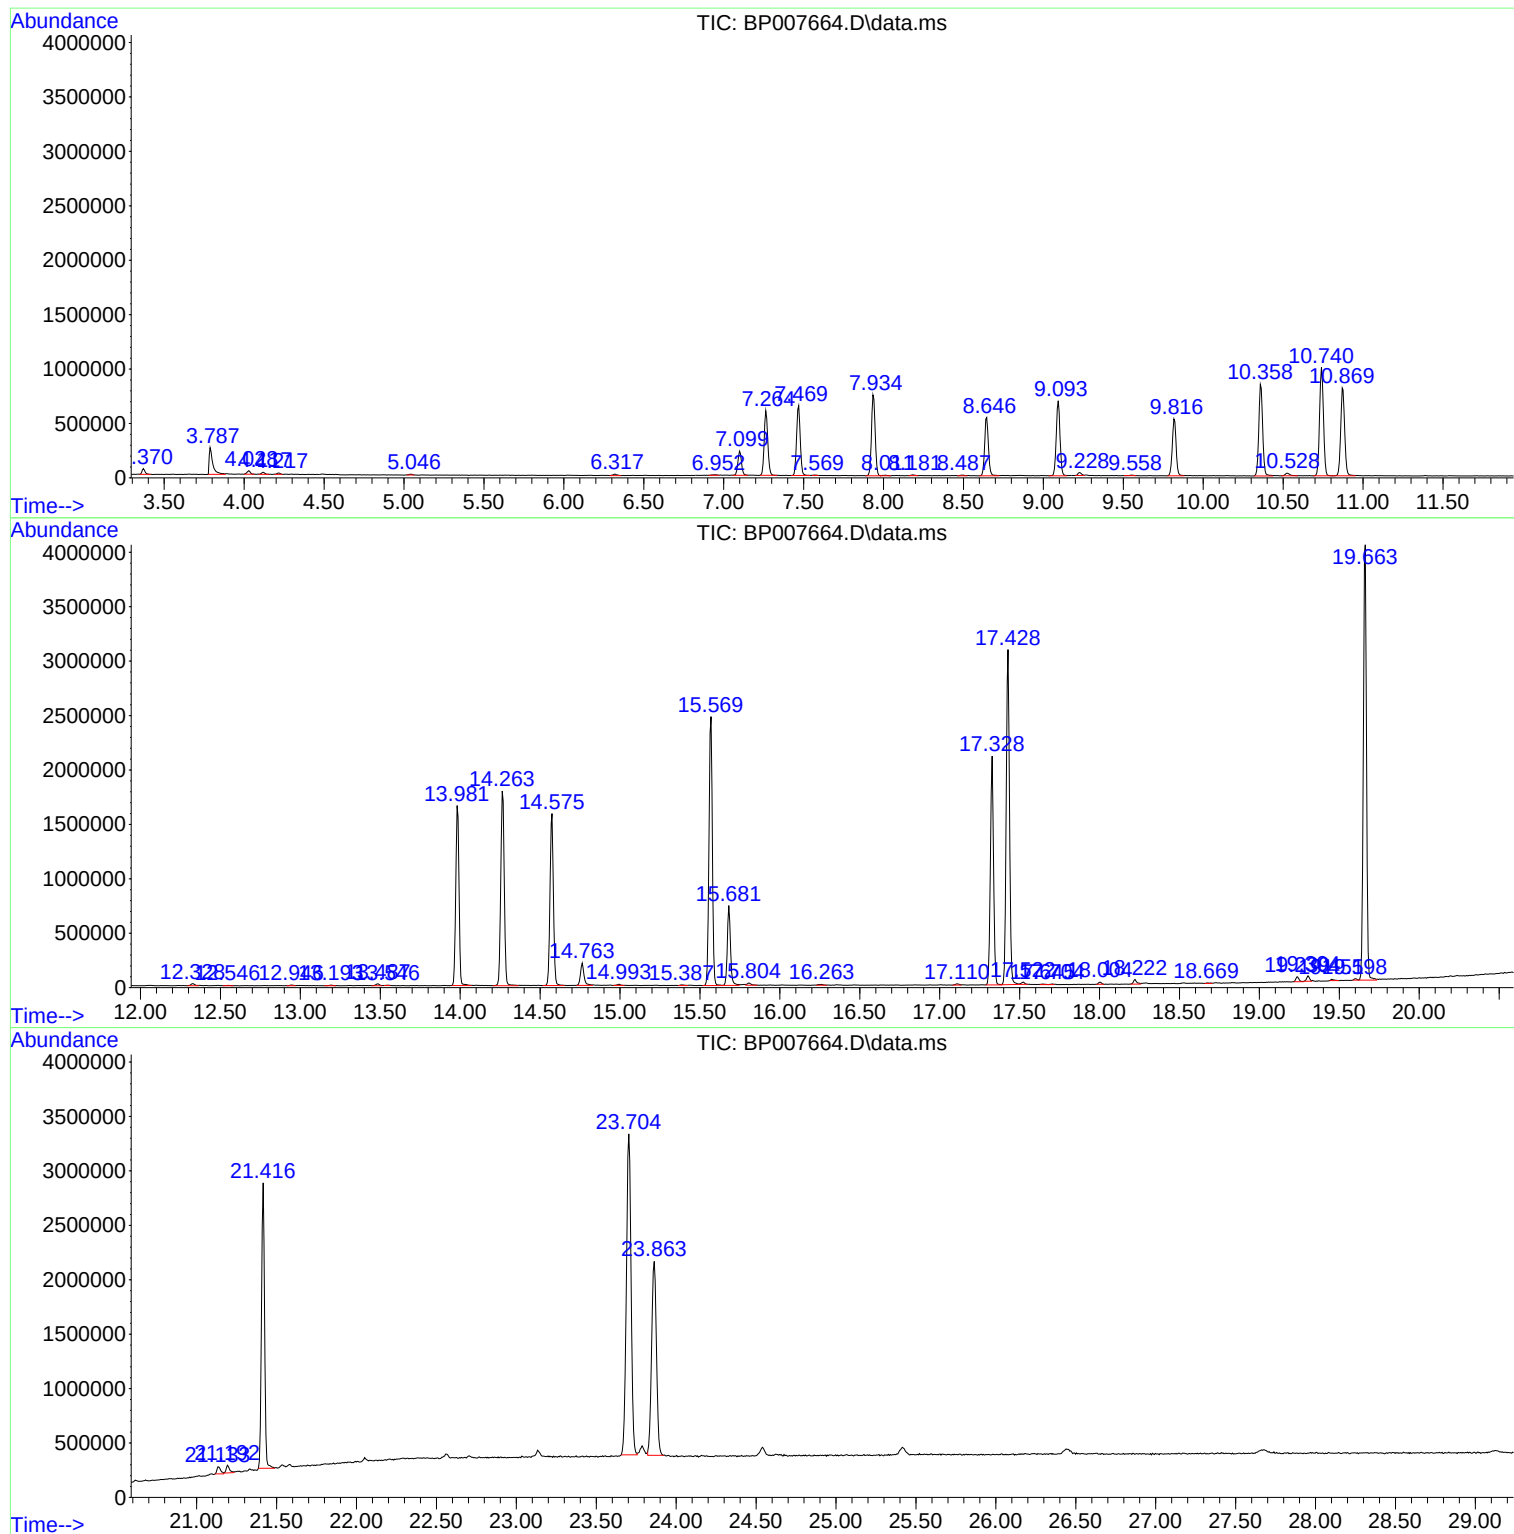

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007664.D
Acq On : 26 Oct 2021 04:26
Operator : CG/JU
Sample : M4291-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P011-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007664.D
Acq On : 26 Oct 2021 04:26
Operator : CG/JU
Sample : M4291-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P011-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
