

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007665.D
 Acq On : 26 Oct 2021 05:00
 Operator : CG/JU
 Sample : M4291-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P022-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	20	rVB	39738	50510	0.91%	0.109%
2	3.793	84	86	95	rBV	87583	140022	2.52%	0.301%
3	3.987	116	119	121	rBV4	5140	6458	0.12%	0.014%
4	4.028	122	126	133	rVB2	29380	45742	0.82%	0.098%
5	4.117	138	141	145	rVB2	12499	15610	0.28%	0.034%
6	4.217	154	158	166	rVB6	13615	22917	0.41%	0.049%
7	5.040	295	298	302	rVB3	7351	10781	0.19%	0.023%
8	6.317	510	515	520	rBV5	10847	19344	0.35%	0.042%
9	6.946	616	622	625	rBV7	6932	14313	0.26%	0.031%
10	7.099	641	648	657	rBV	193670	307161	5.54%	0.661%
11	7.264	670	676	685	rBV	578513	916672	16.52%	1.974%
12	7.469	704	711	723	rVV	601832	982850	17.71%	2.116%
13	7.575	724	729	732	rVB7	4907	7201	0.13%	0.016%
14	7.934	783	790	798	rVB	626461	996664	17.96%	2.146%
15	8.181	826	832	839	rBV3	8938	17400	0.31%	0.037%
16	8.493	881	885	889	rBV6	6639	9789	0.18%	0.021%
17	8.646	902	911	925	rBV	513352	835502	15.06%	1.799%
18	9.093	980	987	996	rBV	680687	1099522	19.81%	2.367%
19	9.558	1062	1066	1071	rVB4	6326	10491	0.19%	0.023%
20	9.816	1103	1110	1118	rBV	504920	831395	14.98%	1.790%
21	10.358	1193	1202	1219	rBV	820785	1384783	24.96%	2.982%
22	10.522	1225	1230	1240	rBV2	39607	72991	1.32%	0.157%
23	10.740	1260	1267	1274	rBV	854331	1405638	25.33%	3.027%
24	10.875	1281	1290	1306	rBV	642376	1136257	20.48%	2.447%
25	12.052	1486	1490	1496	rBV8	3503	6478	0.12%	0.014%
26	12.328	1529	1537	1542	rVV2	18010	31319	0.56%	0.067%
27	12.946	1637	1642	1646	rBV8	3643	7363	0.13%	0.016%
28	13.193	1679	1684	1690	rVB10	4453	7121	0.13%	0.015%
29	13.487	1730	1734	1739	rBV8	3705	7004	0.13%	0.015%
30	13.546	1739	1744	1749	rVB7	4664	7150	0.13%	0.015%
31	13.981	1812	1818	1825	rBV	1643936	2294010	41.34%	4.939%
32	14.263	1855	1866	1874	rBV	1819542	2648911	47.74%	5.704%
33	14.575	1908	1919	1926	rBV	1330098	1967586	35.46%	4.237%
34	14.763	1945	1951	1965	rBV	166888	267799	4.83%	0.577%
35	14.993	1985	1990	1995	rBV9	10940	17395	0.31%	0.037%
36	15.393	2052	2058	2063	rBV8	6295	10313	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007665.D
 Acq On : 26 Oct 2021 05:00
 Operator : CG/JU
 Sample : M4291-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P022-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.569	2081	2088	2098	rBV	2395298	3549748	63.97%	7.643%
38	15.681	2101	2107	2120	rVV	680158	940802	16.95%	2.026%
39	15.804	2124	2128	2132	rVV2	18224	29987	0.54%	0.065%
40	15.845	2133	2135	2139	rVB5	6311	7538	0.14%	0.016%
41	16.140	2179	2185	2191	rBV5	4589	10206	0.18%	0.022%
42	16.263	2200	2206	2210	rVB8	7299	14807	0.27%	0.032%
43	16.328	2214	2217	2220	rVV3	8243	8327	0.15%	0.018%
44	16.628	2263	2268	2271	rBV7	3777	7298	0.13%	0.016%
45	16.687	2274	2278	2283	rVB8	5085	8884	0.16%	0.019%
46	17.004	2326	2332	2335	rBV7	5145	7976	0.14%	0.017%
47	17.110	2346	2350	2353	rBV3	6215	9687	0.17%	0.021%
48	17.151	2355	2357	2361	rVB5	7688	8920	0.16%	0.019%
49	17.328	2380	2387	2397	rBV	1745728	2462887	44.38%	5.303%
50	17.428	2397	2404	2417	rBV2	2826245	4152325	74.83%	8.941%
51	18.004	2498	2502	2506	rBV3	16724	22535	0.41%	0.049%
52	18.222	2531	2539	2546	rBV4	57879	109832	1.98%	0.236%
53	19.239	2708	2712	2719	rBV2	43196	64135	1.16%	0.138%
54	19.304	2719	2723	2732	rVV	47667	70035	1.26%	0.151%
55	19.457	2745	2749	2753	rBV7	19251	26159	0.47%	0.056%
56	19.598	2771	2773	2777	rVB5	15481	14288	0.26%	0.031%
57	19.657	2777	2783	2790	rBV	3772910	5164026	93.06%	11.119%
58	20.563	2934	2937	2942	rVB3	52692	54959	0.99%	0.118%
59	21.133	3030	3034	3040	rBV2	132335	215894	3.89%	0.465%
60	21.192	3041	3044	3051	rVB	70872	101006	1.82%	0.217%
61	21.416	3076	3082	3087	rBV	2229723	3041278	54.81%	6.548%
62	23.698	3463	3470	3480	rVB2	2716984	5548993	100.00%	11.948%
63	23.857	3490	3497	3509	rVB2	1544852	3177998	57.27%	6.843%




Sum of corrected areas: 46442992

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007665.D
Acq On : 26 Oct 2021 05:00
Operator : CG/JU
Sample : M4291-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P022-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

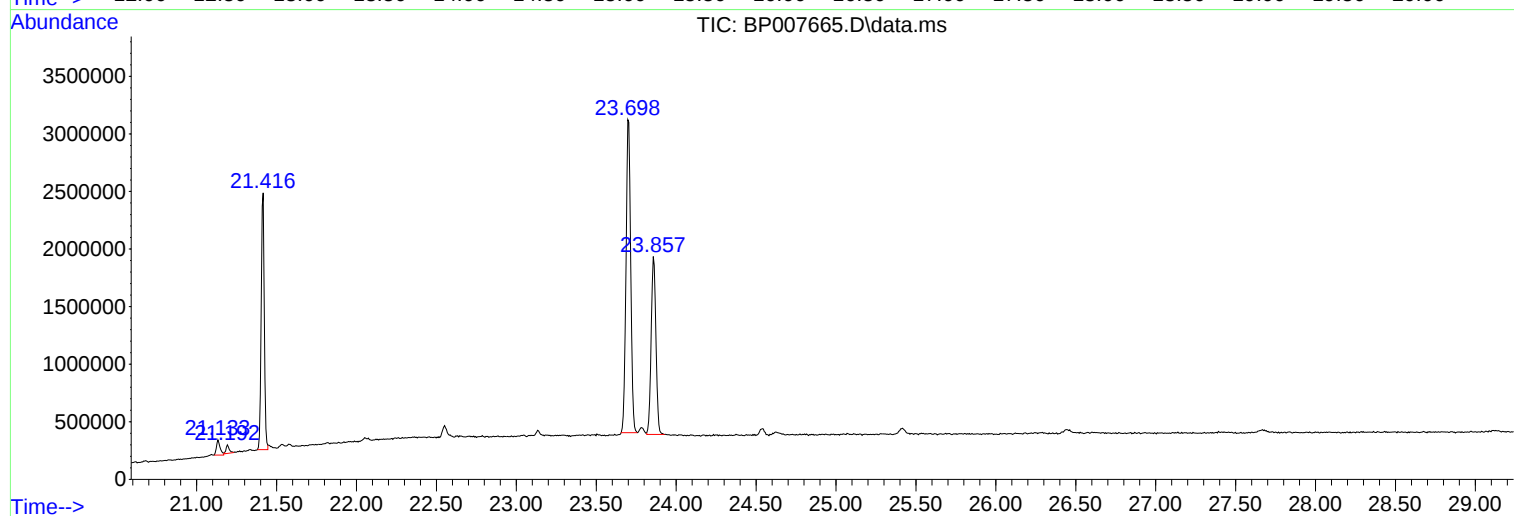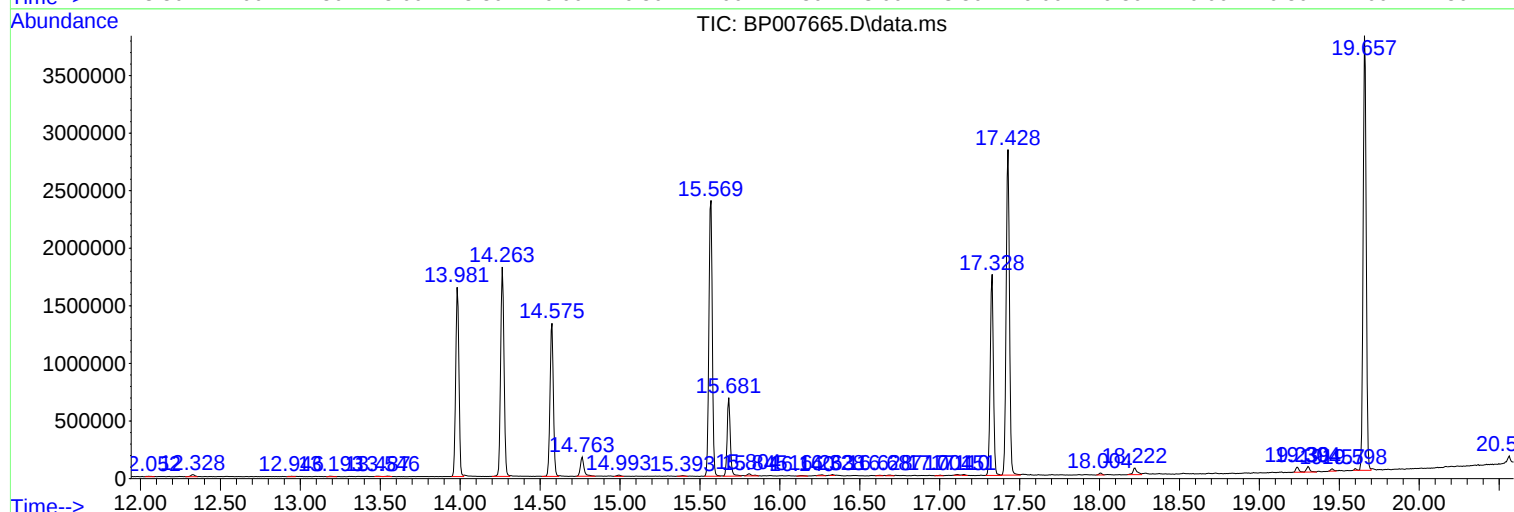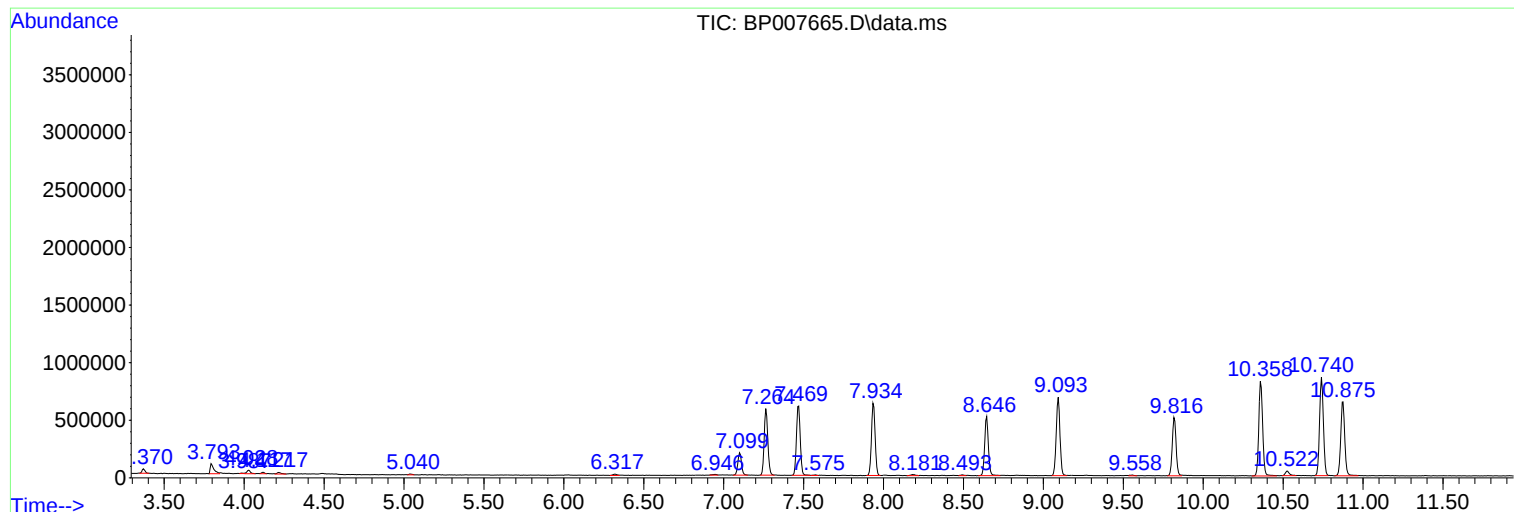

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007665.D
Acq On : 26 Oct 2021 05:00
Operator : CG/JU
Sample : M4291-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P022-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007665.D
Acq On : 26 Oct 2021 05:00
Operator : CG/JU
Sample : M4291-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P022-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
