

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007666.D
 Acq On : 26 Oct 2021 05:33
 Operator : CG/JU
 Sample : M4291-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P028-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	22	rVB	43944	61254	0.96%	0.118%
2	3.793	83	86	100	rBV	85101	140854	2.20%	0.271%
3	3.987	115	119	121	rBV4	6707	8770	0.14%	0.017%
4	4.028	121	126	132	rVB2	31486	49035	0.77%	0.094%
5	4.122	138	142	146	rVB3	13725	21899	0.34%	0.042%
6	4.216	154	158	164	rVB6	12732	21722	0.34%	0.042%
7	5.040	292	298	303	rVB3	7888	15795	0.25%	0.030%
8	6.316	511	515	521	rVB2	12702	18779	0.29%	0.036%
9	6.946	616	622	626	rBV4	6157	11677	0.18%	0.022%
10	7.099	642	648	657	rVB	195636	309544	4.84%	0.596%
11	7.263	669	676	687	rBV	633670	996271	15.59%	1.917%
12	7.469	704	711	722	rVB	634843	1026714	16.06%	1.976%
13	7.569	722	728	731	rBV8	4620	8407	0.13%	0.016%
14	7.934	783	790	798	rBV	699779	1095885	17.14%	2.109%
15	8.010	798	803	807	rVB7	5181	7783	0.12%	0.015%
16	8.187	827	833	838	rBV5	10308	19188	0.30%	0.037%
17	8.493	881	885	888	rBV3	5838	9218	0.14%	0.018%
18	8.646	903	911	924	rBV	520711	857841	13.42%	1.651%
19	9.093	978	987	995	rBV	726395	1195256	18.70%	2.300%
20	9.557	1063	1066	1070	rVB5	7370	8266	0.13%	0.016%
21	9.816	1102	1110	1123	rBV	557716	931837	14.58%	1.793%
22	10.357	1194	1202	1217	rBV	892518	1496351	23.41%	2.880%
23	10.522	1224	1230	1242	rBV	84651	154993	2.42%	0.298%
24	10.740	1259	1267	1276	rBV	929037	1567475	24.52%	3.017%
25	10.875	1281	1290	1300	rBV	672994	1166514	18.25%	2.245%
26	12.328	1530	1537	1541	rBV2	19347	34937	0.55%	0.067%
27	13.187	1680	1683	1689	rVB7	5092	7674	0.12%	0.015%
28	13.487	1727	1734	1737	rBV7	5768	8676	0.14%	0.017%
29	13.545	1739	1744	1750	rBV8	5955	9789	0.15%	0.019%
30	13.981	1809	1818	1824	rBV	1716018	2474036	38.70%	4.762%
31	14.263	1855	1866	1878	rBV	1946814	2898019	45.34%	5.578%
32	14.575	1911	1919	1929	rBV	1453626	2214332	34.64%	4.262%
33	14.763	1942	1951	1969	rBV	181127	312934	4.90%	0.602%
34	14.992	1985	1990	1995	rBV3	24929	36933	0.58%	0.071%
35	15.392	2052	2058	2063	rVB7	6470	11060	0.17%	0.021%
36	15.569	2081	2088	2100	rBV	2565317	3926388	61.43%	7.557%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007666.D
 Acq On : 26 Oct 2021 05:33
 Operator : CG/JU
 Sample : M4291-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P028-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.681	2100	2107	2123	rBV	821860	1109963	17.36%	2.136%
38	15.810	2123	2129	2135	rVB	18755	31132	0.49%	0.060%
39	16.263	2199	2206	2210	rBV8	8858	18408	0.29%	0.035%
40	16.363	2218	2223	2226	rVB7	5328	8773	0.14%	0.017%
41	17.110	2346	2350	2353	rBV3	9253	14202	0.22%	0.027%
42	17.139	2353	2355	2363	rVB8	5470	8618	0.13%	0.017%
43	17.328	2380	2387	2395	rBV	1922943	2756824	43.13%	5.306%
44	17.428	2397	2404	2415	rBV2	3344153	4818705	75.39%	9.274%
45	17.628	2434	2438	2442	rBV7	5521	9436	0.15%	0.018%
46	17.704	2447	2451	2453	rBV5	5768	7528	0.12%	0.014%
47	18.004	2497	2502	2507	rBV3	28010	42724	0.67%	0.082%
48	18.222	2535	2539	2546	rBV3	37165	58461	0.91%	0.113%
49	19.239	2707	2712	2716	rBV	56739	77666	1.22%	0.149%
50	19.304	2719	2723	2730	rVB2	51341	75757	1.19%	0.146%
51	19.604	2771	2774	2777	rBV4	19035	21430	0.34%	0.041%
52	19.663	2778	2784	2790	rBV	4258513	5923150	92.66%	11.400%
53	21.133	3031	3034	3040	rBV4	118558	176540	2.76%	0.340%
54	21.192	3042	3044	3050	rVB	69676	84860	1.33%	0.163%
55	21.416	3077	3082	3088	rBV	2552628	3349102	52.39%	6.446%
56	22.551	3271	3275	3283	rBV5	141246	266440	4.17%	0.513%
57	23.704	3463	3471	3480	rBV2	3206409	6392100	100.00%	12.302%
58	23.863	3491	3498	3509	rVB2	1679658	3570799	55.86%	6.872%




Sum of corrected areas: 51958724

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007666.D
Acq On : 26 Oct 2021 05:33
Operator : CG/JU
Sample : M4291-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P028-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

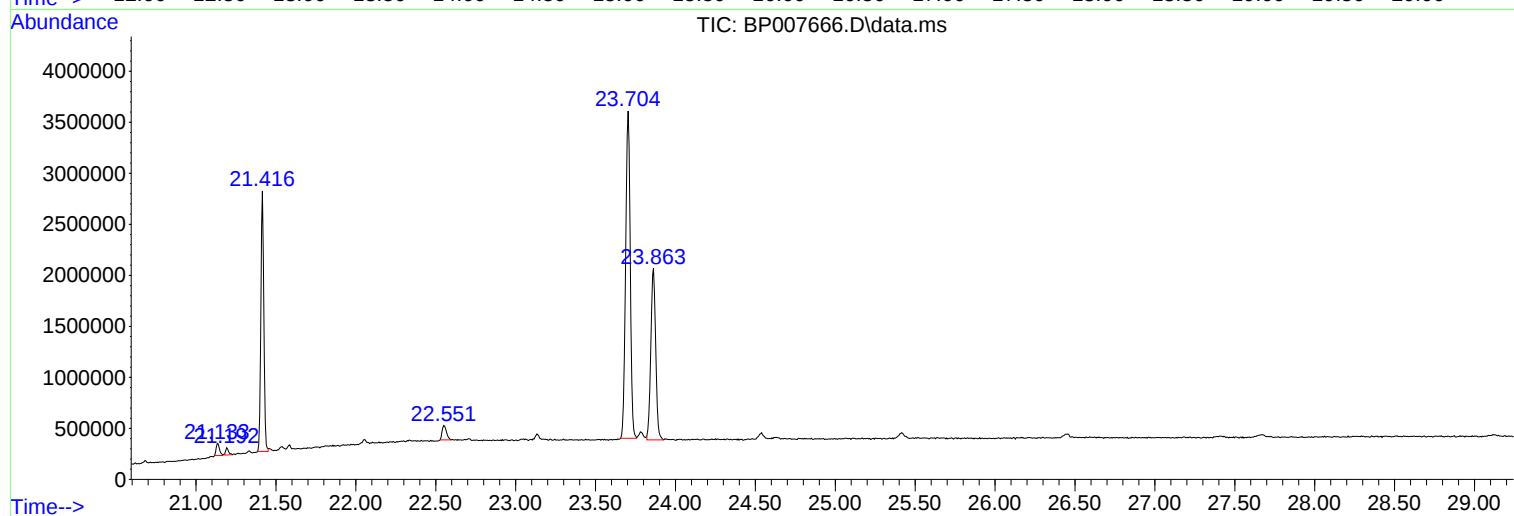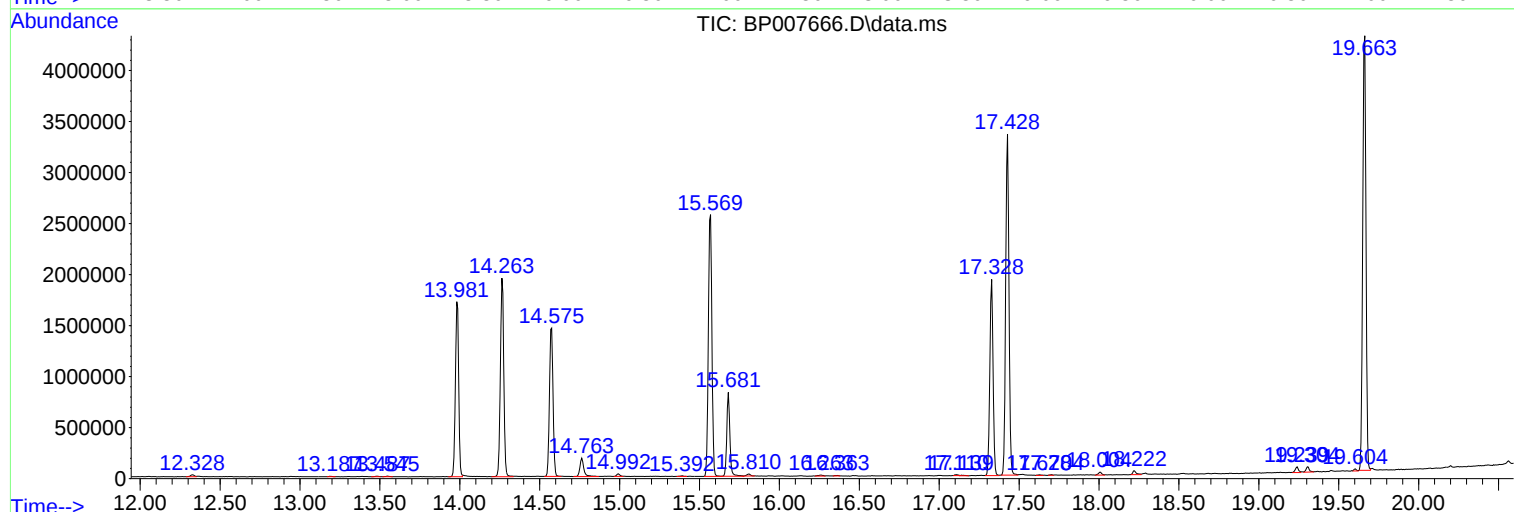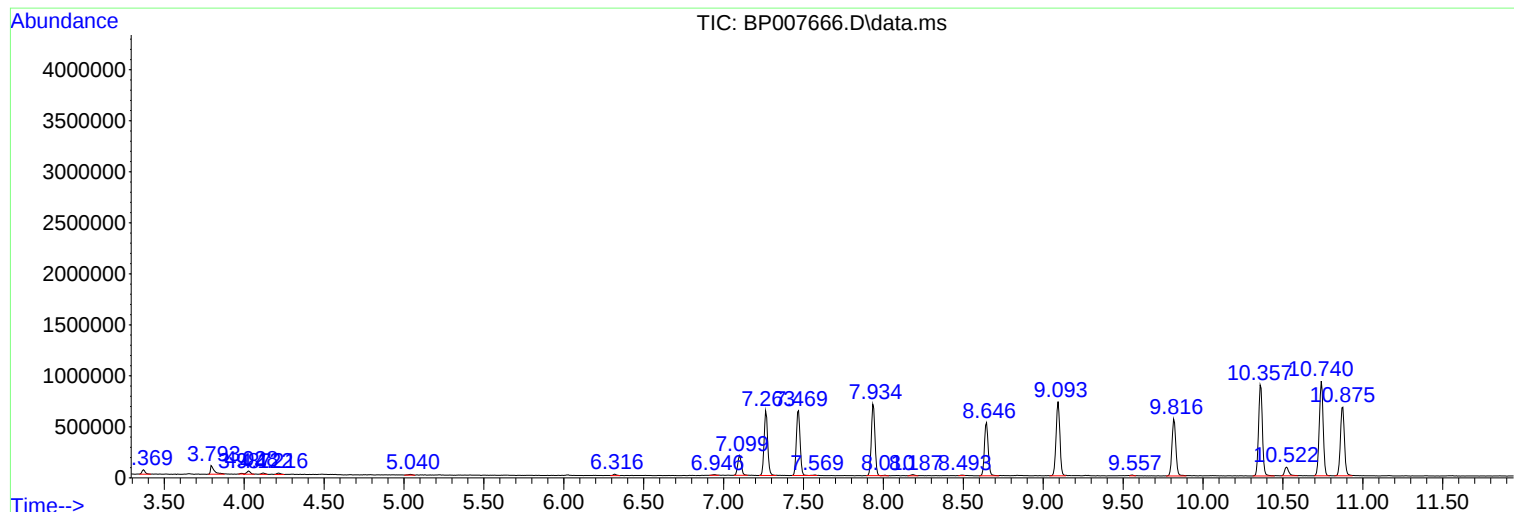

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007666.D
Acq On : 26 Oct 2021 05:33
Operator : CG/JU
Sample : M4291-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P028-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007666.D
Acq On : 26 Oct 2021 05:33
Operator : CG/JU
Sample : M4291-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P028-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------