

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007667.D
 Acq On : 26 Oct 2021 06:07
 Operator : CG/JU
 Sample : M4291-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P029-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	11	14	23	rVB	48809	62194	0.99%	0.114%
2	3.652	59	62	70	rVB3	7892	12645	0.20%	0.023%
3	3.793	83	86	98	rBV	147739	233219	3.70%	0.427%
4	3.987	114	119	122	rBV2	12510	22921	0.36%	0.042%
5	4.028	122	126	131	rVB	37410	53498	0.85%	0.098%
6	4.117	138	141	145	rVB2	11962	15512	0.25%	0.028%
7	4.217	154	158	163	rVB3	14051	24264	0.38%	0.044%
8	5.046	295	299	303	rVB5	7061	11651	0.18%	0.021%
9	6.317	511	515	521	rVB	14048	20147	0.32%	0.037%
10	6.946	616	622	627	rBV6	8638	17003	0.27%	0.031%
11	7.099	640	648	657	rBV	251373	399739	6.34%	0.732%
12	7.264	669	676	691	rVB	644500	1023325	16.23%	1.873%
13	7.469	703	711	721	rBV	687878	1116275	17.70%	2.043%
14	7.934	783	790	798	rBV	732349	1168781	18.54%	2.139%
15	8.011	798	803	807	rVB7	4902	8184	0.13%	0.015%
16	8.181	825	832	843	rBV7	9546	19956	0.32%	0.037%
17	8.493	880	885	890	rBV5	7172	12736	0.20%	0.023%
18	8.646	901	911	924	rBV	612775	1022450	16.22%	1.872%
19	9.093	979	987	995	rBV	759719	1222984	19.40%	2.239%
20	9.222	1005	1009	1012	rBV6	5957	9615	0.15%	0.018%
21	9.263	1012	1016	1023	rVB10	5432	10846	0.17%	0.020%
22	9.558	1059	1066	1071	rVB10	4972	10599	0.17%	0.019%
23	9.816	1100	1110	1118	rBV	586014	962785	15.27%	1.762%
24	10.357	1194	1202	1219	rBV	953612	1585642	25.15%	2.902%
25	10.522	1223	1230	1239	rBV	137609	237613	3.77%	0.435%
26	10.740	1258	1267	1277	rBV	970815	1659608	26.32%	3.038%
27	10.869	1281	1289	1304	rBV	774372	1364896	21.65%	2.498%
28	12.046	1486	1489	1495	rVB7	4126	6676	0.11%	0.012%
29	12.328	1532	1537	1542	rBV2	18851	33358	0.53%	0.061%
30	12.946	1638	1642	1643	rBV3	6129	6669	0.11%	0.012%
31	13.193	1680	1684	1693	rVB8	7504	11009	0.17%	0.020%
32	13.481	1728	1733	1739	rBV7	8848	17263	0.27%	0.032%
33	13.540	1739	1743	1748	rBV8	4806	8272	0.13%	0.015%
34	13.981	1811	1818	1832	rBV	1931338	2690529	42.67%	4.925%
35	14.110	1836	1840	1846	rVB9	3721	6914	0.11%	0.013%
36	14.263	1855	1866	1879	rBV	2072861	3097825	49.13%	5.670%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007667.D
 Acq On : 26 Oct 2021 06:07
 Operator : CG/JU
 Sample : M4291-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P029-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.575	1909	1919	1932	rBV	1594966	2383837	37.81%	4.363%
38	14.763	1942	1951	1962	rBV	236883	373362	5.92%	0.683%
39	14.993	1985	1990	1996	rVB4	22722	34911	0.55%	0.064%
40	15.393	2051	2058	2061	rBV9	6997	13107	0.21%	0.024%
41	15.569	2081	2088	2096	rBV	2750254	4079182	64.69%	7.467%
42	15.681	2101	2107	2116	rBV	784796	1094176	17.35%	2.003%
43	15.810	2123	2129	2136	rVB	21873	35945	0.57%	0.066%
44	16.016	2161	2164	2169	rVB7	5521	6501	0.10%	0.012%
45	16.128	2179	2183	2189	rBV9	6053	11655	0.18%	0.021%
46	16.257	2198	2205	2210	rBV10	7357	17455	0.28%	0.032%
47	16.351	2215	2221	2230	rVB10	7340	13569	0.22%	0.025%
48	16.475	2236	2242	2247	rVB10	5481	12442	0.20%	0.023%
49	16.728	2283	2285	2290	rVB6	5743	8344	0.13%	0.015%
50	17.104	2344	2349	2355	rBV4	15607	29364	0.47%	0.054%
51	17.328	2380	2387	2394	rBV	2035349	2916933	46.26%	5.339%
52	17.428	2397	2404	2416	rVV	3372728	4831614	76.63%	8.844%
53	17.516	2417	2419	2427	rVB8	9819	16613	0.26%	0.030%
54	17.704	2447	2451	2454	rBV3	6306	8851	0.14%	0.016%
55	18.010	2497	2503	2507	rBV	56769	75149	1.19%	0.138%
56	18.222	2534	2539	2546	rBV	140636	201718	3.20%	0.369%
57	18.516	2586	2589	2590	rBV3	8861	7941	0.13%	0.015%
58	19.139	2691	2695	2698	rVB2	45080	48819	0.77%	0.089%
59	19.239	2708	2712	2715	rBV2	47268	63441	1.01%	0.116%
60	19.304	2719	2723	2727	rVB	52536	65108	1.03%	0.119%
61	19.457	2745	2749	2753	rBV6	25643	40083	0.64%	0.073%
62	19.604	2771	2774	2777	rVB5	18114	19824	0.31%	0.036%
63	19.657	2777	2783	2790	rBV	4235203	5946157	94.30%	10.884%
64	20.563	2934	2937	2942	rVB2	87401	100238	1.59%	0.183%
65	21.139	3031	3035	3040	rBV6	90308	148379	2.35%	0.272%
66	21.192	3042	3044	3049	rVB2	52677	65708	1.04%	0.120%
67	21.416	3077	3082	3088	rBV	2773062	3523177	55.87%	6.449%
68	22.551	3272	3275	3284	rVB4	149207	258490	4.10%	0.473%
69	23.704	3463	3471	3480	rBV2	3123602	6305506	100.00%	11.542%
70	23.863	3491	3498	3509	rVB2	1777627	3686441	58.46%	6.748%




Sum of corrected areas: 54631643

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007667.D
Acq On : 26 Oct 2021 06:07
Operator : CG/JU
Sample : M4291-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P029-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

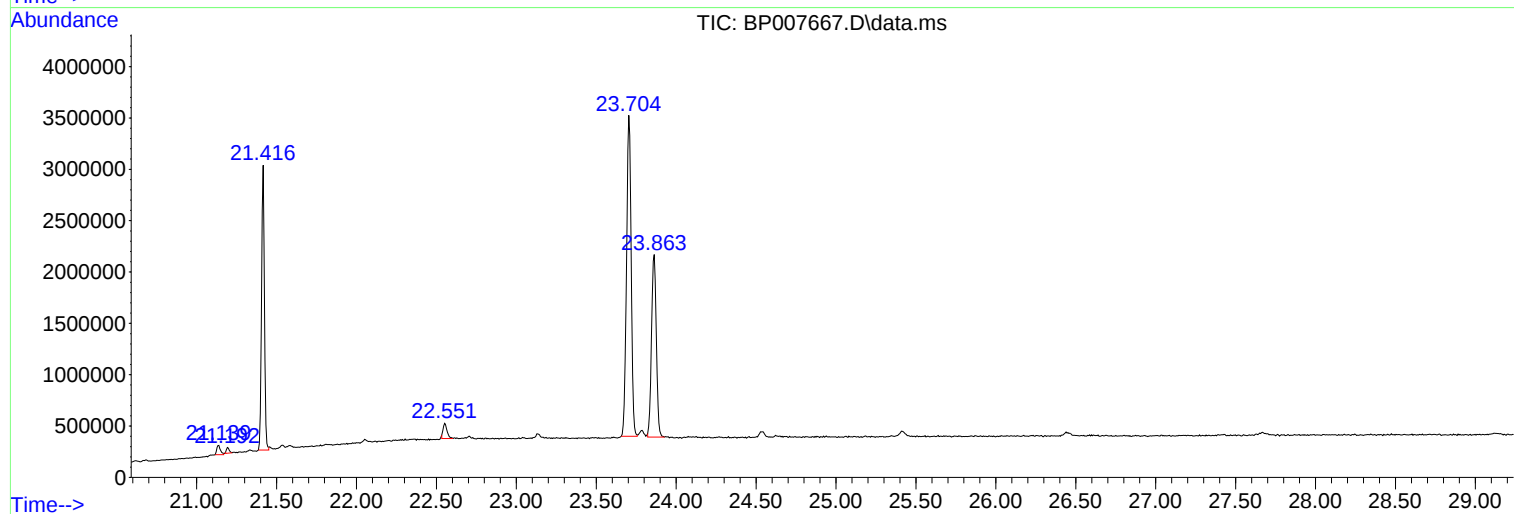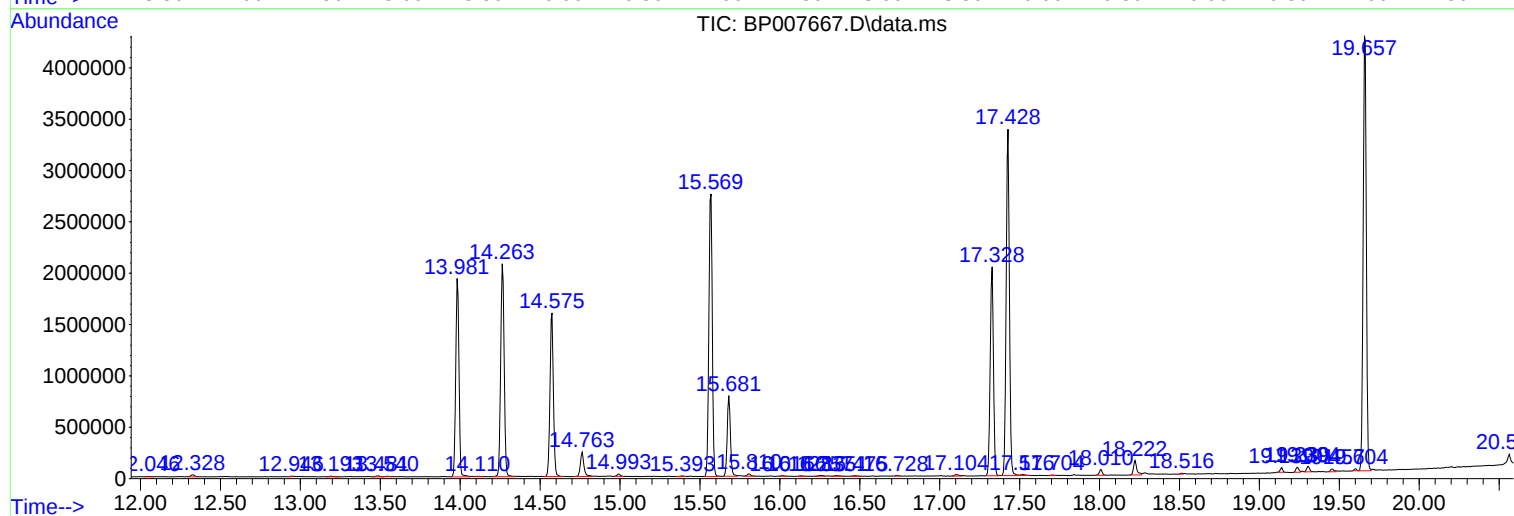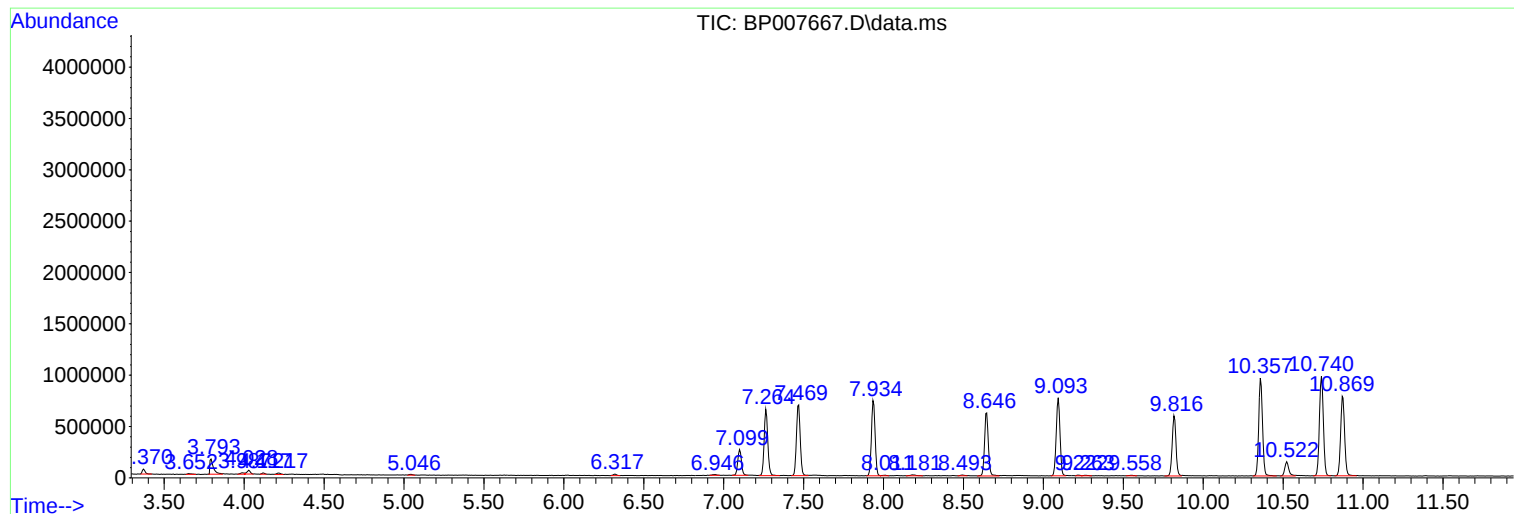

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007667.D
Acq On : 26 Oct 2021 06:07
Operator : CG/JU
Sample : M4291-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P029-TW001-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.522	2.86 ng/ul	237613	Naphthalene-d8	10.740

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

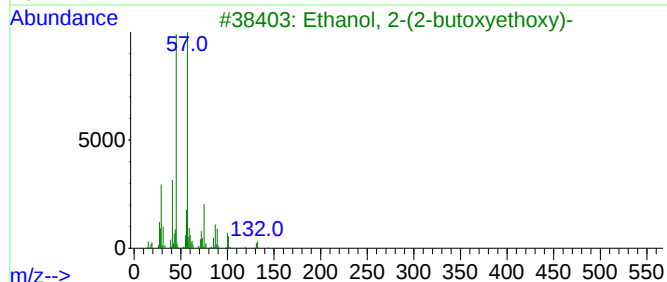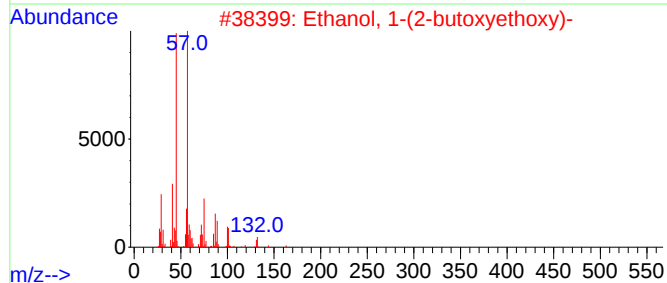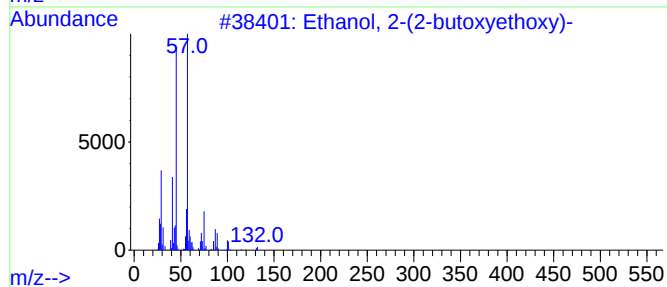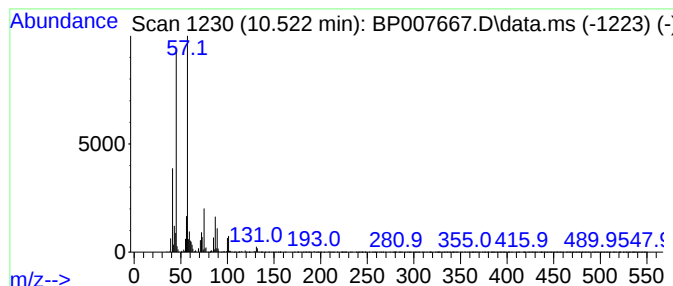

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007667.D
Acq On : 26 Oct 2021 06:07
Operator : CG/JU
Sample : M4291-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P029-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.522	2.9	ng/u1	237613	2	10.740	1659610	20.0