

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007668.D
 Acq On : 26 Oct 2021 06:41
 Operator : CG/JU
 Sample : M4291-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P030-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	22	rVB	54009	68652	1.05%	0.120%
2	3.787	82	85	97	rBV	242856	387438	5.90%	0.678%
3	3.993	116	120	121	rBV3	7356	10464	0.16%	0.018%
4	4.028	122	126	135	rVB	38638	67180	1.02%	0.118%
5	4.123	137	142	147	rBV	14459	20136	0.31%	0.035%
6	4.217	155	158	164	rVB3	15661	22385	0.34%	0.039%
7	5.040	294	298	306	rVB3	7553	12383	0.19%	0.022%
8	6.322	511	516	522	rVB	13156	21070	0.32%	0.037%
9	6.946	613	622	626	rBV9	10678	27330	0.42%	0.048%
10	7.099	642	648	659	rVB	257989	404285	6.16%	0.707%
11	7.264	669	676	686	rBV	703181	1099049	16.75%	1.923%
12	7.469	703	711	723	rVB	749498	1177150	17.94%	2.060%
13	7.564	723	727	731	rBV6	5653	9906	0.15%	0.017%
14	7.934	783	790	800	rVB	779844	1236369	18.84%	2.164%
15	8.187	827	833	842	rBV4	11192	21652	0.33%	0.038%
16	8.493	881	885	890	rBV4	7709	13094	0.20%	0.023%
17	8.646	903	911	925	rBV	639105	1049558	15.99%	1.837%
18	9.093	979	987	997	rBV	812450	1331896	20.30%	2.331%
19	9.269	1013	1017	1025	rVB	7041	12228	0.19%	0.021%
20	9.552	1060	1065	1071	rVB8	7661	14821	0.23%	0.026%
21	9.816	1102	1110	1122	rBV	618059	1036089	15.79%	1.813%
22	10.358	1193	1202	1212	rBV	994574	1657548	25.26%	2.901%
23	10.522	1223	1230	1241	rBV	164151	286660	4.37%	0.502%
24	10.740	1259	1267	1276	rVB	1062073	1756235	26.76%	3.073%
25	10.869	1281	1289	1300	rBV	880123	1536656	23.42%	2.689%
26	11.387	1372	1377	1384	rVB10	3743	8268	0.13%	0.014%
27	12.052	1483	1490	1493	rBV8	4717	8975	0.14%	0.016%
28	12.328	1530	1537	1542	rBV	22998	41109	0.63%	0.072%
29	12.940	1637	1641	1644	rBV5	6788	11649	0.18%	0.020%
30	13.193	1678	1684	1688	rBV6	9264	14780	0.23%	0.026%
31	13.481	1727	1733	1739	rVV4	15391	26160	0.40%	0.046%
32	13.546	1739	1744	1750	rVB9	4982	9589	0.15%	0.017%
33	13.981	1811	1818	1825	rBV	2065088	2825756	43.06%	4.945%
34	14.263	1856	1866	1880	rBV	2184485	3286847	50.09%	5.752%
35	14.487	1899	1904	1909	rVB9	5318	7962	0.12%	0.014%
36	14.569	1909	1918	1930	rBV	1590915	2502080	38.13%	4.378%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007668.D
 Acq On : 26 Oct 2021 06:41
 Operator : CG/JU
 Sample : M4291-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P030-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.763	1945	1951	1963	rBV	230839	352881	5.38%	0.618%
38	14.987	1985	1989	1998	rVB	12944	21721	0.33%	0.038%
39	15.393	2052	2058	2063	rBV5	9720	20533	0.31%	0.036%
40	15.440	2063	2066	2072	rVB6	7149	10342	0.16%	0.018%
41	15.569	2081	2088	2100	rBV	2929763	4329573	65.97%	7.576%
42	15.681	2100	2107	2122	rVV	851710	1165842	17.77%	2.040%
43	15.810	2124	2129	2134	rVB	22740	34180	0.52%	0.060%
44	16.016	2159	2164	2168	rVB7	6999	11344	0.17%	0.020%
45	16.128	2179	2183	2184	rBV4	5316	7766	0.12%	0.014%
46	16.263	2202	2206	2210	rVB7	6881	9795	0.15%	0.017%
47	16.304	2210	2213	2216	rVB4	7645	8013	0.12%	0.014%
48	16.351	2218	2221	2227	rVB8	5605	10833	0.17%	0.019%
49	16.475	2234	2242	2246	rBV8	8183	14714	0.22%	0.026%
50	17.104	2344	2349	2353	rBV4	13781	24663	0.38%	0.043%
51	17.328	2380	2387	2394	rVV	2136993	3065366	46.71%	5.364%
52	17.428	2397	2404	2415	rVV2	3516874	5049843	76.95%	8.837%
53	17.522	2416	2420	2426	rVB8	23756	36075	0.55%	0.063%
54	17.704	2447	2451	2453	rBV4	6623	9615	0.15%	0.017%
55	17.922	2485	2488	2492	rBV6	5074	6664	0.10%	0.012%
56	18.010	2498	2503	2509	rVB	78294	99604	1.52%	0.174%
57	18.222	2535	2539	2545	rBV	37567	56631	0.86%	0.099%
58	18.287	2547	2550	2553	rVB2	11718	14234	0.22%	0.025%
59	18.516	2585	2589	2596	rBV10	7434	17965	0.27%	0.031%
60	19.139	2691	2695	2699	rVB	90818	94247	1.44%	0.165%
61	19.239	2707	2712	2715	rBV2	53190	72784	1.11%	0.127%
62	19.269	2715	2717	2719	rVV2	18375	17334	0.26%	0.030%
63	19.304	2719	2723	2730	rVB	57760	79666	1.21%	0.139%
64	19.457	2746	2749	2753	rBV6	12064	14150	0.22%	0.025%
65	19.598	2771	2773	2777	rBV4	14773	17883	0.27%	0.031%
66	19.663	2778	2784	2790	rVV	4474743	6173548	94.07%	10.803%
67	21.133	3031	3034	3041	rBV5	99036	159135	2.42%	0.278%
68	21.416	3077	3082	3088	rBV	2752123	3669724	55.92%	6.422%
69	23.704	3463	3471	3480	rBV2	3295623	6562502	100.00%	11.484%
70	23.863	3491	3498	3509	rVB2	1872775	3883868	59.18%	6.796%




Sum of corrected areas: 57146447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007668.D
Acq On : 26 Oct 2021 06:41
Operator : CG/JU
Sample : M4291-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

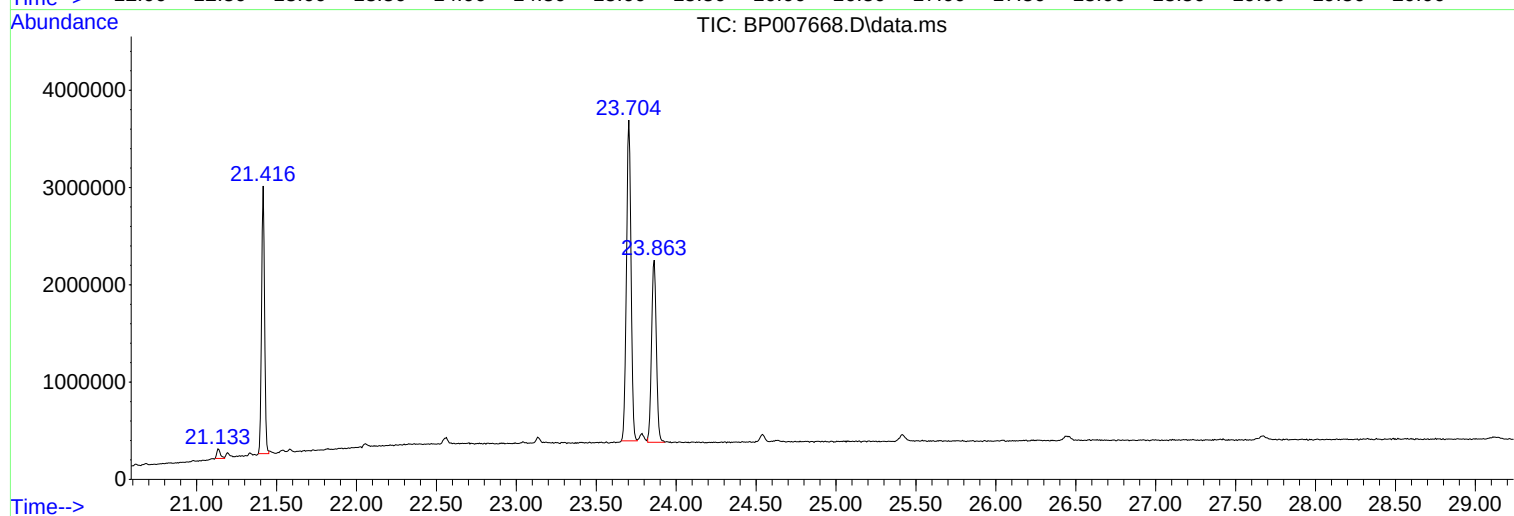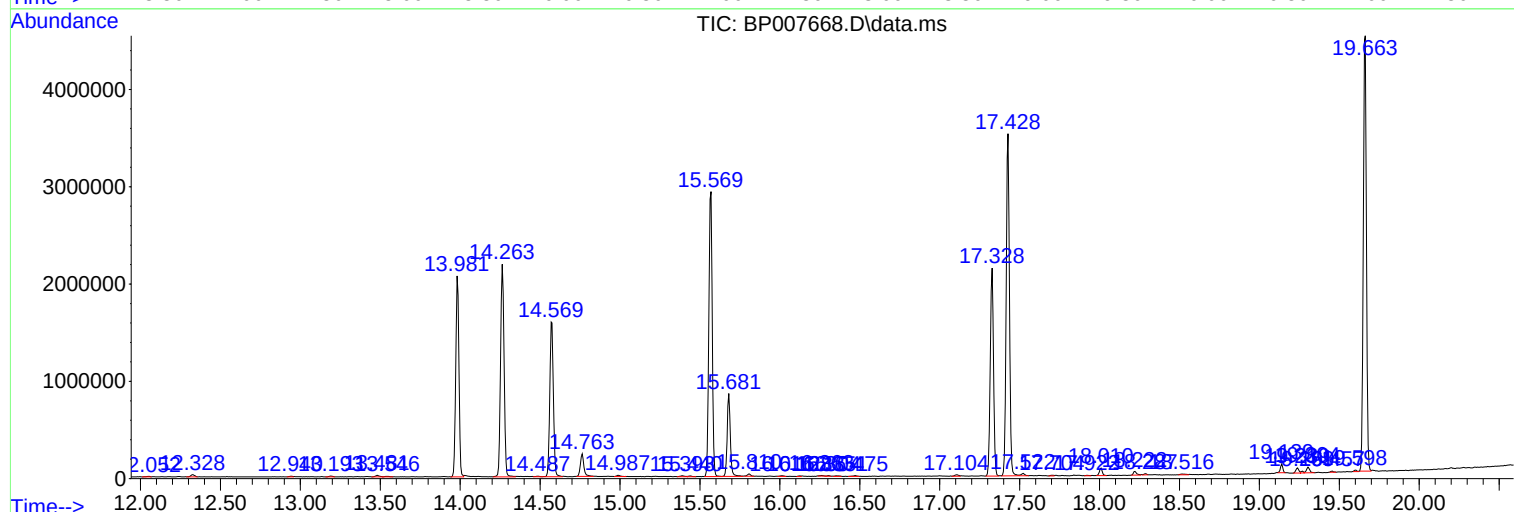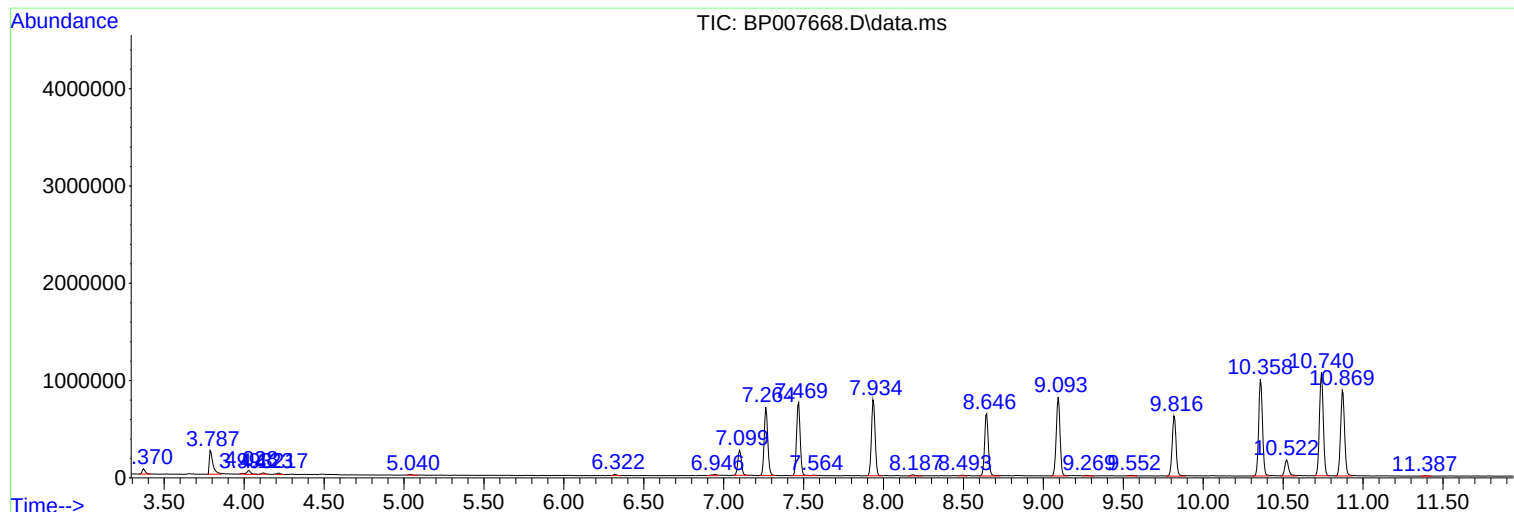

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007668.D
Acq On : 26 Oct 2021 06:41
Operator : CG/JU
Sample : M4291-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW001-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.522	3.26 ng/ul	286660	Naphthalene-d8	10.740

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

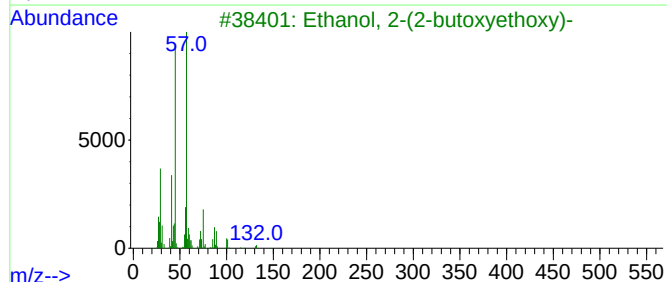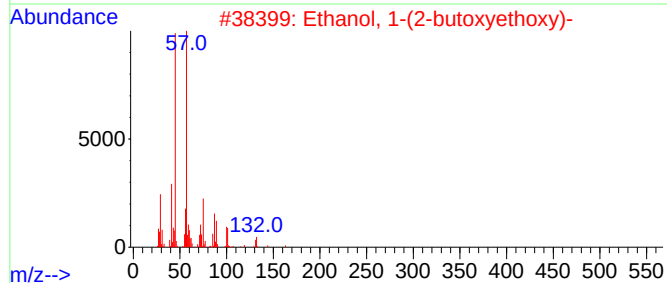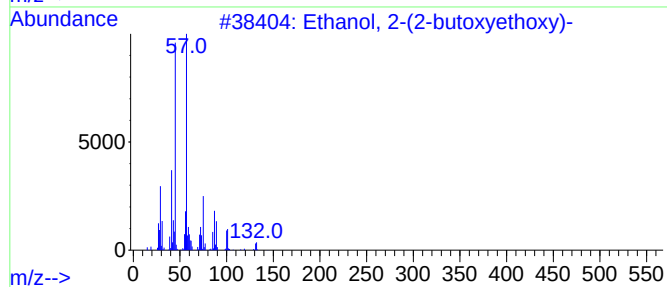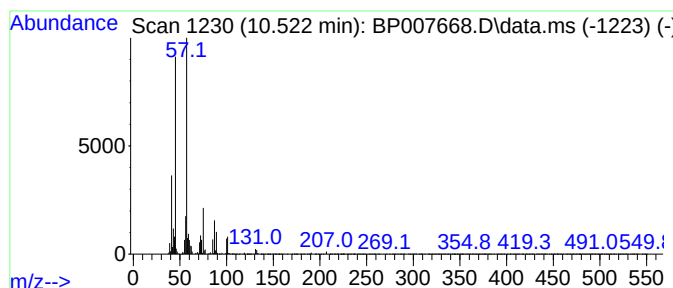

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007668.D
Acq On : 26 Oct 2021 06:41
Operator : CG/JU
Sample : M4291-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.522	3.3	ng/u1	286660	2	10.740	1756240	20.0