

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007672.D
 Acq On : 26 Oct 2021 09:31
 Operator : CG/JU
 Sample : PB140137BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	22	rVB	57082	80334	1.37%	0.142%
2	3.781	81	84	105	rBV	779418	1192278	20.30%	2.101%
3	4.117	138	141	146	rVB2	13439	19115	0.33%	0.034%
4	7.099	641	648	658	rBV	889787	1384738	23.57%	2.440%
5	7.264	669	676	686	rVB	713348	1104605	18.80%	1.946%
6	7.464	703	710	725	rBV	891460	1433772	24.41%	2.526%
7	7.934	782	790	798	rBV	738530	1180410	20.10%	2.080%
8	8.387	860	867	870	rBV9	3550	6714	0.11%	0.012%
9	8.640	902	910	926	rBV	1066116	1752811	29.84%	3.088%
10	8.758	926	930	938	rVV	5406	11518	0.20%	0.020%
11	9.093	979	987	999	rBV	821404	1344789	22.89%	2.369%
12	9.669	1080	1085	1091	rVB9	3744	8354	0.14%	0.015%
13	9.816	1103	1110	1121	rBV	675690	1090807	18.57%	1.922%
14	10.152	1162	1167	1172	rVB9	3859	7471	0.13%	0.013%
15	10.358	1194	1202	1214	rBV	1094083	1788057	30.44%	3.150%
16	10.740	1258	1267	1280	rVB	989254	1681173	28.62%	2.962%
17	10.869	1280	1289	1308	rBV	1036972	1812049	30.85%	3.193%
18	11.087	1323	1326	1334	rVB10	3995	6296	0.11%	0.011%
19	12.328	1532	1537	1545	rVV	19549	32083	0.55%	0.057%
20	12.405	1545	1550	1553	rVB4	4032	6765	0.12%	0.012%
21	12.540	1567	1573	1578	rBV10	3878	6867	0.12%	0.012%
22	12.616	1583	1586	1590	rVB6	5772	8136	0.14%	0.014%
23	12.769	1607	1612	1617	rBV9	4851	7331	0.12%	0.013%
24	13.369	1709	1714	1717	rBV7	7676	13230	0.23%	0.023%
25	13.446	1724	1727	1734	rVB4	5324	9530	0.16%	0.017%
26	13.546	1739	1744	1749	rVB5	4729	8424	0.14%	0.015%
27	13.981	1811	1818	1825	rBV	1930075	2729348	46.46%	4.809%
28	14.263	1857	1866	1876	rBV	2210069	3175681	54.06%	5.595%
29	14.575	1911	1919	1926	rBV	1505202	2314416	39.40%	4.078%
30	14.634	1926	1929	1936	rVB6	8278	15349	0.26%	0.027%
31	14.763	1943	1951	1968	rBV	919466	1340278	22.82%	2.361%
32	14.893	1970	1973	1976	rVV4	10214	15179	0.26%	0.027%
33	14.928	1977	1979	1983	rVV5	7920	12701	0.22%	0.022%
34	14.975	1983	1987	1996	rVB3	8892	18919	0.32%	0.033%
35	15.204	2021	2026	2029	rBV6	5477	7436	0.13%	0.013%
36	15.393	2053	2058	2063	rBV4	8028	12667	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007672.D
 Acq On : 26 Oct 2021 09:31
 Operator : CG/JU
 Sample : PB140137BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK137

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.569	2081	2088	2094	rBV	2765769	4037453	68.73%	7.114%
38	15.616	2094	2096	2101	rVV4	16352	24159	0.41%	0.043%
39	15.681	2101	2107	2119	rVV	746000	1025792	17.46%	1.807%
40	15.810	2124	2129	2137	rVB2	22944	44969	0.77%	0.079%
41	16.245	2196	2203	2209	rBV2	6232	12749	0.22%	0.022%
42	16.357	2218	2222	2225	rBV6	4410	7168	0.12%	0.013%
43	16.516	2244	2249	2254	rBV9	5945	10883	0.19%	0.019%
44	16.628	2265	2268	2276	rVB7	5857	9560	0.16%	0.017%
45	16.787	2291	2295	2300	rBV8	5246	9104	0.15%	0.016%
46	17.116	2346	2351	2356	rVB4	9225	16664	0.28%	0.029%
47	17.328	2380	2387	2397	rBV	1974188	2831713	48.21%	4.989%
48	17.428	2397	2404	2418	rVV	3139423	4456145	75.86%	7.851%
49	17.704	2448	2451	2454	rBV4	5206	8848	0.15%	0.016%
50	17.734	2454	2456	2461	rVB4	8429	10542	0.18%	0.019%
51	18.287	2547	2550	2557	rVB2	7365	12188	0.21%	0.021%
52	19.239	2707	2712	2718	rBV2	49606	73113	1.24%	0.129%
53	19.310	2719	2724	2727	rBV	44065	64528	1.10%	0.114%
54	19.663	2778	2784	2793	rBV	4159266	5504309	93.70%	9.698%
55	21.416	3077	3082	3088	rBV	2567887	3429998	58.39%	6.043%
56	23.710	3464	3472	3481	rBV2	2885032	5874127	100.00%	10.350%
57	23.863	3491	3498	3510	rVB2	1758973	3653301	62.19%	6.437%




Sum of corrected areas: 56756944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007672.D
Acq On : 26 Oct 2021 09:31
Operator : CG/JU
Sample : PB140137BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

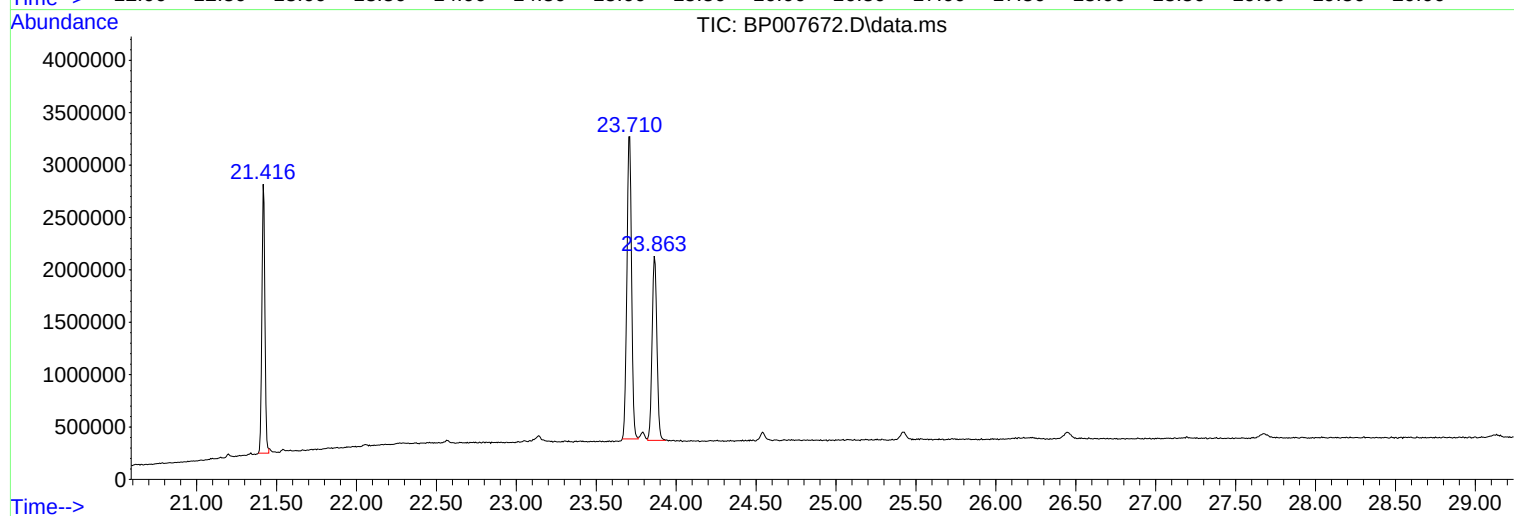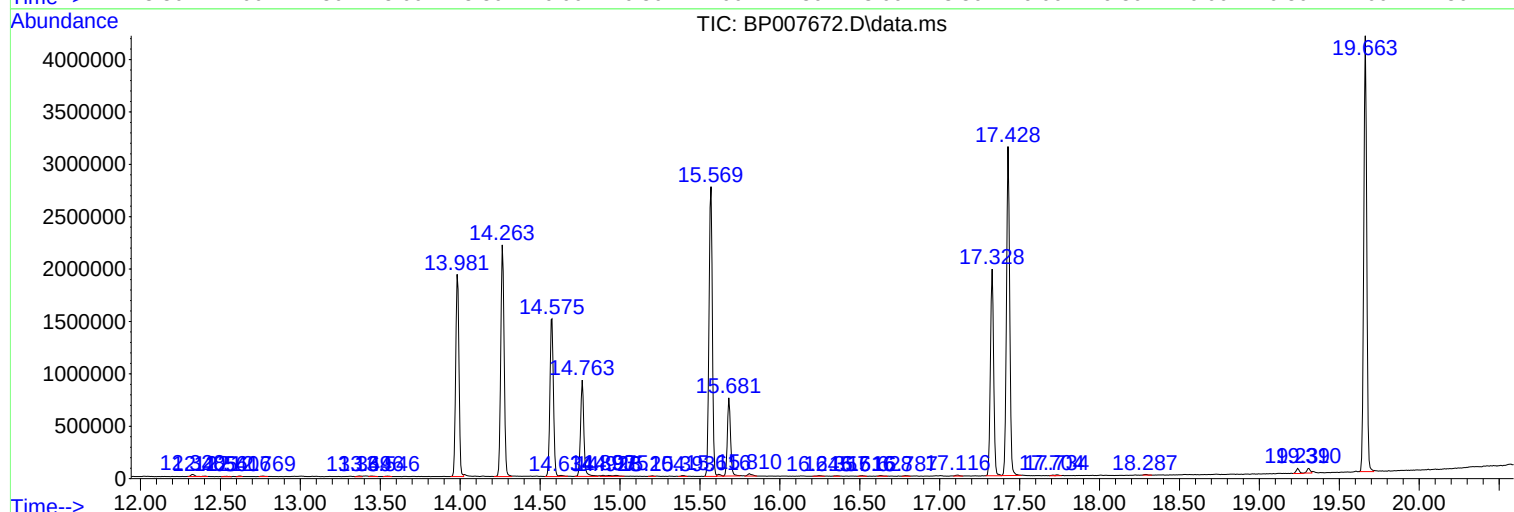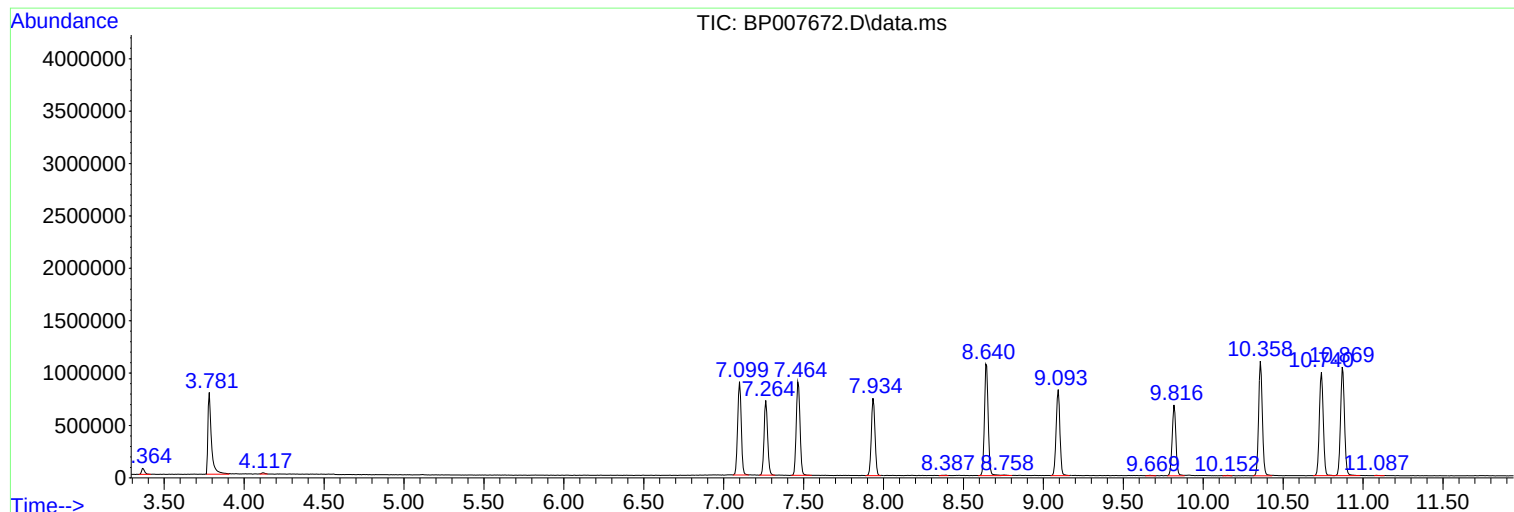

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007672.D
Acq On : 26 Oct 2021 09:31
Operator : CG/JU
Sample : PB140137BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007672.D
Acq On : 26 Oct 2021 09:31
Operator : CG/JU
Sample : PB140137BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK137

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------