

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007674.D
 Acq On : 26 Oct 2021 10:39
 Operator : CG/JU
 Sample : M4291-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P030-TW002-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	22	rVB	46998	64356	1.05%	0.124%
2	3.787	82	85	96	rBV	216212	333343	5.42%	0.643%
3	3.981	116	118	121	rBV4	6250	10055	0.16%	0.019%
4	4.028	121	126	131	rVB	30823	48744	0.79%	0.094%
5	4.117	137	141	145	rBV	12010	16022	0.26%	0.031%
6	4.217	154	158	162	rVB5	12001	16247	0.26%	0.031%
7	4.481	201	203	209	rVB6	4518	6849	0.11%	0.013%
8	5.040	293	298	301	rBV4	5435	9854	0.16%	0.019%
9	6.317	510	515	521	rVB4	10931	18021	0.29%	0.035%
10	6.940	616	621	626	rBV9	6807	13096	0.21%	0.025%
11	7.099	641	648	657	rVB	197905	311061	5.05%	0.600%
12	7.264	670	676	689	rVB	603337	945545	15.36%	1.823%
13	7.464	703	710	723	rVV	617723	997971	16.21%	1.925%
14	7.569	723	728	734	rVV10	6457	13984	0.23%	0.027%
15	7.934	783	790	799	rVB	742981	1149434	18.68%	2.217%
16	8.005	799	802	806	rBV6	3970	6197	0.10%	0.012%
17	8.181	826	832	838	rBV5	8309	14783	0.24%	0.029%
18	8.493	880	885	888	rBV7	5406	7007	0.11%	0.014%
19	8.640	904	910	921	rBV	506473	835871	13.58%	1.612%
20	9.093	978	987	997	rBV	702135	1157943	18.81%	2.233%
21	9.275	1013	1018	1021	rVB7	5632	9705	0.16%	0.019%
22	9.552	1062	1065	1072	rVB9	6589	11464	0.19%	0.022%
23	9.816	1103	1110	1121	rBV	547325	884737	14.37%	1.706%
24	9.910	1124	1126	1131	rVB6	4767	6333	0.10%	0.012%
25	10.063	1146	1152	1158	rVB10	5060	11635	0.19%	0.022%
26	10.358	1194	1202	1219	rBV	855562	1438235	23.37%	2.774%
27	10.522	1224	1230	1242	rBV2	167766	300519	4.88%	0.580%
28	10.740	1259	1267	1281	rVB	959990	1627617	26.44%	3.139%
29	10.869	1281	1289	1300	rBV	772353	1353225	21.99%	2.610%
30	12.046	1487	1489	1500	rVB9	5588	9398	0.15%	0.018%
31	12.328	1532	1537	1543	rBV2	19675	33726	0.55%	0.065%
32	12.622	1581	1587	1592	rBV10	4420	8141	0.13%	0.016%
33	12.940	1637	1641	1647	rBV7	5208	10670	0.17%	0.021%
34	13.193	1676	1684	1690	rVB7	8558	15067	0.24%	0.029%
35	13.369	1710	1714	1718	rBV7	5708	10985	0.18%	0.021%
36	13.481	1729	1733	1738	rVB2	23698	36998	0.60%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007674.D
 Acq On : 26 Oct 2021 10:39
 Operator : CG/JU
 Sample : M4291-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P030-TW002-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	13.546	1738	1744	1749	rBV8	5561	8012	0.13%	0.015%
38	13.898	1800	1804	1809	rVB7	4500	8246	0.13%	0.016%
39	13.981	1809	1818	1824	rBV	1844569	2534442	41.18%	4.888%
40	14.263	1856	1866	1882	rBV	1979550	2912460	47.32%	5.617%
41	14.575	1911	1919	1926	rBV	1472349	2244200	36.46%	4.328%
42	14.763	1942	1951	1965	rBV2	184998	314963	5.12%	0.607%
43	14.893	1969	1973	1977	rBV5	4791	6414	0.10%	0.012%
44	14.993	1983	1990	1995	rVB5	13100	25034	0.41%	0.048%
45	15.128	2006	2013	2018	rBV2	52001	146331	2.38%	0.282%
46	15.398	2054	2059	2062	rVB2	11991	17365	0.28%	0.033%
47	15.569	2081	2088	2095	rBV	2700415	3962966	64.39%	7.643%
48	15.622	2095	2097	2101	rVB4	12819	13797	0.22%	0.027%
49	15.681	2101	2107	2117	rBV	771672	1048569	17.04%	2.022%
50	15.810	2124	2129	2137	rVB5	21312	41239	0.67%	0.080%
51	15.940	2147	2151	2156	rBV8	4555	7418	0.12%	0.014%
52	16.022	2160	2165	2168	rVB6	5457	9563	0.16%	0.018%
53	16.257	2200	2205	2210	rBV8	7266	15438	0.25%	0.030%
54	16.469	2237	2241	2245	rBV7	6753	12060	0.20%	0.023%
55	16.634	2266	2269	2275	rBV8	6978	9443	0.15%	0.018%
56	17.004	2330	2332	2337	rVB6	5739	7026	0.11%	0.014%
57	17.110	2345	2350	2356	rBV3	12220	22393	0.36%	0.043%
58	17.328	2380	2387	2397	rBV	1873726	2704532	43.94%	5.216%
59	17.428	2397	2404	2415	rVV2	3287720	4687398	76.16%	9.040%
60	17.522	2416	2420	2425	rVB6	24937	35007	0.57%	0.068%
61	18.010	2499	2503	2510	rVB2	80441	98686	1.60%	0.190%
62	18.222	2535	2539	2546	rBV3	65166	102148	1.66%	0.197%
63	19.139	2692	2695	2701	rVB2	76870	93453	1.52%	0.180%
64	19.245	2710	2713	2716	rBV2	49555	66979	1.09%	0.129%
65	19.310	2721	2724	2727	rBV	48274	60918	0.99%	0.117%
66	19.663	2778	2784	2790	rBV	4304150	5751653	93.45%	11.092%
67	21.133	3031	3034	3040	rBV2	130857	205096	3.33%	0.396%
68	21.416	3077	3082	3093	rBV	2499370	3315225	53.86%	6.393%
69	23.704	3464	3471	3480	rBV2	3024953	6154728	100.00%	11.869%
70	23.863	3491	3498	3512	rVB2	1644532	3466125	56.32%	6.684%




Sum of corrected areas: 51854165

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007674.D
Acq On : 26 Oct 2021 10:39
Operator : CG/JU
Sample : M4291-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW002-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

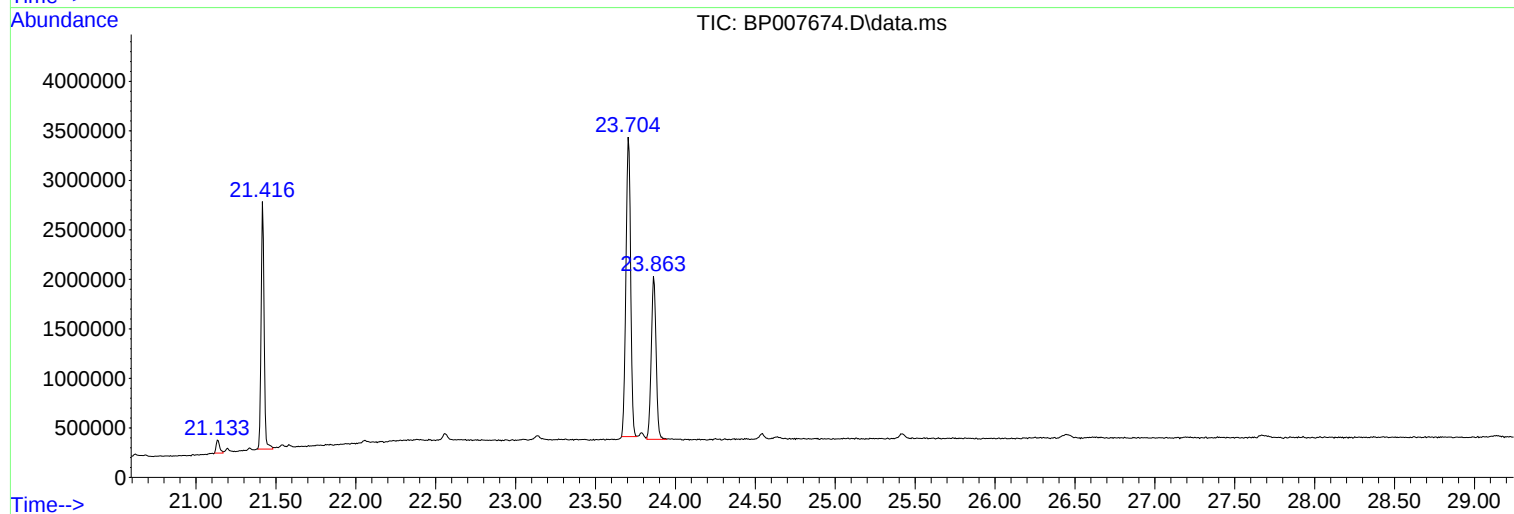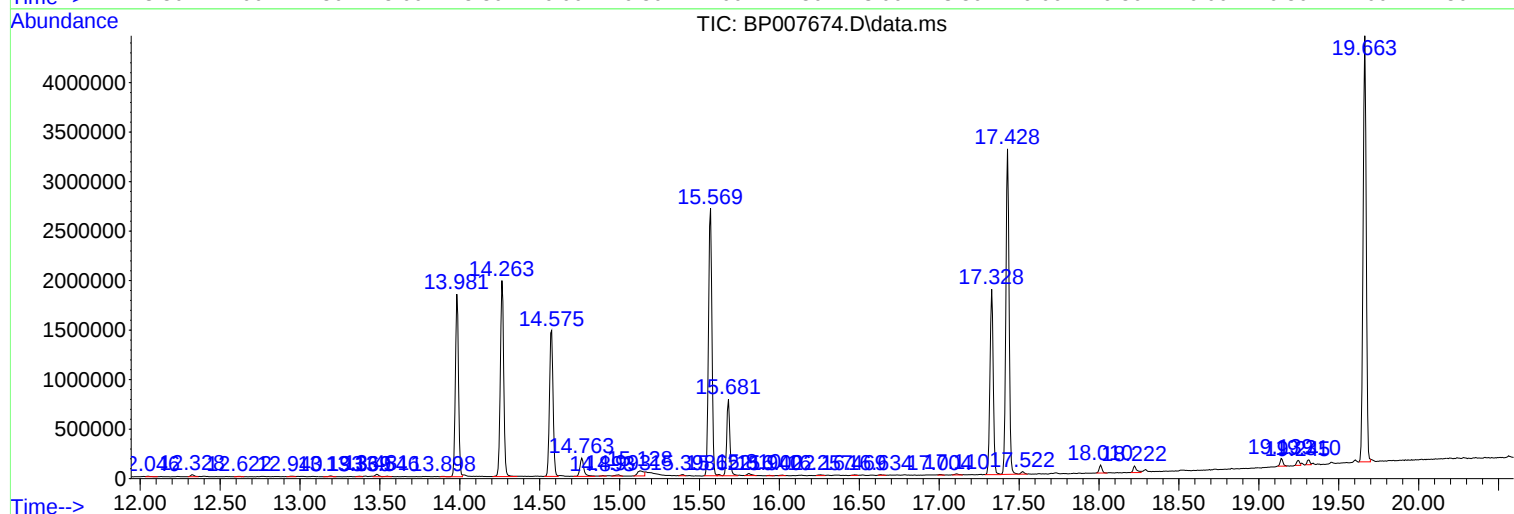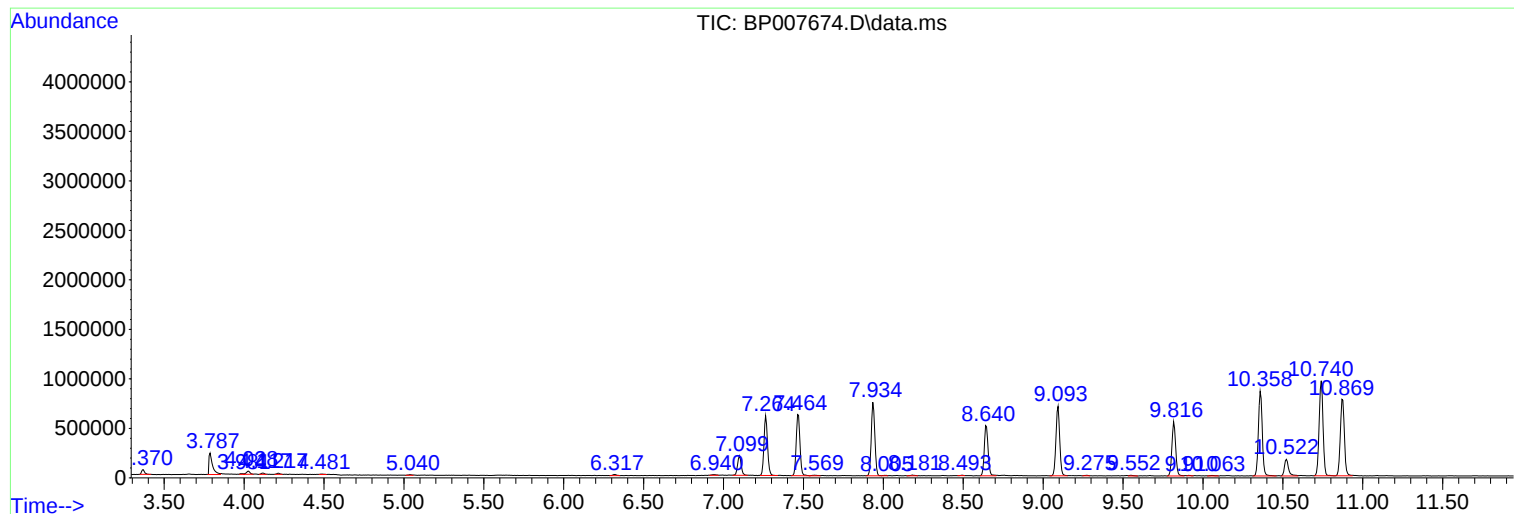

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007674.D
Acq On : 26 Oct 2021 10:39
Operator : CG/JU
Sample : M4291-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW002-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.522	3.69 ng/ul	300519	Naphthalene-d8	10.740

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

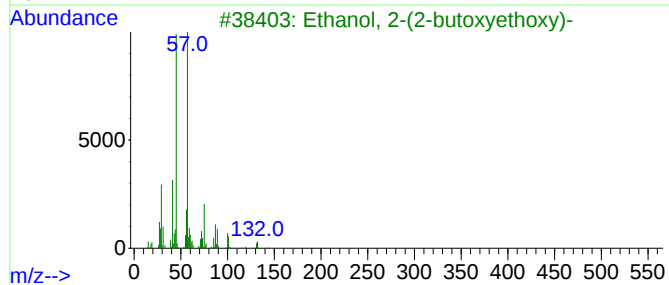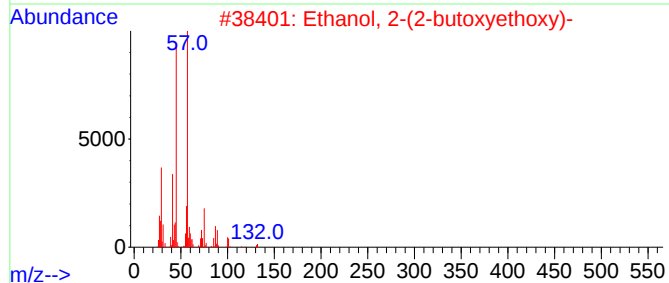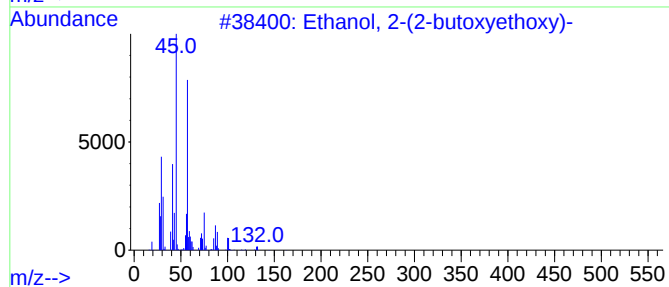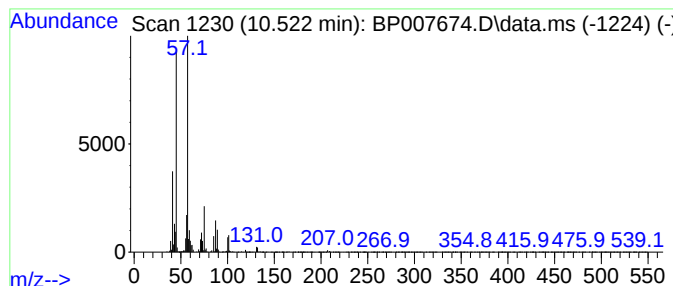

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007674.D
Acq On : 26 Oct 2021 10:39
Operator : CG/JU
Sample : M4291-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P030-TW002-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.522	3.7	ng/u1	300519	2	10.740	1627620	20.0