

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007675.D
 Acq On : 26 Oct 2021 11:13
 Operator : CG/JU
 Sample : M4291-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P041-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	9	14	20	rBV	42578	57759	0.94%	0.111%
2	3.787	83	85	94	rBV	205864	305150	4.97%	0.587%
3	3.987	116	119	122	rBV3	6343	9531	0.16%	0.018%
4	4.022	122	125	133	rVV	29836	49146	0.80%	0.094%
5	4.117	137	141	149	rVB2	15221	26282	0.43%	0.051%
6	4.211	154	157	162	rVB2	14357	19098	0.31%	0.037%
7	5.040	294	298	302	rVB4	5448	8036	0.13%	0.015%
8	6.322	511	516	521	rVB4	10116	17380	0.28%	0.033%
9	6.940	616	621	625	rBV4	5747	9302	0.15%	0.018%
10	7.099	641	648	657	rVB	236732	360237	5.86%	0.693%
11	7.263	668	676	688	rVB	674113	1058964	17.24%	2.036%
12	7.463	703	710	720	rBV	710305	1124512	18.30%	2.162%
13	7.581	724	730	733	rBV8	5061	9672	0.16%	0.019%
14	7.934	781	790	799	rBV	775598	1215290	19.78%	2.336%
15	8.010	799	803	807	rVB4	6524	10771	0.18%	0.021%
16	8.181	825	832	837	rBV8	8375	19210	0.31%	0.037%
17	8.499	880	886	891	rBV7	6224	10302	0.17%	0.020%
18	8.640	903	910	923	rBV	586145	938150	15.27%	1.803%
19	9.093	977	987	998	rBV	788842	1278156	20.81%	2.457%
20	9.552	1062	1065	1070	rVB7	3733	6147	0.10%	0.012%
21	9.816	1103	1110	1119	rBV	607773	979456	15.94%	1.883%
22	10.357	1194	1202	1221	rBV	947474	1573299	25.61%	3.025%
23	10.522	1224	1230	1236	rBV2	62119	111984	1.82%	0.215%
24	10.740	1258	1267	1278	rBV	981768	1684487	27.42%	3.238%
25	10.869	1281	1289	1303	rBV	778799	1345591	21.90%	2.587%
26	12.046	1484	1489	1497	rVB	4043	8315	0.14%	0.016%
27	12.328	1530	1537	1545	rBV2	20478	37853	0.62%	0.073%
28	13.193	1679	1684	1688	rVB7	3401	6867	0.11%	0.013%
29	13.540	1738	1743	1750	rVB9	6197	11872	0.19%	0.023%
30	13.981	1808	1818	1833	rBV	1811270	2503213	40.75%	4.812%
31	14.263	1856	1866	1874	rBV	2066227	3028604	49.30%	5.822%
32	14.575	1908	1919	1928	rBV	1488885	2262682	36.83%	4.350%
33	14.763	1945	1951	1962	rBV	176511	281346	4.58%	0.541%
34	14.992	1986	1990	1995	rVB8	7986	12216	0.20%	0.023%
35	15.392	2055	2058	2063	rVB7	3920	6375	0.10%	0.012%
36	15.569	2081	2088	2096	rBV	2670689	3945002	64.22%	7.584%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007675.D
 Acq On : 26 Oct 2021 11:13
 Operator : CG/JU
 Sample : M4291-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P041-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.681	2100	2107	2116	rBV	732726	984424	16.02%	1.892%
38	15.810	2124	2129	2136	rVB2	20736	34672	0.56%	0.067%
39	16.251	2197	2204	2210	rBV2	7446	17870	0.29%	0.034%
40	16.357	2218	2222	2226	rBV6	5790	10231	0.17%	0.020%
41	16.469	2238	2241	2246	rVB7	4302	6857	0.11%	0.013%
42	16.657	2266	2273	2275	rBV8	3952	8675	0.14%	0.017%
43	17.010	2327	2333	2336	rVB8	3795	6870	0.11%	0.013%
44	17.110	2345	2350	2356	rBV	8933	18426	0.30%	0.035%
45	17.328	2380	2387	2397	rBV	1909377	2761154	44.95%	5.308%
46	17.428	2397	2404	2417	rVV2	3255301	4607613	75.00%	8.858%
47	17.522	2417	2420	2426	rVB6	23979	33391	0.54%	0.064%
48	18.010	2499	2503	2508	rVB2	21810	28545	0.46%	0.055%
49	18.122	2518	2522	2527	rBV7	6481	12180	0.20%	0.023%
50	18.222	2535	2539	2546	rBV	45600	71459	1.16%	0.137%
51	18.522	2586	2590	2596	rBV8	16759	33998	0.55%	0.065%
52	19.122	2690	2692	2696	rBV5	13277	18519	0.30%	0.036%
53	19.239	2707	2712	2716	rBV2	53569	74293	1.21%	0.143%
54	19.310	2719	2724	2727	rBV	53807	79561	1.30%	0.153%
55	19.663	2778	2784	2793	rBV	4193973	5840259	95.07%	11.227%
56	21.416	3078	3082	3088	rBV	2379387	3188554	51.90%	6.130%
57	23.710	3465	3472	3481	rVB2	3064486	6143361	100.00%	11.810%
58	23.868	3492	3499	3512	rVB2	1745303	3705245	60.31%	7.123%




Sum of corrected areas: 52018414

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007675.D
Acq On : 26 Oct 2021 11:13
Operator : CG/JU
Sample : M4291-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P041-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

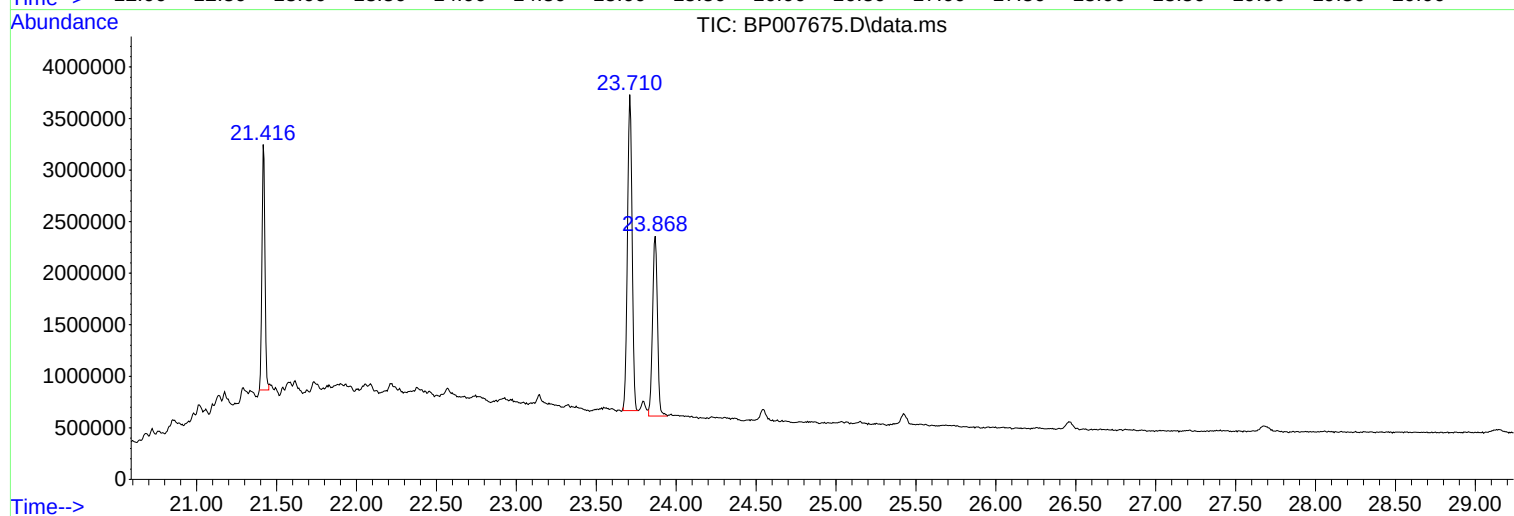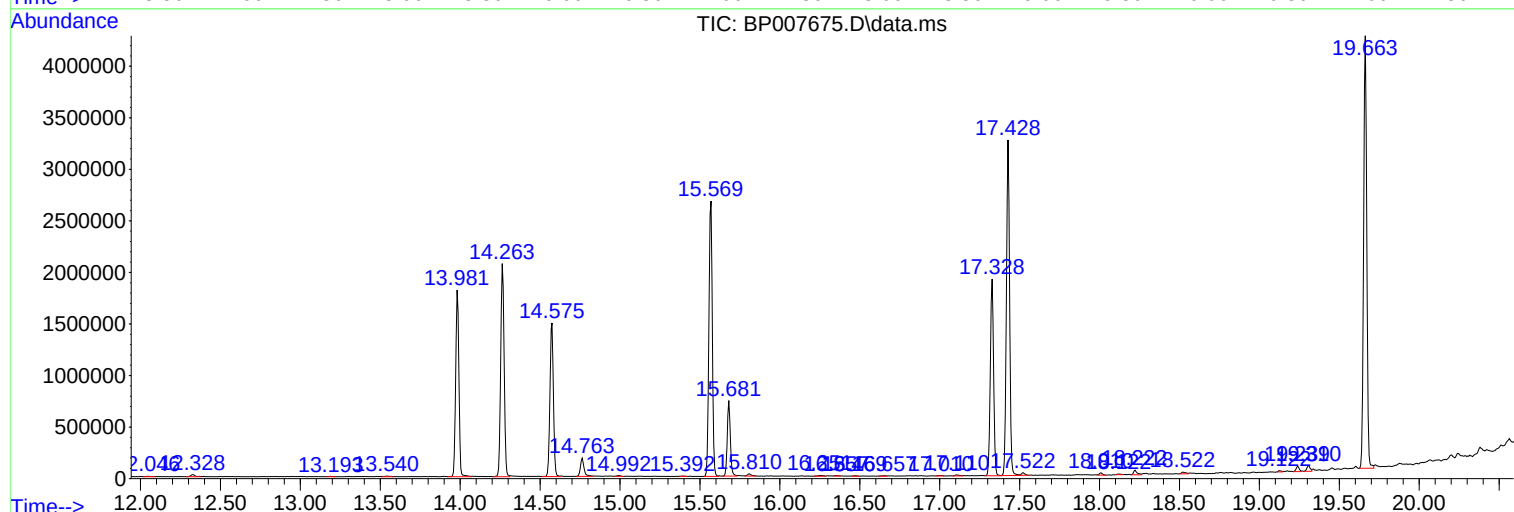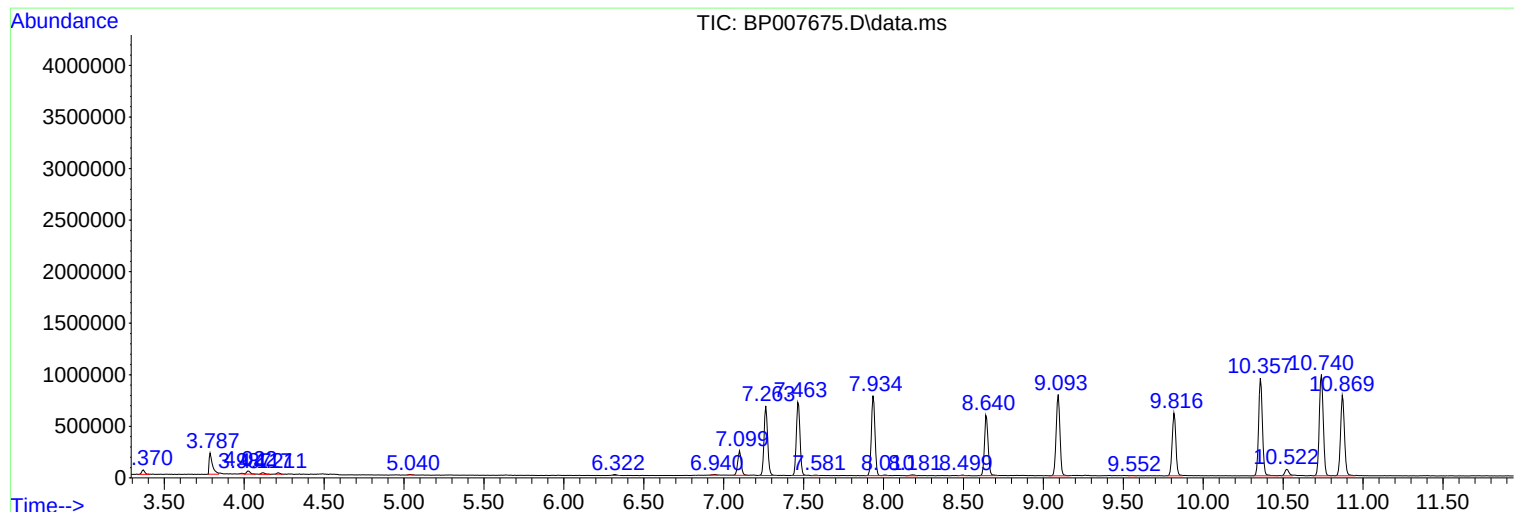

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007675.D
Acq On : 26 Oct 2021 11:13
Operator : CG/JU
Sample : M4291-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P041-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007675.D
Acq On : 26 Oct 2021 11:13
Operator : CG/JU
Sample : M4291-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P041-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------