

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007676.D
 Acq On : 26 Oct 2021 11:47
 Operator : CG/JU
 Sample : M4291-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P045-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	9	14	23	rVB	48698	70602	1.09%	0.129%
2	3.787	83	85	100	rBV	217832	347780	5.35%	0.637%
3	3.987	116	119	121	rBV4	5992	8266	0.13%	0.015%
4	4.028	122	126	132	rVB	33165	49972	0.77%	0.092%
5	4.117	137	141	149	rVB2	14677	25122	0.39%	0.046%
6	4.217	154	158	162	rVB3	11148	14091	0.22%	0.026%
7	5.040	294	298	301	rBV4	5661	8043	0.12%	0.015%
8	6.322	510	516	521	rBV3	11106	17319	0.27%	0.032%
9	6.940	617	621	627	rVB6	8509	11968	0.18%	0.022%
10	7.099	642	648	657	rVB	226834	348404	5.36%	0.638%
11	7.263	670	676	689	rVB	701827	1086126	16.70%	1.990%
12	7.469	703	711	718	rBV	700544	1132308	17.41%	2.074%
13	7.934	782	790	799	rBV	815403	1296502	19.93%	2.375%
14	8.187	828	833	841	rVB3	9986	19231	0.30%	0.035%
15	8.493	880	885	889	rBV7	6416	9611	0.15%	0.018%
16	8.646	902	911	919	rBV	588558	952564	14.64%	1.745%
17	9.093	977	987	998	rBV	801904	1315697	20.23%	2.410%
18	9.269	1012	1017	1022	rVB8	8319	14405	0.22%	0.026%
19	9.552	1061	1065	1070	rVB7	5071	8831	0.14%	0.016%
20	9.816	1103	1110	1120	rBV	616031	1022055	15.71%	1.872%
21	10.357	1195	1202	1213	rBV	957135	1627690	25.02%	2.982%
22	10.522	1224	1230	1239	rBV2	38164	78646	1.21%	0.144%
23	10.740	1259	1267	1276	rBV	1046580	1810643	27.83%	3.317%
24	10.875	1280	1290	1300	rBV	812400	1416458	21.78%	2.595%
25	12.246	1517	1523	1528	rVV8	4253	7676	0.12%	0.014%
26	12.334	1531	1538	1543	rVV2	21754	40653	0.62%	0.074%
27	13.545	1741	1744	1751	rVB7	5379	9344	0.14%	0.017%
28	13.987	1812	1819	1832	rBV	1813374	2565725	39.44%	4.700%
29	14.269	1857	1867	1876	rBV	2049922	3149302	48.41%	5.770%
30	14.410	1889	1891	1899	rVB9	6576	11684	0.18%	0.021%
31	14.487	1900	1904	1910	rVB4	13613	16704	0.26%	0.031%
32	14.575	1911	1919	1931	rBV	1675046	2488493	38.26%	4.559%
33	14.763	1945	1951	1961	rBV	178783	295923	4.55%	0.542%
34	14.992	1986	1990	1996	rBV9	9433	15452	0.24%	0.028%
35	15.110	2006	2010	2014	rBV5	14111	21571	0.33%	0.040%
36	15.439	2062	2066	2069	rBV3	20799	25333	0.39%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007676.D
 Acq On : 26 Oct 2021 11:47
 Operator : CG/JU
 Sample : M4291-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P045-TW001-01

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.569	2081	2088	2096	rBV	2792082	4015208	61.73%	7.356%
38	15.681	2101	2107	2115	rBV	746077	1029271	15.82%	1.886%
39	15.816	2125	2130	2131	rBV3	21278	33486	0.51%	0.061%
40	16.057	2168	2171	2175	rBV4	15777	24084	0.37%	0.044%
41	16.304	2210	2213	2215	rBV2	47014	58169	0.89%	0.107%
42	16.334	2215	2218	2228	rVB	67562	114120	1.75%	0.209%
43	17.104	2346	2349	2352	rBV2	38152	55768	0.86%	0.102%
44	17.157	2355	2358	2370	rVB2	77220	132999	2.04%	0.244%
45	17.328	2381	2387	2393	rBV	2079342	2928710	45.02%	5.365%
46	17.428	2398	2404	2412	rVV2	3227359	4648280	71.46%	8.516%
47	18.010	2500	2503	2507	rVB	73807	84473	1.30%	0.155%
48	19.663	2778	2784	2792	rBV	4274729	5906320	90.80%	10.820%
49	21.333	3066	3068	3072	rVB	325211	333185	5.12%	0.610%
50	21.416	3078	3082	3094	rVB	2518780	3484445	53.57%	6.383%
51	23.710	3465	3472	3481	rVB2	3239012	6504925	100.00%	11.917%
52	23.868	3492	3499	3508	rVB	1854007	3891597	59.83%	7.129%




Sum of corrected areas: 54585234

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007676.D
Acq On : 26 Oct 2021 11:47
Operator : CG/JU
Sample : M4291-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P045-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

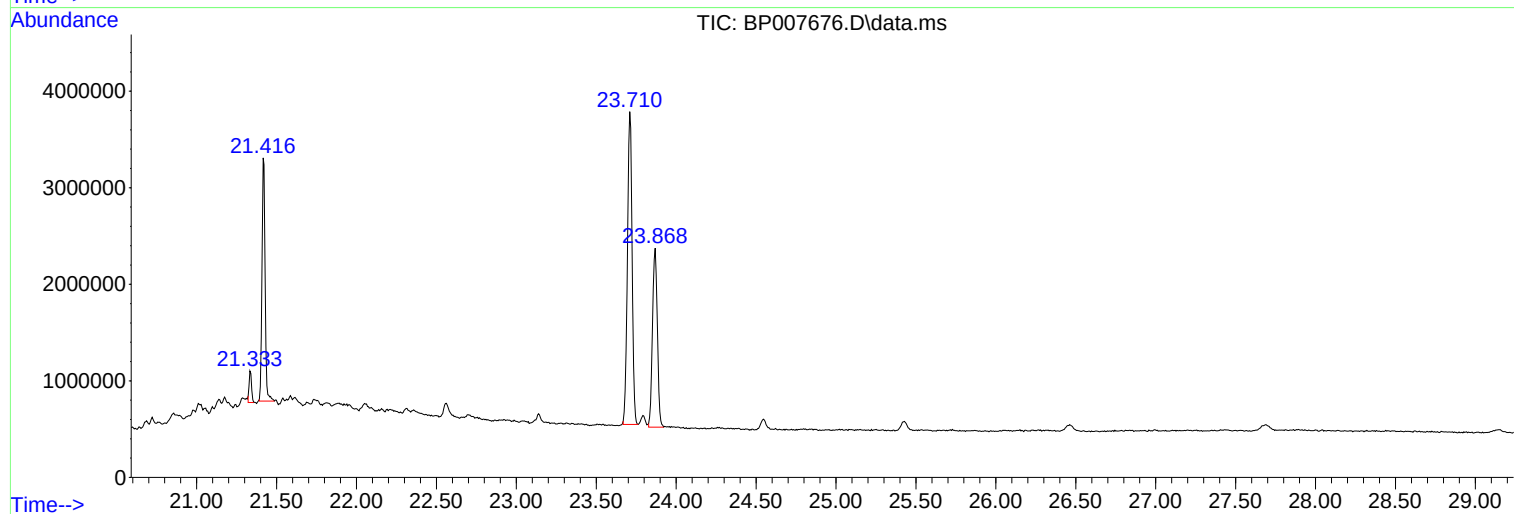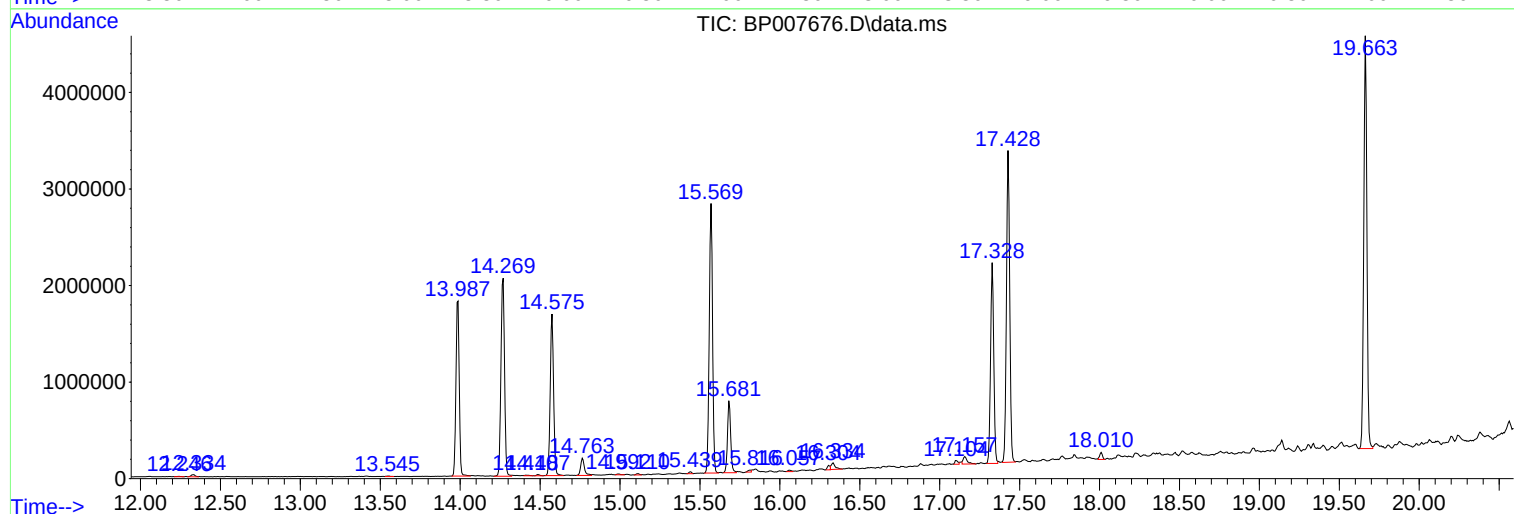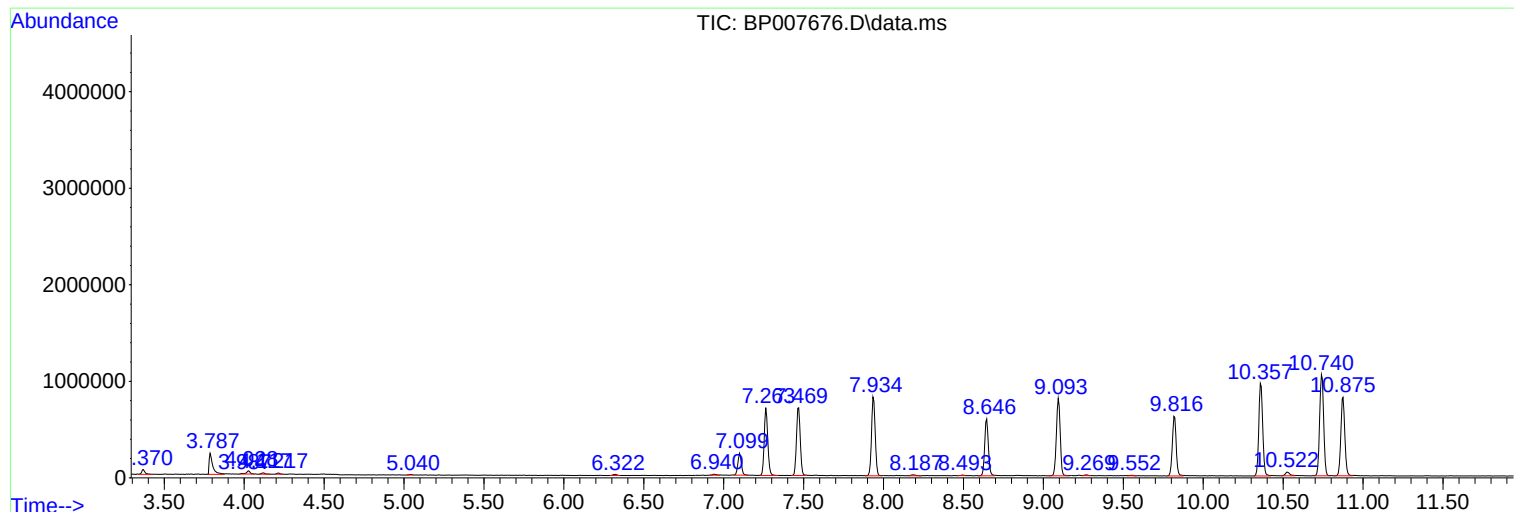

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007676.D
Acq On : 26 Oct 2021 11:47
Operator : CG/JU
Sample : M4291-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P045-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007676.D
Acq On : 26 Oct 2021 11:47
Operator : CG/JU
Sample : M4291-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P045-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
