

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007677.D
 Acq On : 26 Oct 2021 12:21
 Operator : CG/JU
 Sample : M4291-15
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P031-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	5	9	11	rBV	41094	52895	0.75%	0.095%
2	3.370	11	14	20	rVB	52163	66270	0.94%	0.119%
3	3.787	82	85	102	rBV	184946	304903	4.32%	0.547%
4	4.028	121	126	130	rBV	30166	43199	0.61%	0.077%
5	4.117	138	141	145	rVB	13554	15217	0.22%	0.027%
6	4.217	154	158	162	rBV5	12743	17697	0.25%	0.032%
7	5.040	294	298	304	rBV2	5118	8510	0.12%	0.015%
8	6.322	511	516	520	rVB3	10618	16504	0.23%	0.030%
9	6.946	619	622	625	rVB5	6250	7569	0.11%	0.014%
10	7.099	642	648	655	rVB	203649	314626	4.46%	0.564%
11	7.263	669	676	693	rVB	649474	1029585	14.60%	1.847%
12	7.469	703	711	721	rBV	670313	1077654	15.28%	1.933%
13	7.934	783	790	797	rBV	770619	1238428	17.56%	2.221%
14	8.181	825	832	839	rBV5	9297	19642	0.28%	0.035%
15	8.646	903	911	920	rBV	553677	900862	12.77%	1.616%
16	9.093	980	987	998	rBV	759614	1247822	17.69%	2.238%
17	9.269	1012	1017	1023	rVB9	7192	13372	0.19%	0.024%
18	9.816	1102	1110	1123	rBV	571580	964436	13.67%	1.730%
19	10.357	1195	1202	1223	rVB	935892	1586828	22.49%	2.846%
20	10.522	1223	1230	1242	rBV	59612	119672	1.70%	0.215%
21	10.740	1260	1267	1278	rBV	1026828	1746085	24.75%	3.132%
22	10.875	1282	1290	1302	rBV	789579	1365030	19.35%	2.448%
23	12.051	1486	1490	1493	rBV6	4448	7785	0.11%	0.014%
24	12.328	1530	1537	1543	rBV	22310	38228	0.54%	0.069%
25	13.193	1680	1684	1691	rVB9	6820	14178	0.20%	0.025%
26	13.487	1729	1734	1737	rBV7	5692	7994	0.11%	0.014%
27	13.545	1741	1744	1749	rVV5	8182	14200	0.20%	0.025%
28	13.987	1812	1819	1825	rBV	1827088	2591831	36.74%	4.649%
29	14.269	1855	1867	1877	rBV	2043095	3104105	44.00%	5.567%
30	14.575	1911	1919	1927	rBV	1633359	2444739	34.66%	4.385%
31	14.763	1945	1951	1962	rBV	192210	309427	4.39%	0.555%
32	14.992	1986	1990	1995	rBV8	9829	15339	0.22%	0.028%
33	15.387	2052	2057	2061	rBV6	5213	8918	0.13%	0.016%
34	15.439	2063	2066	2069	rBV3	7001	8521	0.12%	0.015%
35	15.569	2081	2088	2097	rBV	2886871	4108171	58.24%	7.368%
36	15.681	2100	2107	2118	rBV	832325	1167046	16.54%	2.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007677.D
 Acq On : 26 Oct 2021 12:21
 Operator : CG/JU
 Sample : M4291-15
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P031-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.810	2125	2129	2135	rVB3	19797	27037	0.38%	0.048%
38	16.228	2194	2200	2202	rBV6	11596	18345	0.26%	0.033%
39	16.304	2210	2213	2215	rBV4	9354	9080	0.13%	0.016%
40	16.881	2308	2311	2317	rVB8	6022	8069	0.11%	0.014%
41	17.045	2337	2339	2343	rVB5	7002	7694	0.11%	0.014%
42	17.104	2345	2349	2356	rVV3	17370	35810	0.51%	0.064%
43	17.157	2356	2358	2365	rVB8	9965	14444	0.20%	0.026%
44	17.328	2381	2387	2396	rVB	2046205	2988011	42.36%	5.359%
45	17.428	2398	2404	2416	rVV	3605786	5143993	72.92%	9.226%
46	17.522	2417	2420	2427	rVB9	17669	27947	0.40%	0.050%
47	17.710	2448	2452	2454	rBV4	5928	8251	0.12%	0.015%
48	17.810	2466	2469	2472	rBV5	12495	16874	0.24%	0.030%
49	17.845	2472	2475	2480	rVB5	11875	16436	0.23%	0.029%
50	17.928	2485	2489	2490	rBV4	6054	7966	0.11%	0.014%
51	18.010	2499	2503	2507	rVB	35356	45149	0.64%	0.081%
52	18.222	2536	2539	2544	rBV4	31046	40138	0.57%	0.072%
53	19.239	2708	2712	2716	rBV2	59558	76063	1.08%	0.136%
54	19.310	2720	2724	2728	rBV2	58877	79237	1.12%	0.142%
55	19.663	2778	2784	2791	rBV	4910645	6431936	91.18%	11.536%
56	21.422	3077	3083	3095	rBV	2752959	3798903	53.85%	6.813%
57	23.710	3465	3472	3481	rVB2	3380370	7054275	100.00%	12.652%
58	23.868	3492	3499	3509	rVB2	1902437	3903296	55.33%	7.001%




Sum of corrected areas: 55756242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007677.D
Acq On : 26 Oct 2021 12:21
Operator : CG/JU
Sample : M4291-15
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P031-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

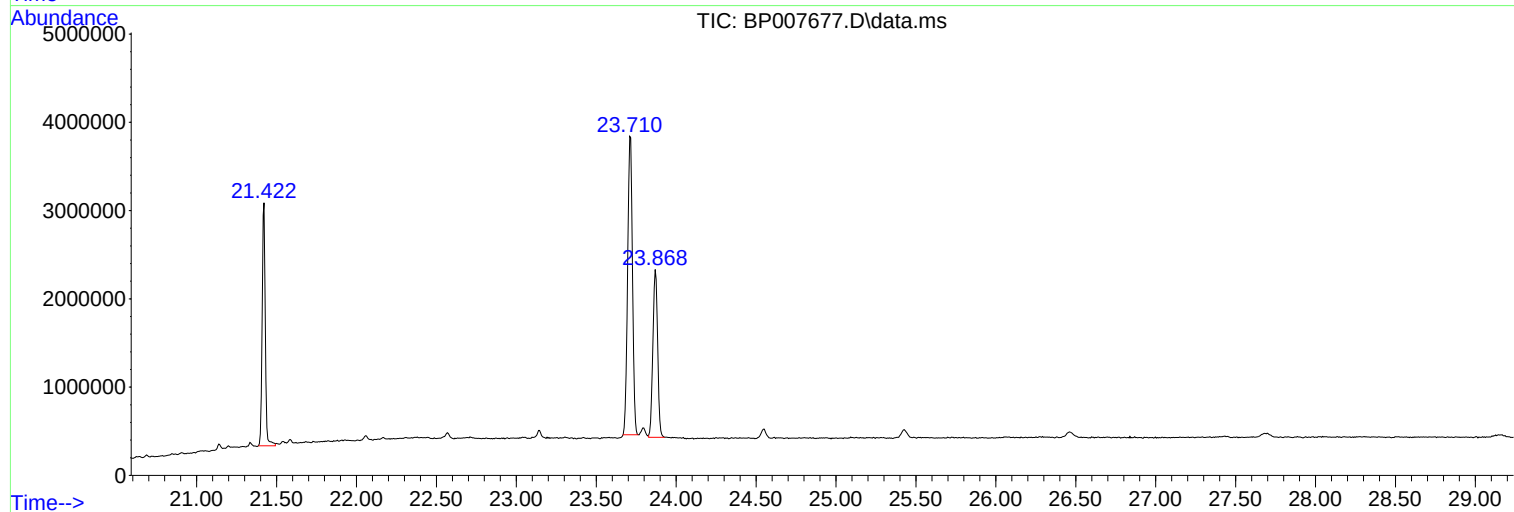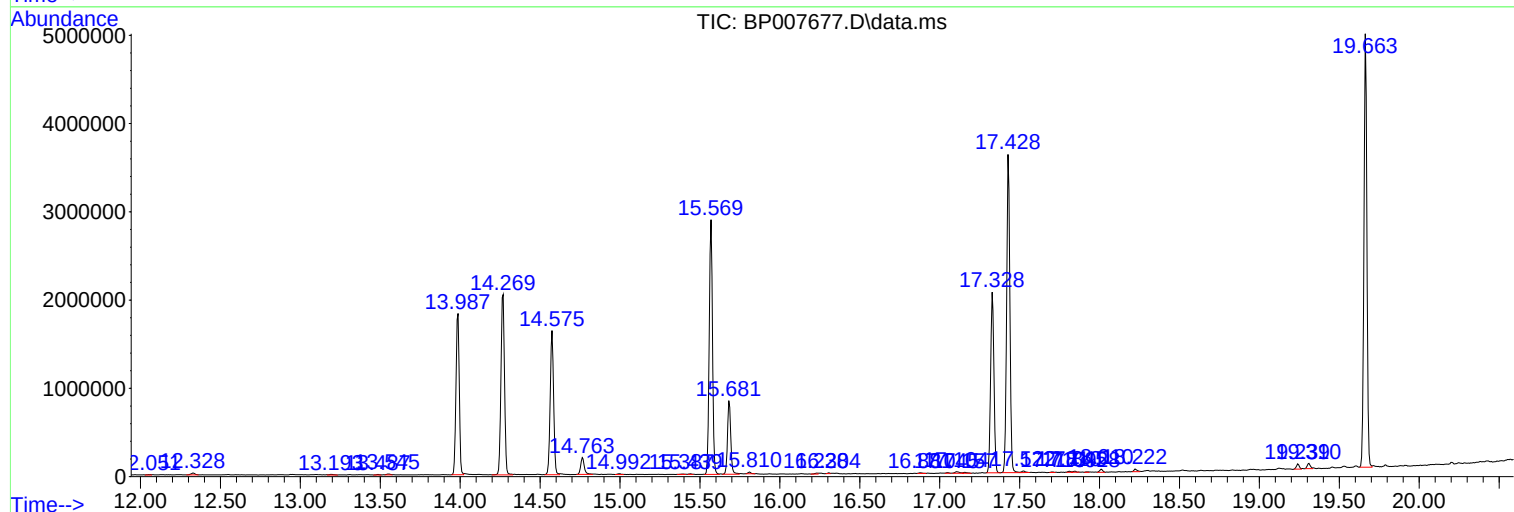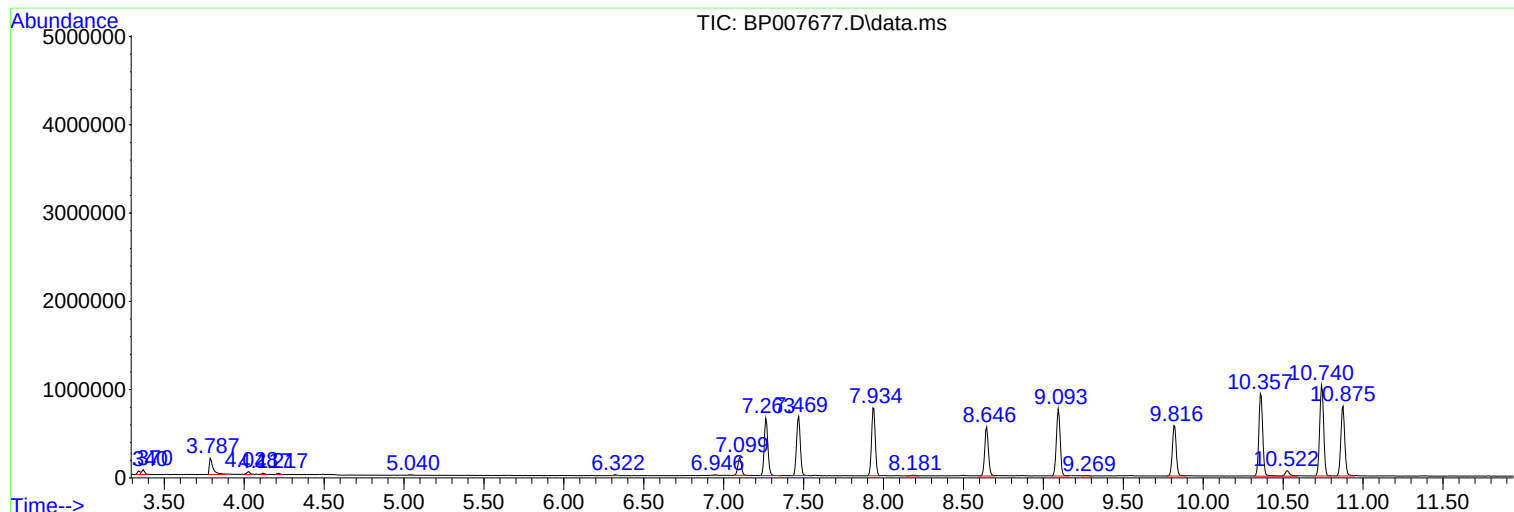

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007677.D
Acq On : 26 Oct 2021 12:21
Operator : CG/JU
Sample : M4291-15
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P031-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007677.D
Acq On : 26 Oct 2021 12:21
Operator : CG/JU
Sample : M4291-15
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P031-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
