

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007679.D
 Acq On : 26 Oct 2021 13:29
 Operator : CG/JU
 Sample : M4291-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P001-TW001-06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	21	rBV	40643	54154	1.06%	0.126%
2	3.793	83	86	103	rBV	84578	153706	3.01%	0.357%
3	4.028	121	126	134	rBV	30826	53299	1.04%	0.124%
4	4.117	137	141	148	rVB2	14420	22570	0.44%	0.052%
5	4.217	154	158	165	rVB5	12790	20212	0.40%	0.047%
6	5.040	295	298	302	rVB4	5578	6871	0.13%	0.016%
7	6.316	512	515	521	rVB3	10203	15044	0.29%	0.035%
8	6.940	619	621	628	rVB8	5227	9734	0.19%	0.023%
9	7.099	642	648	657	rVV	165035	263721	5.16%	0.613%
10	7.263	670	676	688	rVB	562431	875135	17.14%	2.034%
11	7.469	703	711	724	rBV	559356	903666	17.70%	2.101%
12	7.934	783	790	798	rVV	623416	1000256	19.59%	2.325%
13	8.010	798	803	806	rVB7	2874	5393	0.11%	0.013%
14	8.181	826	832	840	rBV9	9056	18390	0.36%	0.043%
15	8.493	880	885	891	rBV4	5472	8755	0.17%	0.020%
16	8.646	902	911	923	rBV	440573	732354	14.34%	1.702%
17	9.093	980	987	995	rBV	639421	1028913	20.15%	2.392%
18	9.275	1013	1018	1021	rVB6	3703	5974	0.12%	0.014%
19	9.552	1060	1065	1074	rVB10	6305	11857	0.23%	0.028%
20	9.816	1100	1110	1125	rBV	471722	795105	15.57%	1.848%
21	10.357	1194	1202	1213	rBV	748534	1265709	24.79%	2.942%
22	10.522	1225	1230	1238	rBV	66714	120624	2.36%	0.280%
23	10.740	1258	1267	1281	rVB	842255	1395919	27.34%	3.245%
24	10.875	1282	1290	1300	rBV	536214	948652	18.58%	2.205%
25	12.051	1486	1490	1493	rBV6	4325	5344	0.10%	0.012%
26	12.328	1532	1537	1541	rBV2	17393	27107	0.53%	0.063%
27	12.946	1638	1642	1648	rVB9	5276	7914	0.15%	0.018%
28	13.193	1681	1684	1689	rVB7	5466	8432	0.17%	0.020%
29	13.487	1729	1734	1741	rBV9	4386	9279	0.18%	0.022%
30	13.545	1741	1744	1747	rBV5	4204	5431	0.11%	0.013%
31	13.981	1812	1818	1835	rBV	1450940	2132485	41.76%	4.957%
32	14.263	1856	1866	1877	rBV	1592699	2424051	47.47%	5.635%
33	14.487	1900	1904	1908	rBV7	3311	5171	0.10%	0.012%
34	14.575	1911	1919	1928	rBV	1256578	1892384	37.06%	4.399%
35	14.763	1943	1951	1969	rBV	129032	225760	4.42%	0.525%
36	14.992	1985	1990	1998	rVB	7352	12011	0.24%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007679.D
 Acq On : 26 Oct 2021 13:29
 Operator : CG/JU
 Sample : M4291-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P001-TW001-06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.392	2052	2058	2063	rBV9	5531	12270	0.24%	0.029%
38	15.440	2063	2066	2072	rVB7	5148	7163	0.14%	0.017%
39	15.569	2081	2088	2098	rBV	2251916	3218961	63.04%	7.482%
40	15.681	2101	2107	2122	rVV	603791	842383	16.50%	1.958%
41	15.810	2125	2129	2135	rVB2	16650	27476	0.54%	0.064%
42	16.134	2180	2184	2189	rVB8	3081	5504	0.11%	0.013%
43	16.263	2198	2206	2213	rBV10	10022	20948	0.41%	0.049%
44	16.351	2219	2221	2229	rVB8	4637	8152	0.16%	0.019%
45	16.475	2236	2242	2248	rBV10	3480	8851	0.17%	0.021%
46	16.587	2256	2261	2265	rBV7	4179	7184	0.14%	0.017%
47	17.004	2327	2332	2336	rVB7	3966	7100	0.14%	0.017%
48	17.116	2346	2351	2357	rBV2	8346	15138	0.30%	0.035%
49	17.328	2380	2387	2397	rBV	1641823	2292275	44.89%	5.328%
50	17.428	2397	2404	2419	rVV2	2632825	3877708	75.94%	9.014%
51	17.710	2448	2452	2458	rVB9	4354	7021	0.14%	0.016%
52	18.010	2499	2503	2509	rVB6	15383	22964	0.45%	0.053%
53	18.222	2535	2539	2543	rBV3	52219	68227	1.34%	0.159%
54	19.239	2708	2712	2718	rBV3	40615	58533	1.15%	0.136%
55	19.310	2720	2724	2731	rVV	42300	60355	1.18%	0.140%
56	19.457	2746	2749	2752	rBV4	17903	20839	0.41%	0.048%
57	19.604	2771	2774	2777	rBV5	14390	18664	0.37%	0.043%
58	19.663	2778	2784	2791	rBV	3598968	4774311	93.50%	11.098%
59	21.139	3031	3035	3042	rBV6	90242	164451	3.22%	0.382%
60	21.416	3077	3082	3089	rBV	2083159	2861834	56.05%	6.652%
61	23.710	3465	3472	3482	rVB2	2556140	5106018	100.00%	11.869%
62	23.868	3492	3499	3511	rVB	1446198	3034810	59.44%	7.054%




Sum of corrected areas: 43020522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007679.D
Acq On : 26 Oct 2021 13:29
Operator : CG/JU
Sample : M4291-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW001-06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

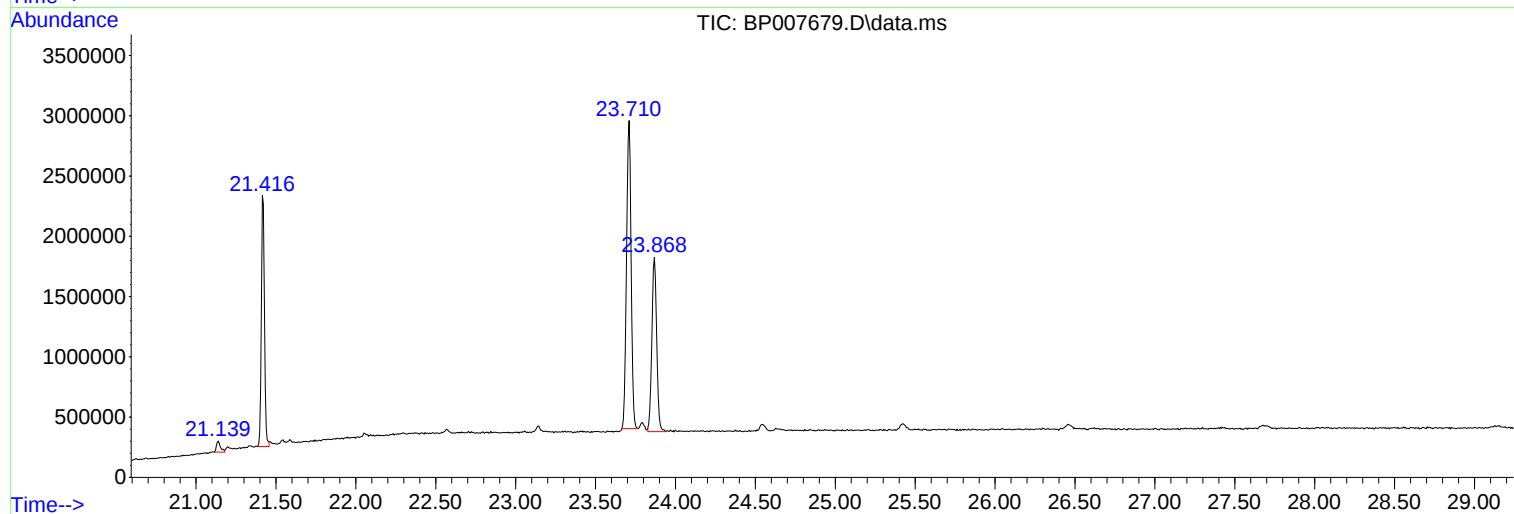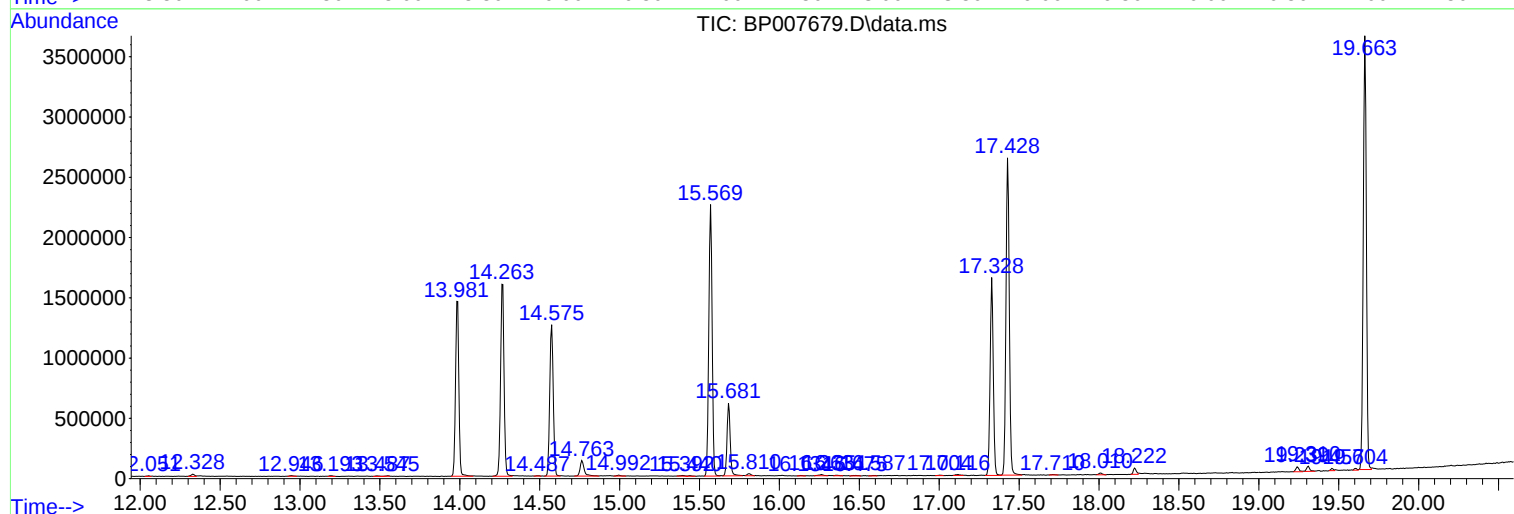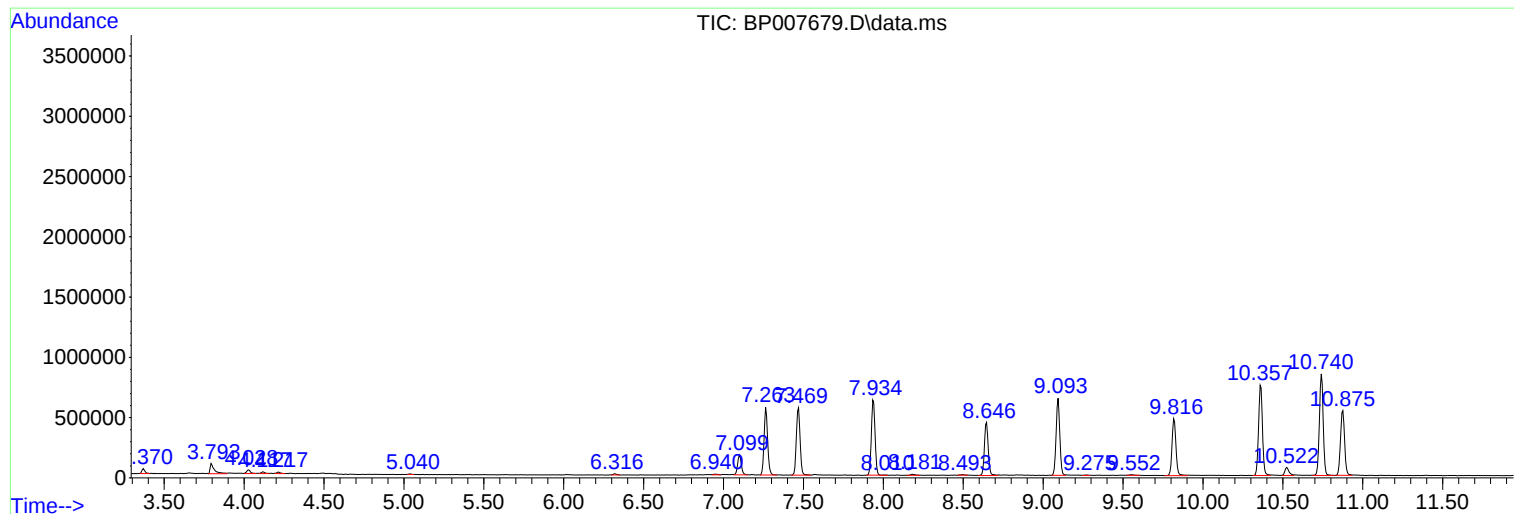

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007679.D
Acq On : 26 Oct 2021 13:29
Operator : CG/JU
Sample : M4291-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW001-06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007679.D
Acq On : 26 Oct 2021 13:29
Operator : CG/JU
Sample : M4291-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW001-06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
