

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007680.D
 Acq On : 26 Oct 2021 14:03
 Operator : CG/JU
 Sample : M4291-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P001-TW002-03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	5	9	11	rBV4	14832	20057	0.41%	0.048%
2	3.370	11	14	26	rVB	40577	56841	1.16%	0.135%
3	3.793	85	86	96	rBV	60100	97092	1.99%	0.231%
4	3.987	115	119	120	rBV4	3481	5267	0.11%	0.013%
5	4.028	121	126	130	rVV	27043	41658	0.85%	0.099%
6	4.117	138	141	145	rVB	12429	16331	0.33%	0.039%
7	4.217	154	158	162	rVB4	10394	15818	0.32%	0.038%
8	5.034	294	297	307	rVB6	7038	15777	0.32%	0.038%
9	6.322	511	516	524	rVB3	10976	18800	0.39%	0.045%
10	6.946	615	622	627	rBV8	6153	12526	0.26%	0.030%
11	7.099	640	648	657	rVB	178510	288014	5.90%	0.685%
12	7.264	670	676	686	rVB	559534	870014	17.82%	2.068%
13	7.469	704	711	723	rVB	562897	917436	18.79%	2.181%
14	7.569	723	728	734	rBV9	3919	7778	0.16%	0.018%
15	7.934	783	790	798	rBV	606619	980737	20.08%	2.331%
16	8.005	799	802	807	rVB7	4506	6652	0.14%	0.016%
17	8.187	826	833	840	rBV6	9633	18840	0.39%	0.045%
18	8.493	881	885	893	rVB7	5279	10596	0.22%	0.025%
19	8.646	904	911	922	rBV	465852	761404	15.59%	1.810%
20	9.093	980	987	998	rBV	632217	1037802	21.25%	2.467%
21	9.558	1058	1066	1070	rVB5	6278	13240	0.27%	0.031%
22	9.816	1099	1110	1124	rBV	464931	800367	16.39%	1.903%
23	10.358	1193	1202	1215	rBV	760400	1296547	26.55%	3.082%
24	10.522	1224	1230	1241	rBV2	52429	97285	1.99%	0.231%
25	10.740	1259	1267	1276	rBV	797851	1378007	28.22%	3.276%
26	10.875	1281	1290	1301	rBV	448783	789511	16.17%	1.877%
27	12.328	1530	1537	1543	rBV3	15897	28557	0.58%	0.068%
28	12.510	1562	1568	1573	rBV3	6820	12387	0.25%	0.029%
29	12.946	1637	1642	1646	rBV6	6828	11799	0.24%	0.028%
30	13.193	1678	1684	1690	rBV8	6410	13387	0.27%	0.032%
31	13.310	1700	1704	1708	rVB7	3376	5973	0.12%	0.014%
32	13.487	1728	1734	1738	rBV8	5174	8880	0.18%	0.021%
33	13.981	1811	1818	1832	rBV	1497216	2136842	43.76%	5.080%
34	14.263	1855	1866	1880	rBV	1597135	2455161	50.28%	5.836%
35	14.575	1910	1919	1930	rBV	1282442	1886490	38.63%	4.485%
36	14.763	1943	1951	1961	rBV	141660	235696	4.83%	0.560%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007680.D
 Acq On : 26 Oct 2021 14:03
 Operator : CG/JU
 Sample : M4291-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P001-TW002-03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.993	1989	1990	1998	rVB8	6576	6952	0.14%	0.017%
38	15.387	2052	2057	2063	rBV6	7302	14621	0.30%	0.035%
39	15.569	2078	2088	2101	rBV	2237932	3231902	66.19%	7.683%
40	15.681	2101	2107	2120	rVV	594367	837367	17.15%	1.991%
41	15.810	2123	2129	2136	rVB3	17527	31749	0.65%	0.075%
42	16.140	2178	2185	2187	rBV8	4409	8239	0.17%	0.020%
43	16.269	2200	2207	2211	rBV8	6559	12543	0.26%	0.030%
44	17.010	2329	2333	2337	rBV7	4337	6870	0.14%	0.016%
45	17.110	2346	2350	2355	rBV4	9048	15488	0.32%	0.037%
46	17.328	2380	2387	2396	rBV	1609042	2290272	46.90%	5.444%
47	17.428	2397	2404	2419	rVV	2679235	3761091	77.02%	8.941%
48	17.704	2446	2451	2453	rBV6	5048	7610	0.16%	0.018%
49	18.010	2499	2503	2508	rVB6	16530	24419	0.50%	0.058%
50	18.222	2535	2539	2546	rBV3	42215	62931	1.29%	0.150%
51	19.239	2708	2712	2716	rBV3	38461	54286	1.11%	0.129%
52	19.310	2720	2724	2727	rVV	37919	50908	1.04%	0.121%
53	19.457	2746	2749	2753	rBV6	14682	21768	0.45%	0.052%
54	19.663	2778	2784	2790	rBV	3495463	4597999	94.16%	10.930%
55	21.139	3031	3035	3038	rBV4	82451	114450	2.34%	0.272%
56	21.416	3077	3082	3088	rBV	2004162	2770164	56.73%	6.585%
57	23.710	3465	3472	3481	rVB2	2475090	4883003	100.00%	11.608%
58	23.869	3492	3499	3511	rVB2	1391715	2892039	59.23%	6.875%




Sum of corrected areas: 42066240

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007680.D
Acq On : 26 Oct 2021 14:03
Operator : CG/JU
Sample : M4291-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW002-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

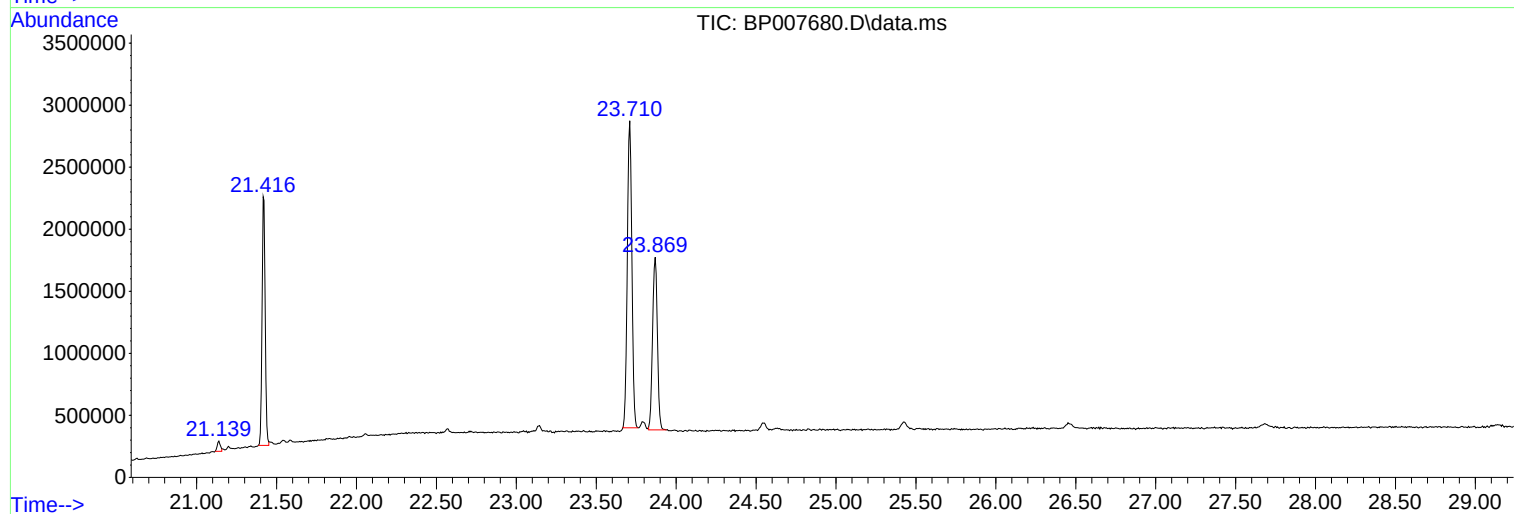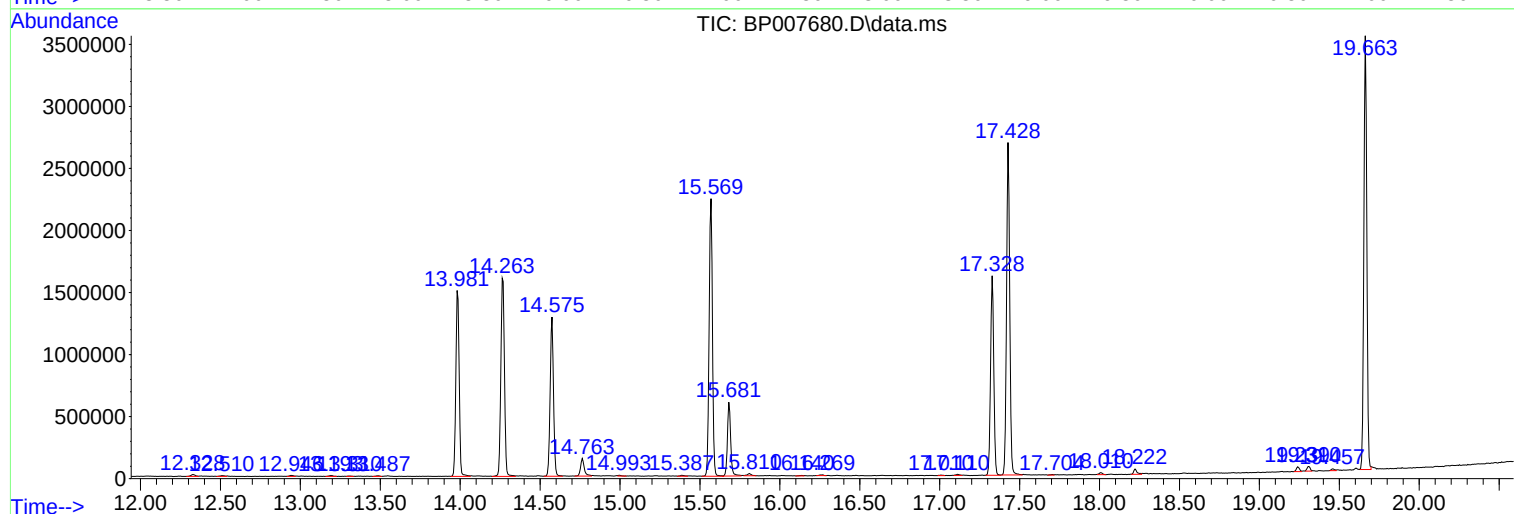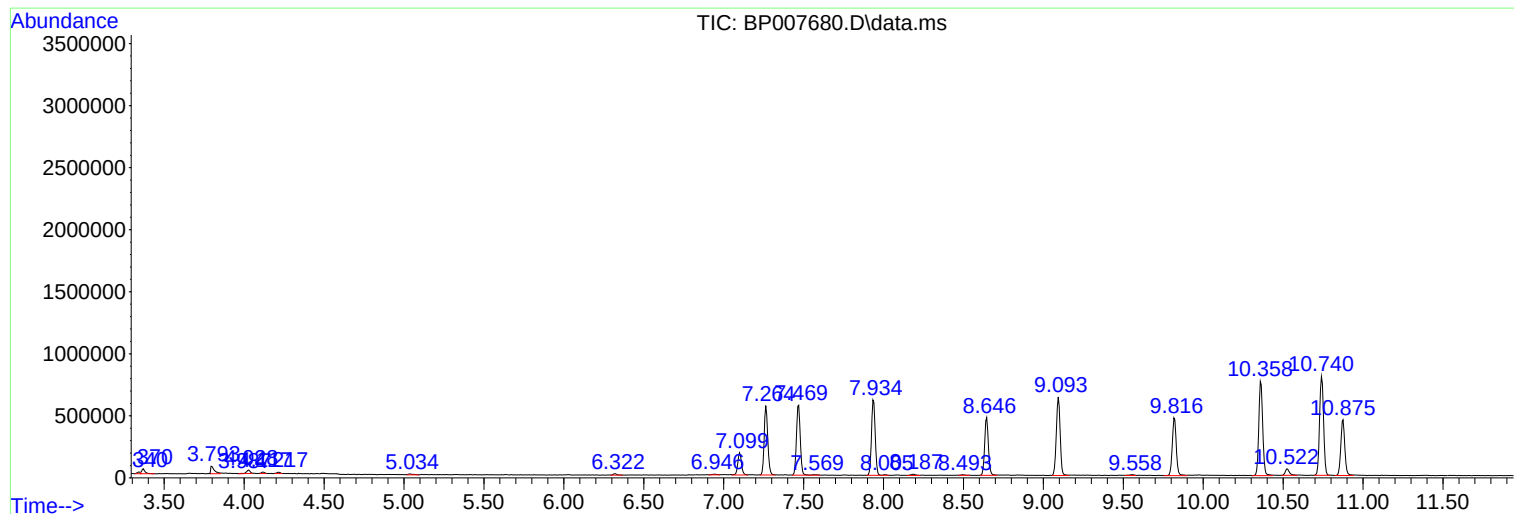

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007680.D
Acq On : 26 Oct 2021 14:03
Operator : CG/JU
Sample : M4291-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW002-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007680.D
Acq On : 26 Oct 2021 14:03
Operator : CG/JU
Sample : M4291-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P001-TW002-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
