

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007681.D
 Acq On : 26 Oct 2021 14:38
 Operator : CG/JU
 Sample : M4291-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P007-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	24	rVB	50632	72078	1.34%	0.165%
2	3.652	60	62	66	rVB3	5765	6452	0.12%	0.015%
3	3.787	82	85	99	rBV	159770	265003	4.93%	0.606%
4	4.028	120	126	131	rBV	30634	47135	0.88%	0.108%
5	4.116	137	141	148	rVB2	13738	21220	0.39%	0.049%
6	4.216	154	158	162	rVB4	11566	16603	0.31%	0.038%
7	4.487	201	204	206	rBV3	5747	8105	0.15%	0.019%
8	5.040	294	298	302	rBV	10226	14910	0.28%	0.034%
9	6.322	510	516	522	rVB2	11866	19085	0.35%	0.044%
10	7.099	641	648	657	rVB	289308	443988	8.25%	1.015%
11	7.263	669	676	687	rBV	557053	874940	16.27%	2.001%
12	7.469	704	711	720	rBV	627176	994667	18.49%	2.274%
13	7.934	783	790	798	rBV	537430	870081	16.18%	1.989%
14	8.187	826	833	841	rBV5	8965	17515	0.33%	0.040%
15	8.493	880	885	891	rBV8	8122	13943	0.26%	0.032%
16	8.646	902	911	921	rBV	591759	972729	18.09%	2.224%
17	9.093	979	987	997	rBV	632291	1038827	19.31%	2.375%
18	9.551	1063	1065	1069	rVB5	5411	7002	0.13%	0.016%
19	9.816	1103	1110	1119	rBV	468690	788162	14.65%	1.802%
20	10.357	1195	1202	1217	rBV	770505	1317250	24.49%	3.012%
21	10.522	1223	1230	1241	rBV	48963	94174	1.75%	0.215%
22	10.740	1257	1267	1277	rBV	731950	1239026	23.04%	2.833%
23	10.875	1281	1290	1300	rBV	649873	1100223	20.46%	2.516%
24	12.328	1532	1537	1544	rBV2	17241	29974	0.56%	0.069%
25	12.945	1634	1642	1646	rBV10	3256	7462	0.14%	0.017%
26	13.192	1677	1684	1686	rBV6	4796	7444	0.14%	0.017%
27	13.492	1728	1735	1738	rBV9	2507	5699	0.11%	0.013%
28	13.551	1738	1745	1750	rVB9	4667	8484	0.16%	0.019%
29	13.981	1812	1818	1826	rBV	1508375	2173302	40.41%	4.969%
30	14.263	1856	1866	1878	rBV	1673127	2506985	46.61%	5.732%
31	14.575	1912	1919	1929	rVV	1174372	1706896	31.73%	3.903%
32	14.763	1944	1951	1968	rBV	291264	448710	8.34%	1.026%
33	14.992	1985	1990	1995	rVB8	8494	13768	0.26%	0.031%
34	15.569	2081	2088	2097	rBV	2368442	3308729	61.52%	7.566%
35	15.681	2100	2107	2122	rVV	661596	928347	17.26%	2.123%
36	15.810	2122	2129	2136	rVB	18682	38242	0.71%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007681.D
 Acq On : 26 Oct 2021 14:38
 Operator : CG/JU
 Sample : M4291-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P007-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.263	2196	2206	2210	rBV	8678	22226	0.41%	0.051%
38	16.363	2218	2223	2229	rVB9	4718	9968	0.19%	0.023%
39	17.010	2329	2333	2339	rVB9	4040	6706	0.12%	0.015%
40	17.110	2346	2350	2354	rBV6	8394	15049	0.28%	0.034%
41	17.328	2381	2387	2396	rBV	1443727	2073185	38.54%	4.740%
42	17.428	2397	2404	2417	rBV2	2879613	4106984	76.36%	9.391%
43	18.010	2499	2503	2508	rVB7	13514	16596	0.31%	0.038%
44	18.222	2534	2539	2547	rBV3	53255	80525	1.50%	0.184%
45	19.239	2708	2712	2717	rBV	42487	56795	1.06%	0.130%
46	19.310	2720	2724	2731	rVB	43982	60005	1.12%	0.137%
47	19.457	2746	2749	2752	rBV3	23221	26360	0.49%	0.060%
48	19.604	2772	2774	2778	rVB5	18440	17678	0.33%	0.040%
49	19.663	2778	2784	2798	rBV	3830954	5040431	93.71%	11.525%
50	21.139	3031	3035	3042	rBV5	74544	134959	2.51%	0.309%
51	21.416	3077	3082	3089	rBV	1900303	2580921	47.98%	5.901%
52	23.710	3465	3472	3482	rBV2	2706112	5378623	100.00%	12.299%
53	23.868	3492	3499	3510	rVB2	1270006	2679699	49.82%	6.127%




Sum of corrected areas: 43733870

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007681.D
Acq On : 26 Oct 2021 14:38
Operator : CG/JU
Sample : M4291-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P007-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

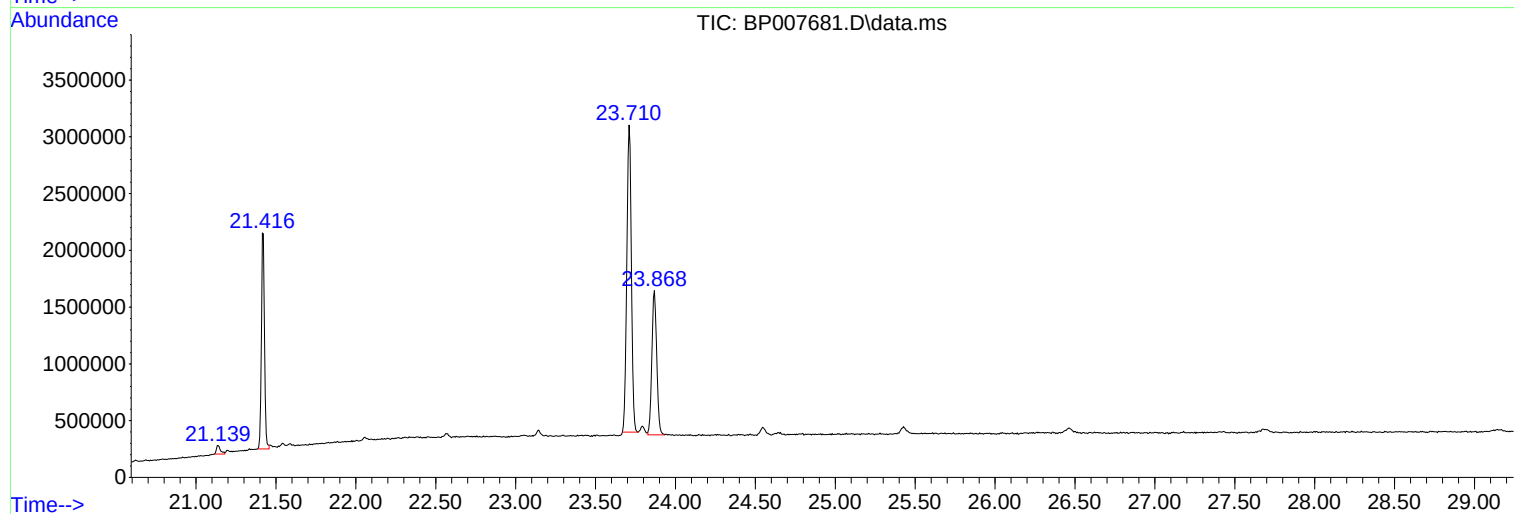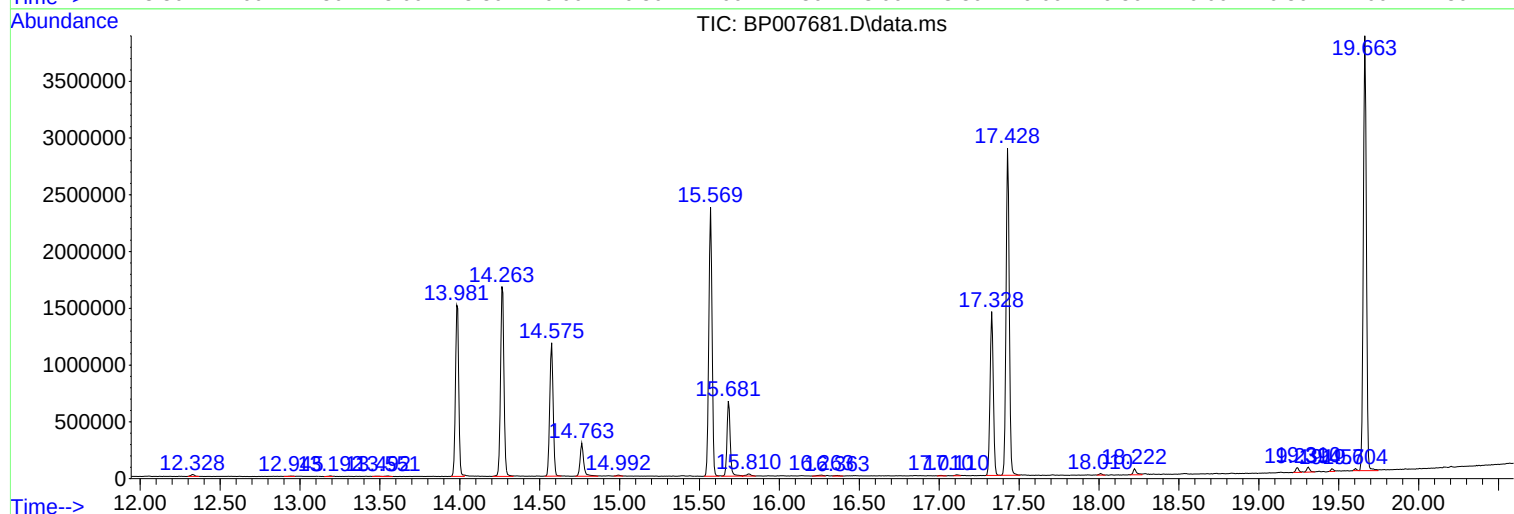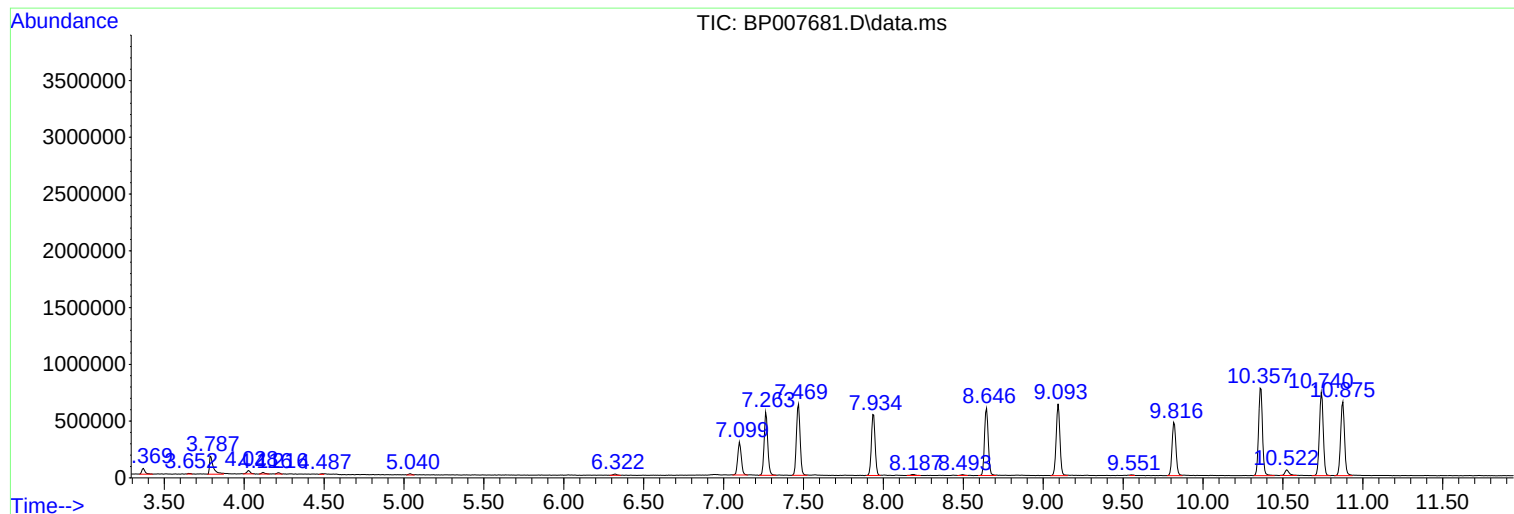

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007681.D
Acq On : 26 Oct 2021 14:38
Operator : CG/JU
Sample : M4291-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P007-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007681.D
Acq On : 26 Oct 2021 14:38
Operator : CG/JU
Sample : M4291-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P007-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
