

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007683.D
 Acq On : 26 Oct 2021 17:53
 Operator : CG/JU
 Sample : PB140168BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	21	rBV	48538	67177	1.35%	0.142%
2	3.781	81	84	104	rBV	695109	1021664	20.49%	2.153%
3	4.116	138	141	148	rVB	13166	18306	0.37%	0.039%
4	7.099	641	648	658	rVB	775194	1182525	23.72%	2.492%
5	7.263	669	676	687	rVB	595359	948281	19.02%	1.998%
6	7.463	703	710	718	rBV	771062	1225208	24.58%	2.582%
7	7.934	778	790	798	rBV	603721	948031	19.02%	1.998%
8	8.640	903	910	927	rBV	926498	1505889	30.21%	3.173%
9	9.093	979	987	996	rBV	697833	1128638	22.64%	2.378%
10	9.816	1102	1110	1120	rBV	558348	918461	18.42%	1.935%
11	10.357	1193	1202	1214	rBV	946282	1532141	30.73%	3.228%
12	10.740	1258	1267	1276	rBV	833274	1358293	27.25%	2.862%
13	10.869	1281	1289	1302	rBV	890320	1560746	31.31%	3.289%
14	12.328	1530	1537	1548	rVB	19835	35727	0.72%	0.075%
15	13.545	1741	1744	1749	rVB7	3598	5996	0.12%	0.013%
16	13.981	1811	1818	1831	rBV	1694398	2343560	47.01%	4.938%
17	14.263	1856	1866	1884	rBV	1859212	2735267	54.87%	5.764%
18	14.569	1911	1918	1926	rBV	1204346	1863892	37.39%	3.927%
19	14.763	1944	1951	1964	rBV	752630	1121194	22.49%	2.363%
20	14.992	1986	1990	1997	rVB8	3345	7298	0.15%	0.015%
21	15.563	2081	2087	2100	rBV	2286850	3480333	69.81%	7.334%
22	15.681	2100	2107	2119	rBV	635776	878239	17.62%	1.851%
23	15.804	2124	2128	2135	rVB3	19114	32010	0.64%	0.067%
24	16.133	2181	2184	2189	rBV6	3122	5329	0.11%	0.011%
25	16.245	2196	2203	2205	rBV8	5881	9146	0.18%	0.019%
26	16.357	2218	2222	2229	rBV9	3997	10035	0.20%	0.021%
27	17.010	2327	2333	2336	rBV8	3981	7611	0.15%	0.016%
28	17.110	2346	2350	2355	rBV2	8069	13420	0.27%	0.028%
29	17.328	2380	2387	2395	rBV	1642260	2295674	46.05%	4.837%
30	17.428	2397	2404	2419	rVV	2656499	3835479	76.93%	8.082%
31	17.704	2448	2451	2455	rVB4	3882	5233	0.10%	0.011%
32	18.004	2498	2502	2505	rBV5	3772	6041	0.12%	0.013%
33	19.239	2709	2712	2717	rVB3	37240	42944	0.86%	0.090%
34	19.310	2719	2724	2728	rBV	35229	50451	1.01%	0.106%
35	19.663	2778	2784	2793	rBV	3502915	4664548	93.56%	9.829%
36	21.416	3077	3082	3088	rBV	2116221	2749497	55.15%	5.794%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007683.D
Acq On : 26 Oct 2021 17:53
Operator : CG/JU
Sample : PB140168BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Title : SVOA CALIBRATION

37	23.704	3464	3471	3481	rBV2	2420270	4985377	100.00%	10.505%
38	23.862	3492	3498	3509	rVB2	1363774	2858216	57.33%	6.023%


Sum of corrected areas: 47457877

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007683.D
Acq On : 26 Oct 2021 17:53
Operator : CG/JU
Sample : PB140168BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

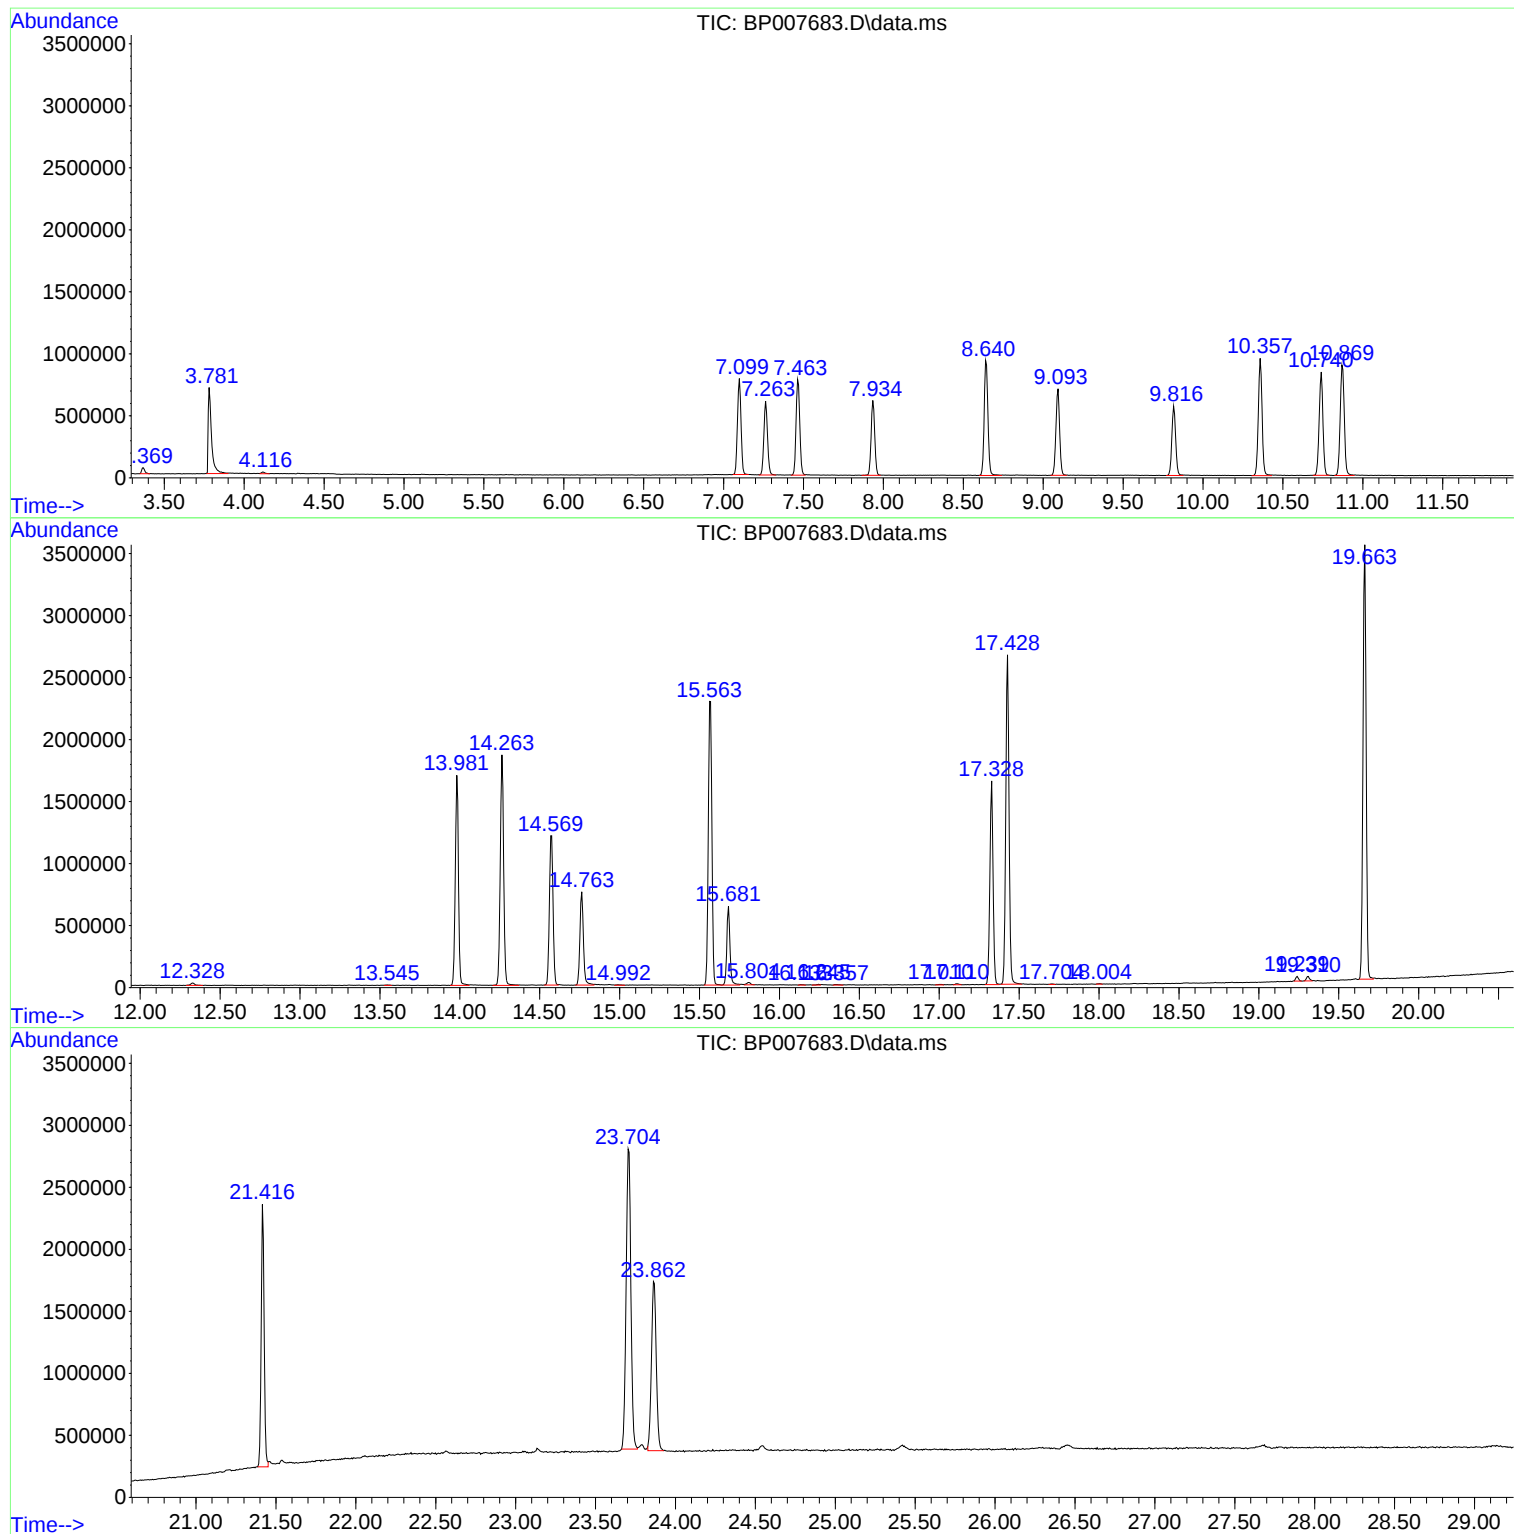

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007683.D
Acq On : 26 Oct 2021 17:53
Operator : CG/JU
Sample : PB140168BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007683.D
Acq On : 26 Oct 2021 17:53
Operator : CG/JU
Sample : PB140168BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
