

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007684.D
 Acq On : 26 Oct 2021 18:27
 Operator : CG/JU
 Sample : PB140178BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	9	13	22	rVB	50354	68427	1.46%	0.152%
2	3.781	81	84	103	rBV	675454	992023	21.10%	2.202%
3	4.117	138	141	145	rVB2	12023	16260	0.35%	0.036%
4	7.099	641	648	661	rVB	732638	1156573	24.60%	2.567%
5	7.264	669	676	692	rVB	588410	938252	19.96%	2.083%
6	7.464	703	710	721	rBV	739256	1185397	25.21%	2.631%
7	7.934	784	790	801	rVB	559295	872631	18.56%	1.937%
8	8.640	902	910	923	rBV	900454	1458374	31.02%	3.237%
9	9.093	978	987	997	rBV	662330	1095217	23.29%	2.431%
10	9.816	1102	1110	1126	rBV	535960	881822	18.76%	1.957%
11	10.358	1194	1202	1214	rBV	886723	1477423	31.42%	3.279%
12	10.740	1259	1267	1278	rVB	732868	1256497	26.72%	2.789%
13	10.869	1281	1289	1299	rBV	890309	1500163	31.91%	3.330%
14	12.328	1532	1537	1542	rBV2	17120	28562	0.61%	0.063%
15	13.546	1740	1744	1747	rBV4	4113	5921	0.13%	0.013%
16	13.981	1811	1818	1834	rBV	1593634	2253635	47.93%	5.002%
17	14.263	1859	1866	1878	rBV	1827049	2607603	55.46%	5.788%
18	14.569	1910	1918	1928	rBV	1145937	1730762	36.81%	3.842%
19	14.763	1944	1951	1965	rBV	735106	1074394	22.85%	2.385%
20	14.928	1977	1979	1983	rVB4	3470	5358	0.11%	0.012%
21	15.569	2081	2088	2100	rVB	2226952	3346464	71.18%	7.428%
22	15.681	2101	2107	2120	rBV	577459	813900	17.31%	1.807%
23	15.804	2125	2128	2138	rVB2	16828	28599	0.61%	0.063%
24	17.104	2347	2349	2357	rBV3	6276	11200	0.24%	0.025%
25	17.328	2379	2387	2395	rBV	1514984	2117775	45.04%	4.701%
26	17.428	2397	2404	2425	rVB	2554576	3681626	78.30%	8.172%
27	19.239	2708	2712	2718	rBV2	37836	51601	1.10%	0.115%
28	19.304	2720	2723	2727	rVV	33346	42231	0.90%	0.094%
29	19.663	2778	2784	2795	rBV	3305416	4460650	94.87%	9.901%
30	21.416	3077	3082	3094	rBV	1980187	2573593	54.74%	5.713%
31	23.704	3464	3471	3481	rBV2	2365435	4701714	100.00%	10.436%
32	23.863	3492	3498	3509	rVB2	1294015	2616203	55.64%	5.807%




Sum of corrected areas: 45050850

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007684.D
Acq On : 26 Oct 2021 18:27
Operator : CG/JU
Sample : PB140178BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK178

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

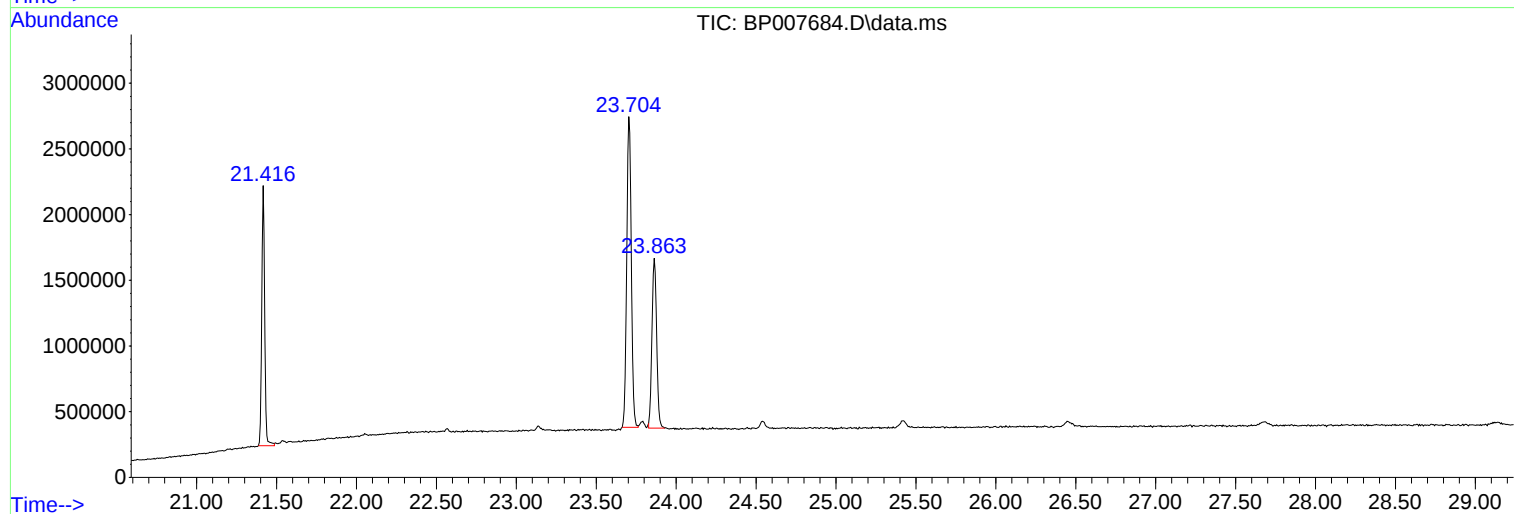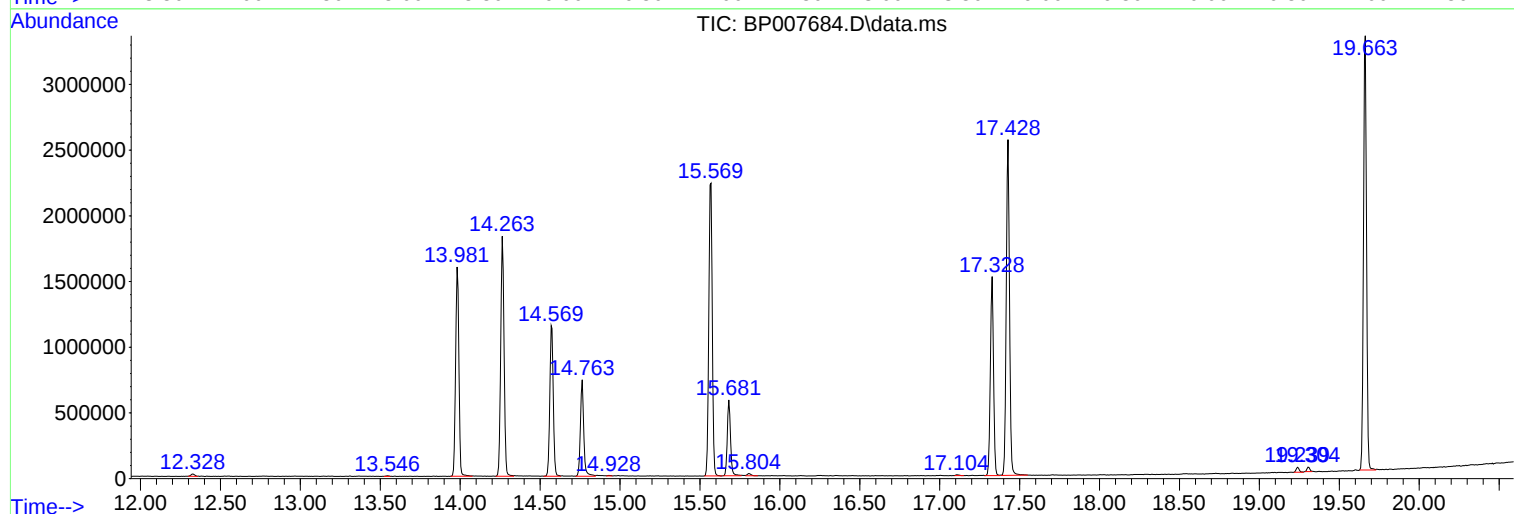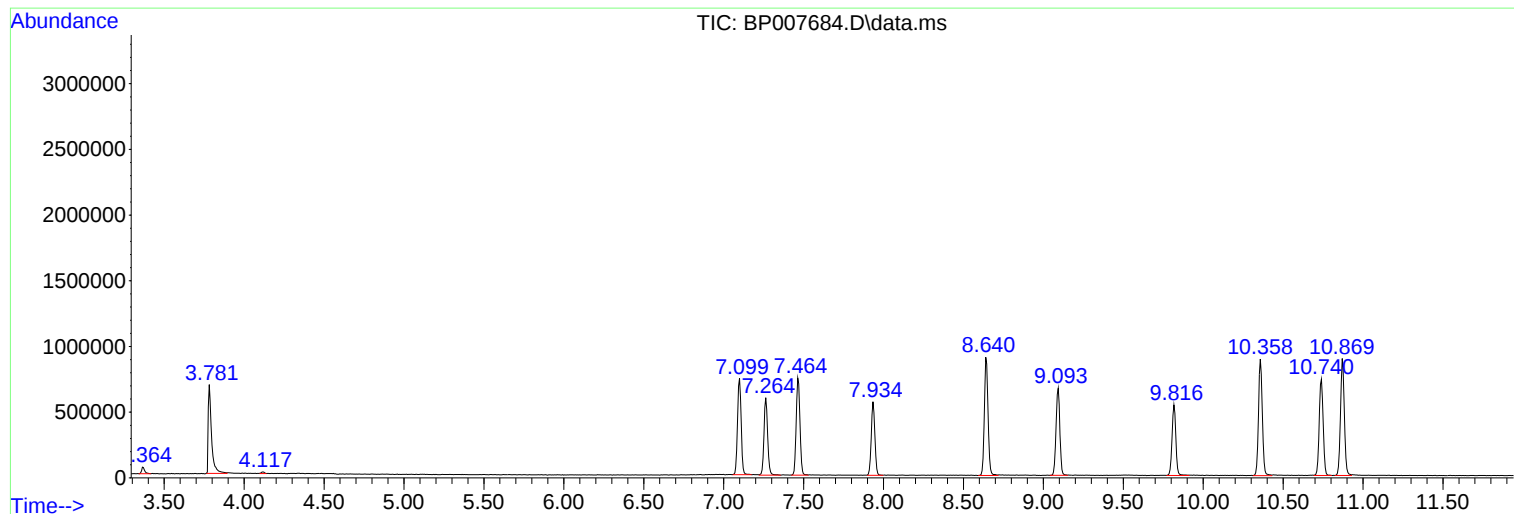

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007684.D
Acq On : 26 Oct 2021 18:27
Operator : CG/JU
Sample : PB140178BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK178

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007684.D
Acq On : 26 Oct 2021 18:27
Operator : CG/JU
Sample : PB140178BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK178

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc