

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007687.D
 Acq On : 26 Oct 2021 20:09
 Operator : CG/JU
 Sample : M4291-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P002-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	20	rVB	36536	50111	0.87%	0.101%
2	3.787	83	85	99	rBV	236136	368460	6.40%	0.745%
3	4.028	121	126	130	rVB	27263	41066	0.71%	0.083%
4	4.116	138	141	146	rVB	16375	21571	0.37%	0.044%
5	4.210	154	157	163	rVB5	12227	17899	0.31%	0.036%
6	5.034	294	297	304	rVB3	8468	14345	0.25%	0.029%
7	6.316	511	515	520	rVB2	12959	16692	0.29%	0.034%
8	6.940	619	621	627	rVB7	5057	8895	0.15%	0.018%
9	7.099	641	648	655	rVB	200421	314264	5.46%	0.636%
10	7.263	669	676	692	rVB	605741	963009	16.74%	1.948%
11	7.463	703	710	720	rBV	636724	1014601	17.63%	2.053%
12	7.934	782	790	798	rBV	706556	1092518	18.99%	2.210%
13	8.010	800	803	808	rVB6	4792	7960	0.14%	0.016%
14	8.187	825	833	837	rBV9	8284	17836	0.31%	0.036%
15	8.487	881	884	888	rBV5	5347	7872	0.14%	0.016%
16	8.640	903	910	921	rBV	544221	868309	15.09%	1.757%
17	9.093	979	987	996	rBV	718391	1160313	20.17%	2.348%
18	9.269	1011	1017	1020	rBV7	6077	9896	0.17%	0.020%
19	9.551	1059	1065	1072	rVB10	6993	13031	0.23%	0.026%
20	9.816	1103	1110	1123	rBV	556679	904789	15.72%	1.831%
21	10.357	1195	1202	1213	rBV	867707	1446364	25.14%	2.926%
22	10.522	1225	1230	1239	rBV2	52347	97085	1.69%	0.196%
23	10.740	1258	1267	1274	rBV	913102	1539969	26.76%	3.116%
24	10.869	1281	1289	1299	rBV	771499	1338551	23.26%	2.708%
25	12.328	1532	1537	1540	rBV3	18614	32810	0.57%	0.066%
26	12.363	1540	1543	1549	rVB2	23041	35853	0.62%	0.073%
27	13.486	1730	1734	1738	rBV7	3391	5782	0.10%	0.012%
28	13.539	1738	1743	1750	rVB10	7775	14709	0.26%	0.030%
29	13.904	1799	1805	1809	rBV7	3885	7668	0.13%	0.016%
30	13.981	1811	1818	1825	rBV	1794074	2464451	42.83%	4.986%
31	14.263	1856	1866	1875	rBV	1945336	2810770	48.85%	5.687%
32	14.569	1910	1918	1925	rBV	1390746	2145052	37.28%	4.340%
33	14.763	1939	1951	1961	rBV	177440	294519	5.12%	0.596%
34	14.992	1984	1990	1997	rVB	8005	14649	0.25%	0.030%
35	15.228	2026	2030	2037	rVB9	4203	7590	0.13%	0.015%
36	15.392	2053	2058	2061	rBV7	4552	8150	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007687.D
 Acq On : 26 Oct 2021 20:09
 Operator : CG/JU
 Sample : M4291-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P002-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.569	2080	2088	2097	rBV	2566778	3801259	66.06%	7.691%
38	15.680	2100	2107	2120	rBV	731238	989978	17.21%	2.003%
39	15.810	2124	2129	2134	rVB2	17245	28501	0.50%	0.058%
40	16.139	2180	2185	2189	rBV8	3298	5795	0.10%	0.012%
41	16.251	2199	2204	2210	rBV10	6767	16124	0.28%	0.033%
42	16.357	2218	2222	2227	rVB7	6189	10931	0.19%	0.022%
43	16.827	2297	2302	2303	rBV5	4504	6659	0.12%	0.013%
44	17.004	2329	2332	2336	rVB6	5371	6761	0.12%	0.014%
45	17.110	2344	2350	2354	rBV4	10365	17495	0.30%	0.035%
46	17.327	2380	2387	2397	rBV	1881096	2626262	45.64%	5.313%
47	17.427	2397	2404	2416	rVV	3213432	4439959	77.16%	8.983%
48	17.522	2416	2420	2424	rVV7	22838	37351	0.65%	0.076%
49	17.569	2426	2428	2434	rVB2	9245	10165	0.18%	0.021%
50	18.010	2499	2503	2506	rVB5	12584	14042	0.24%	0.028%
51	18.222	2532	2539	2546	rBV3	52420	80979	1.41%	0.164%
52	18.527	2588	2591	2595	rVB6	7681	12055	0.21%	0.024%
53	19.239	2708	2712	2718	rBV3	49938	68398	1.19%	0.138%
54	19.304	2719	2723	2730	rVV	48259	73481	1.28%	0.149%
55	19.457	2746	2749	2752	rBV3	19619	25717	0.45%	0.052%
56	19.604	2771	2774	2777	rBV3	16283	17724	0.31%	0.036%
57	19.663	2778	2784	2790	rBV	4134973	5481263	95.26%	11.090%
58	21.133	3031	3034	3039	rBV5	62971	99257	1.73%	0.201%
59	21.415	3077	3082	3094	rBV	2436025	3243482	56.37%	6.562%
60	23.704	3464	3471	3480	rBV2	2892071	5753927	100.00%	11.641%
61	23.862	3491	3498	3510	rVB2	1600874	3382155	58.78%	6.843%




Sum of corrected areas: 49427129

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007687.D
Acq On : 26 Oct 2021 20:09
Operator : CG/JU
Sample : M4291-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P002-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

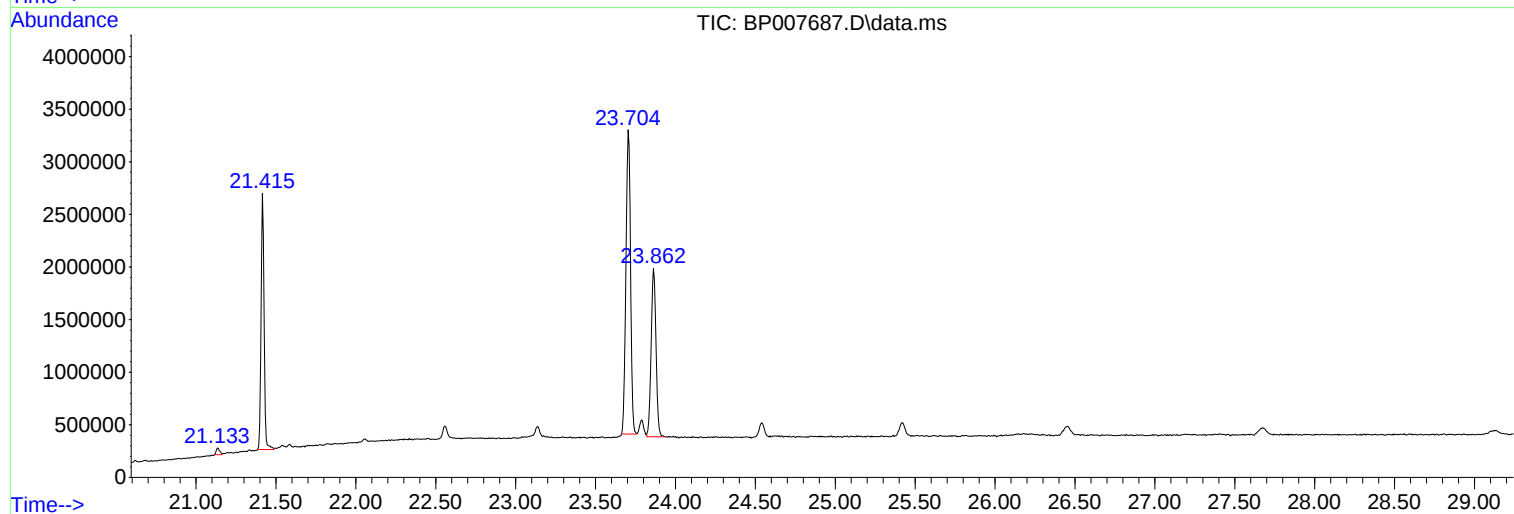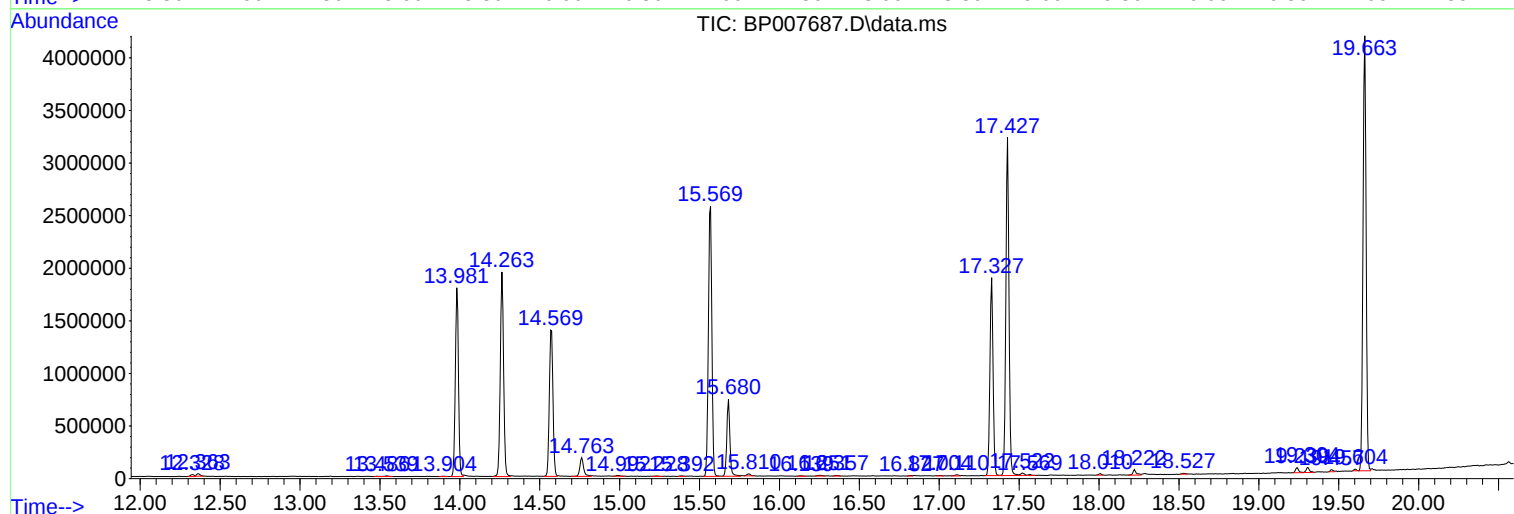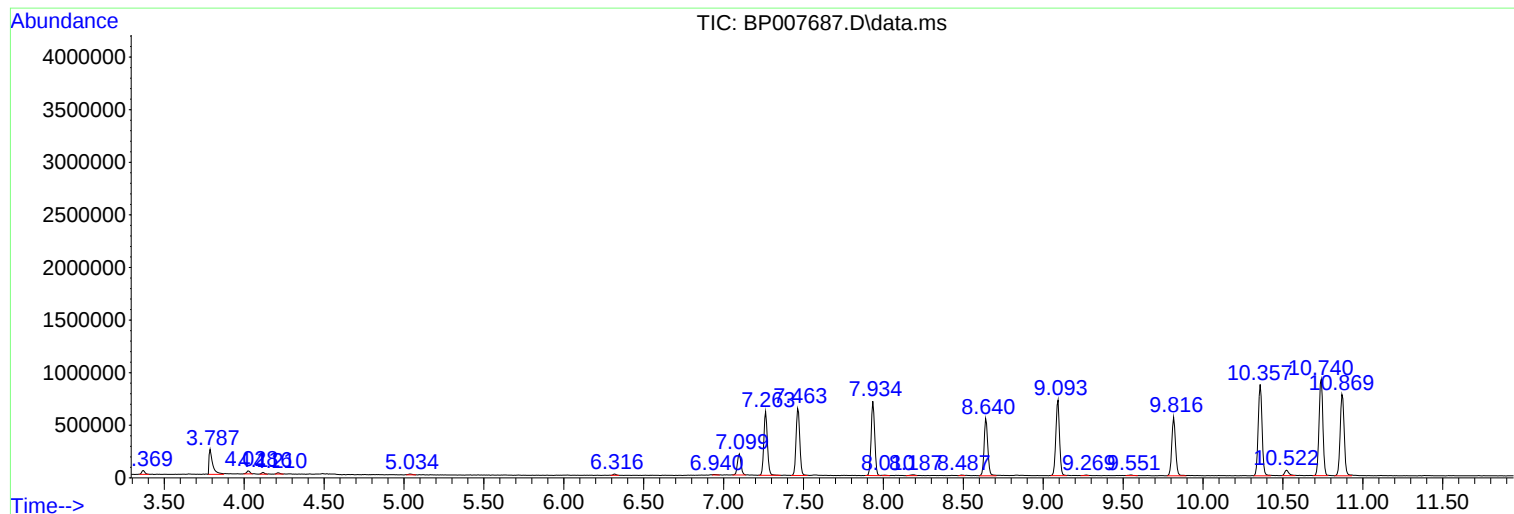

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007687.D
Acq On : 26 Oct 2021 20:09
Operator : CG/JU
Sample : M4291-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P002-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007687.D
Acq On : 26 Oct 2021 20:09
Operator : CG/JU
Sample : M4291-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P002-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
