

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007689.D
 Acq On : 26 Oct 2021 21:17
 Operator : CG/JU
 Sample : M4291-21
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P046-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	6	8	11	rBV4	10056	14696	0.24%	0.029%
2	3.370	11	14	19	rVB	47787	59235	0.98%	0.117%
3	3.787	82	85	99	rBV	200201	325656	5.40%	0.641%
4	4.028	121	126	134	rVB2	33153	55651	0.92%	0.110%
5	4.117	138	141	149	rVB2	13726	21370	0.35%	0.042%
6	4.217	154	158	163	rVB5	14047	24008	0.40%	0.047%
7	5.040	294	298	303	rVB3	9214	14801	0.25%	0.029%
8	6.317	511	515	521	rVB3	10172	15895	0.26%	0.031%
9	6.946	618	622	626	rVB5	4684	7178	0.12%	0.014%
10	7.099	641	648	658	rVB	186746	310393	5.14%	0.611%
11	7.264	670	676	688	rBV	621615	977596	16.20%	1.924%
12	7.464	704	710	720	rBV	638027	1012295	16.77%	1.993%
13	7.934	783	790	798	rBV	728774	1137478	18.84%	2.239%
14	8.181	827	832	839	rVB6	8112	14044	0.23%	0.028%
15	8.640	904	910	924	rBV	521373	837767	13.88%	1.649%
16	9.087	979	986	999	rBV	697187	1181185	19.57%	2.325%
17	9.546	1059	1064	1069	rVB7	5245	9134	0.15%	0.018%
18	9.816	1103	1110	1122	rBV	540066	897648	14.87%	1.767%
19	10.357	1194	1202	1212	rBV	876481	1442206	23.89%	2.839%
20	10.528	1226	1231	1236	rBV6	9965	19625	0.33%	0.039%
21	10.740	1259	1267	1275	rBV	926210	1594150	26.41%	3.138%
22	10.869	1281	1289	1304	rBV	841299	1446367	23.96%	2.847%
23	12.328	1532	1537	1542	rBV2	17819	27306	0.45%	0.054%
24	12.940	1636	1641	1644	rBV6	4920	9549	0.16%	0.019%
25	13.546	1739	1744	1749	rBV8	5384	11848	0.20%	0.023%
26	13.981	1810	1818	1832	rBV	1818331	2499064	41.40%	4.919%
27	14.087	1834	1836	1844	rVB9	3004	6950	0.12%	0.014%
28	14.263	1858	1866	1873	rBV	1917701	2822941	46.77%	5.556%
29	14.569	1910	1918	1927	rBV	1475866	2243685	37.17%	4.416%
30	14.763	1944	1951	1964	rBV	165796	282601	4.68%	0.556%
31	14.993	1984	1990	1996	rBV10	13004	21338	0.35%	0.042%
32	15.569	2080	2088	2099	rBV	2585728	3880127	64.28%	7.637%
33	15.681	2099	2107	2120	rBV	740145	1030753	17.08%	2.029%
34	15.810	2125	2129	2133	rVB4	16753	24368	0.40%	0.048%
35	16.245	2199	2203	2208	rBV8	6315	11029	0.18%	0.022%
36	16.328	2213	2217	2220	rBV4	9739	13174	0.22%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007689.D
 Acq On : 26 Oct 2021 21:17
 Operator : CG/JU
 Sample : M4291-21
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P046-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.004	2327	2332	2334	rBV6	4473	6919	0.11%	0.014%
38	17.110	2345	2350	2354	rBV3	9694	17289	0.29%	0.034%
39	17.157	2354	2358	2362	rVB4	9091	13007	0.22%	0.026%
40	17.328	2379	2387	2397	rBV	1904234	2775584	45.98%	5.463%
41	17.428	2397	2404	2417	rVV	3203531	4616420	76.48%	9.087%
42	17.516	2417	2419	2427	rVB9	11302	20377	0.34%	0.040%
43	17.698	2447	2450	2454	rBV4	6811	10798	0.18%	0.021%
44	18.004	2500	2502	2506	rVB4	9893	11270	0.19%	0.022%
45	18.222	2531	2539	2547	rBV3	53714	106167	1.76%	0.209%
46	19.239	2707	2712	2718	rBV	47613	68191	1.13%	0.134%
47	19.304	2719	2723	2730	rVV	48672	69053	1.14%	0.136%
48	19.457	2745	2749	2752	rBV5	26861	37621	0.62%	0.074%
49	19.604	2770	2774	2777	rBV5	17930	24745	0.41%	0.049%
50	19.657	2778	2783	2791	rBV	4014977	5677012	94.05%	11.174%
51	20.569	2935	2938	2942	rVB2	33414	39025	0.65%	0.077%
52	21.416	3077	3082	3093	rBV	2585451	3407805	56.46%	6.708%
53	23.704	3464	3471	3481	rVB2	3058342	6036079	100.00%	11.881%
54	23.863	3491	3498	3509	rVB2	1711411	3563869	59.04%	7.015%




Sum of corrected areas: 50804342

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007689.D
Acq On : 26 Oct 2021 21:17
Operator : CG/JU
Sample : M4291-21
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P046-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

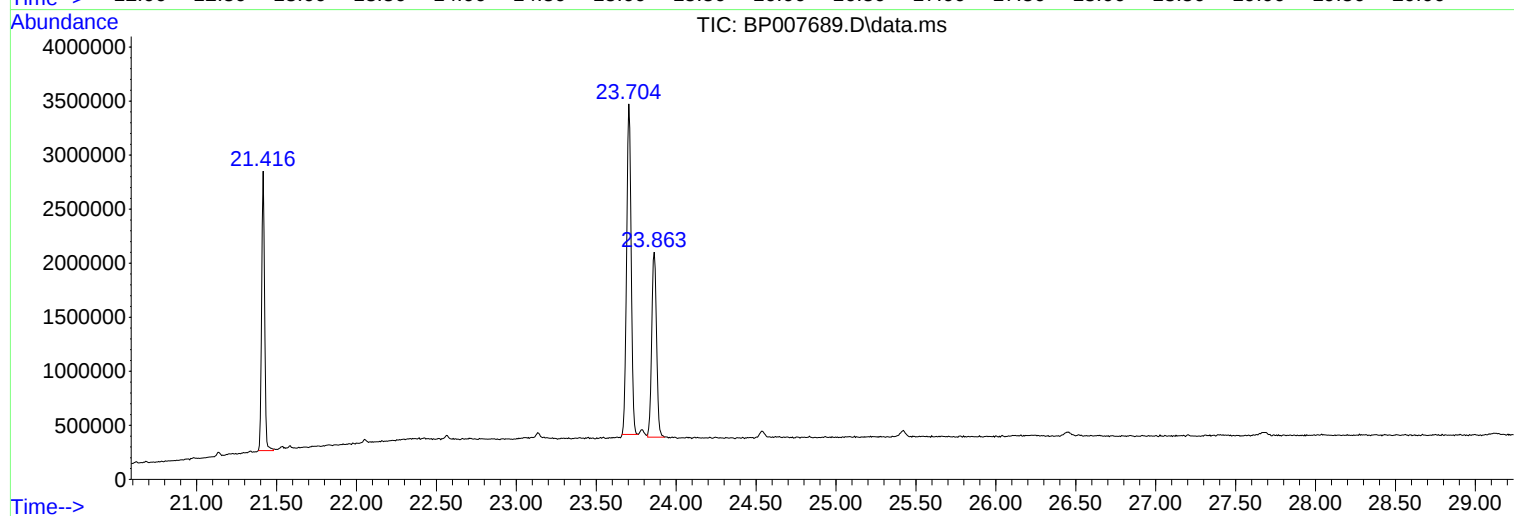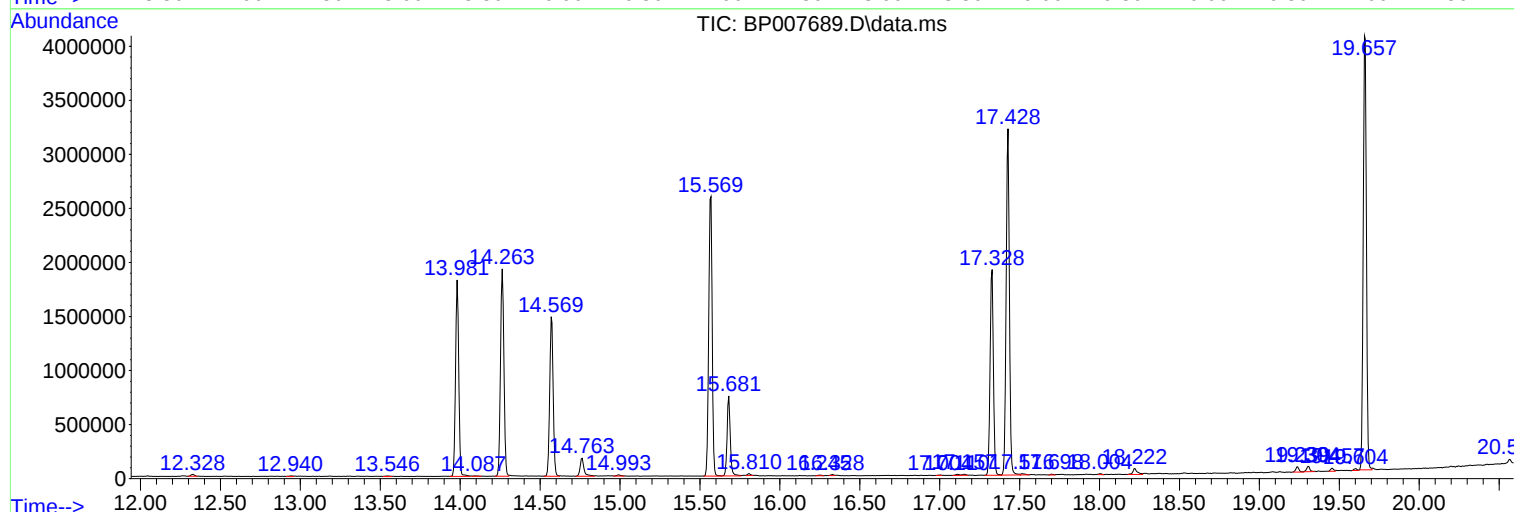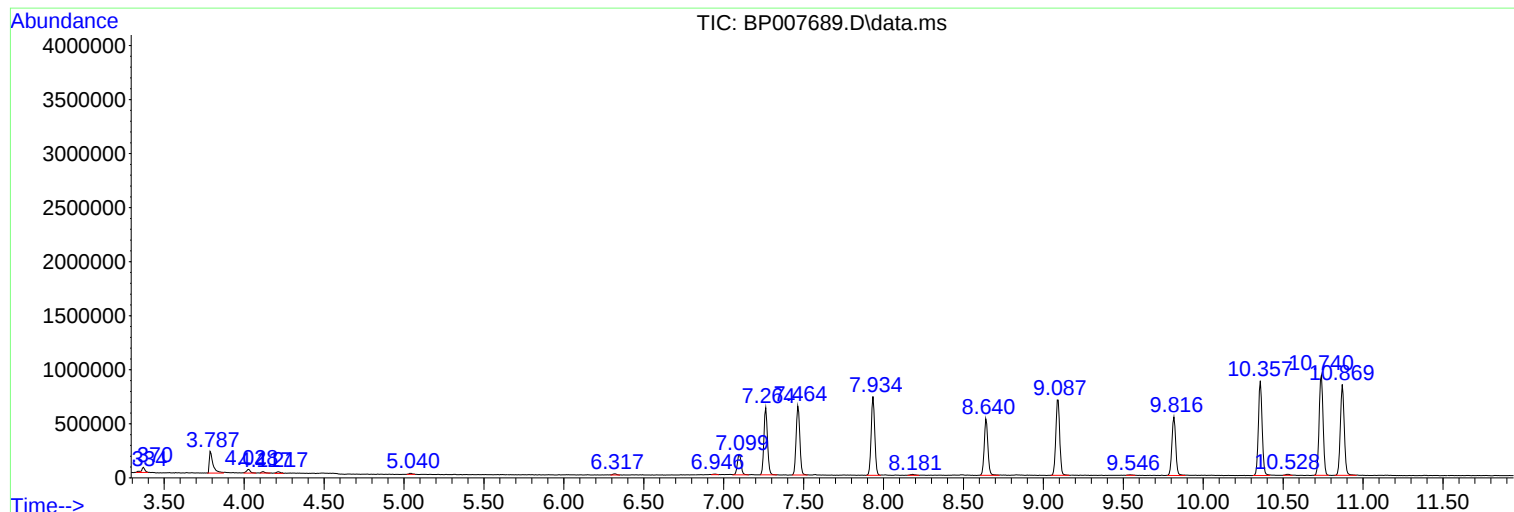

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007689.D
Acq On : 26 Oct 2021 21:17
Operator : CG/JU
Sample : M4291-21
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P046-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007689.D
Acq On : 26 Oct 2021 21:17
Operator : CG/JU
Sample : M4291-21
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P046-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
