

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007691.D
 Acq On : 26 Oct 2021 22:26
 Operator : CG/JU
 Sample : M4291-23
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P050-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	9	14	21	rVB	29894	39922	0.79%	0.098%
2	3.787	82	85	101	rBV	160862	278085	5.47%	0.685%
3	4.028	120	126	132	rVB	40362	63744	1.25%	0.157%
4	4.117	138	141	145	rVB2	14260	18720	0.37%	0.046%
5	4.217	153	158	165	rBV5	20665	36347	0.71%	0.090%
6	4.575	216	219	225	rVB2	12707	20173	0.40%	0.050%
7	5.040	294	298	304	rVB4	19487	32116	0.63%	0.079%
8	6.316	509	515	522	rBV2	18926	32453	0.64%	0.080%
9	6.940	618	621	625	rVB5	6332	9314	0.18%	0.023%
10	7.099	641	648	656	rVB	259713	405536	7.97%	0.999%
11	7.263	669	676	687	rVB	472304	753719	14.82%	1.857%
12	7.463	703	710	721	rVV	537421	837822	16.48%	2.064%
13	7.569	725	728	736	rVB9	7105	13761	0.27%	0.034%
14	7.934	784	790	801	rVB	617621	981763	19.31%	2.419%
15	8.069	808	813	815	rBV6	3664	5183	0.10%	0.013%
16	8.181	827	832	843	rVB5	13368	29820	0.59%	0.073%
17	8.493	880	885	889	rBV3	8762	12208	0.24%	0.030%
18	8.640	902	910	920	rBV	522780	848648	16.69%	2.091%
19	9.093	979	987	997	rBV	533922	890452	17.51%	2.194%
20	9.552	1055	1065	1069	rBV	4490	12283	0.24%	0.030%
21	9.816	1100	1110	1117	rBV	290714	484248	9.52%	1.193%
22	10.357	1194	1202	1215	rBV	655981	1100630	21.64%	2.711%
23	10.740	1258	1267	1278	rBV	805196	1391744	27.37%	3.428%
24	10.869	1283	1289	1300	rBV	106299	202737	3.99%	0.499%
25	11.546	1398	1404	1407	rBV7	3551	6053	0.12%	0.015%
26	12.046	1485	1489	1493	rBV6	3638	5601	0.11%	0.014%
27	12.328	1532	1537	1542	rVB2	14332	22275	0.44%	0.055%
28	12.498	1560	1566	1576	rBV5	11127	27673	0.54%	0.068%
29	13.551	1742	1745	1749	rVB6	3681	5246	0.10%	0.013%
30	13.981	1811	1818	1824	rBV	1439165	1945704	38.26%	4.793%
31	14.263	1857	1866	1877	rBV	1445805	2081012	40.92%	5.126%
32	14.569	1912	1918	1929	rVB	1275643	1920307	37.76%	4.731%
33	14.763	1944	1951	1965	rBV	225991	372538	7.33%	0.918%
34	14.992	1985	1990	1997	rVB7	15418	24823	0.49%	0.061%
35	15.563	2078	2087	2098	rBV	2029722	2966405	58.33%	7.308%
36	15.681	2100	2107	2117	rBV	459120	654722	12.88%	1.613%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007691.D
 Acq On : 26 Oct 2021 22:26
 Operator : CG/JU
 Sample : M4291-23
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P050-TW001-01

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2124	2128	2134	rVB4	15741	25177	0.50%	0.062%
38	15.898	2138	2144	2148	rBV9	3352	5575	0.11%	0.014%
39	16.263	2200	2206	2210	rBV5	8728	14570	0.29%	0.036%
40	16.351	2217	2221	2226	rVB6	3177	5891	0.12%	0.015%
41	17.004	2328	2332	2336	rVB7	4188	5561	0.11%	0.014%
42	17.110	2344	2350	2356	rBV	10291	16831	0.33%	0.041%
43	17.322	2380	2386	2394	rBV	1614597	2355959	46.33%	5.804%
44	17.428	2397	2404	2416	rBV	2630537	3833343	75.38%	9.443%
45	17.998	2498	2501	2507	rVB8	6154	8835	0.17%	0.022%
46	18.216	2534	2538	2544	rBV5	25975	44467	0.87%	0.110%
47	19.239	2708	2712	2719	rBV2	39508	51708	1.02%	0.127%
48	19.304	2719	2723	2728	rBV2	41807	59313	1.17%	0.146%
49	19.451	2746	2748	2751	rBV4	13313	16491	0.32%	0.041%
50	19.657	2777	2783	2797	rBV	3436509	4745517	93.32%	11.690%
51	21.416	3077	3082	3094	rBV	2140292	2828055	55.61%	6.967%
52	23.704	3463	3471	3479	rBV2	2504510	5085196	100.00%	12.527%
53	23.863	3491	3498	3509	rVB2	1414941	2957418	58.16%	7.285%




Sum of corrected areas: 40593694

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007691.D
Acq On : 26 Oct 2021 22:26
Operator : CG/JU
Sample : M4291-23
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P050-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

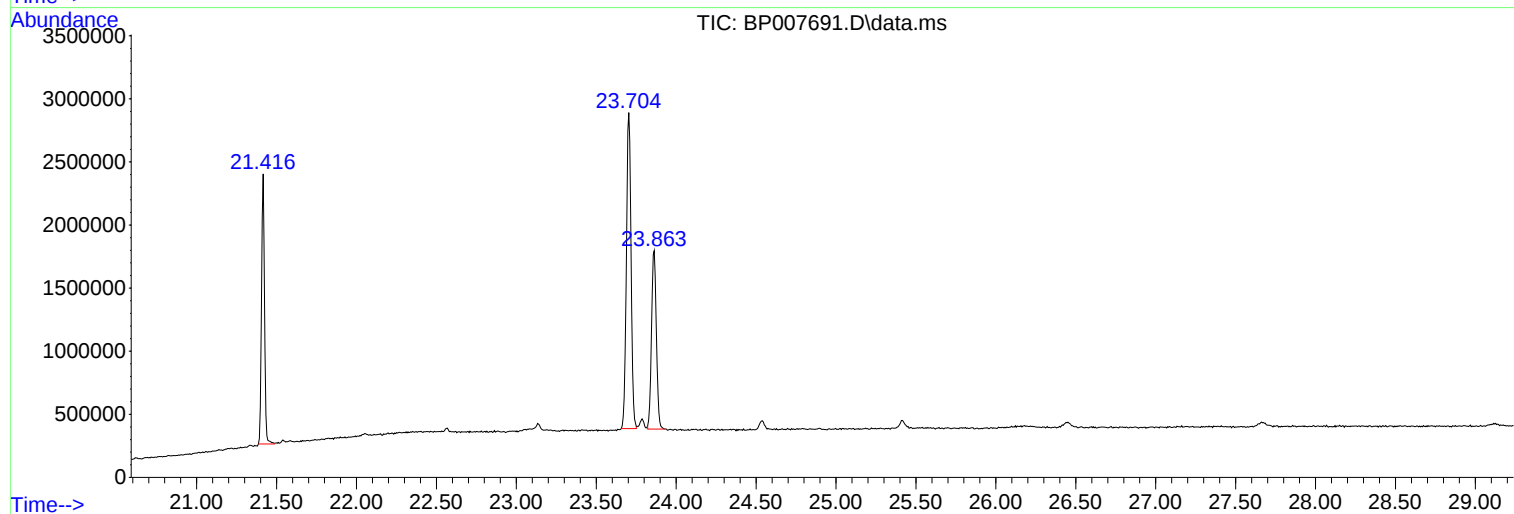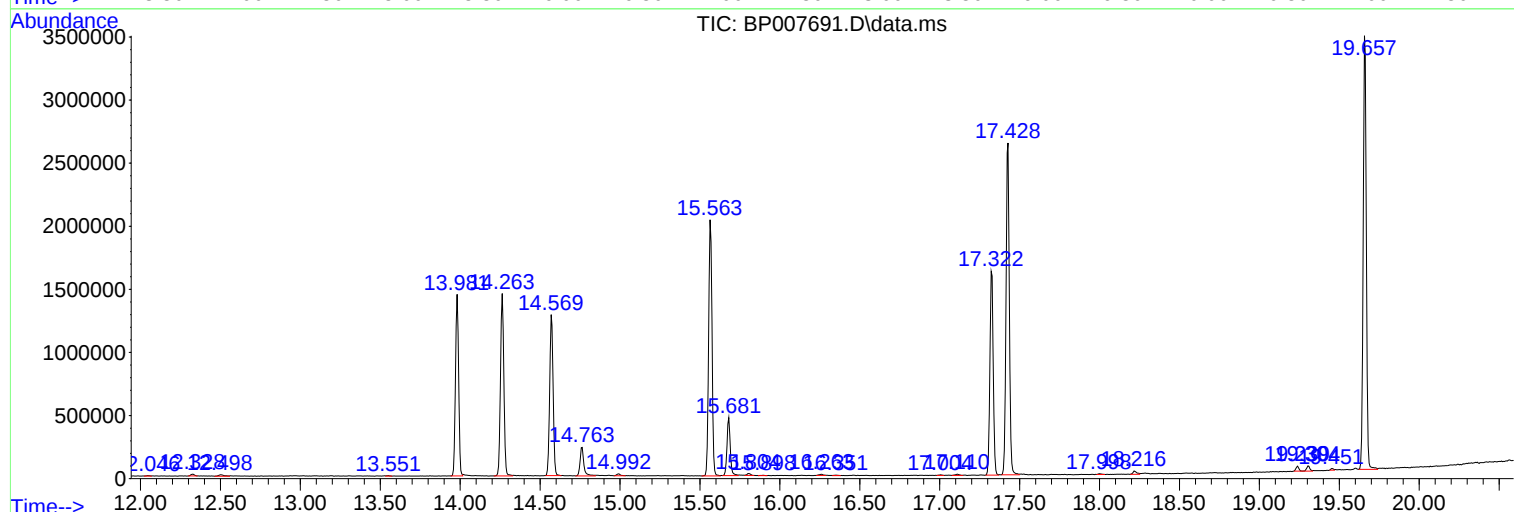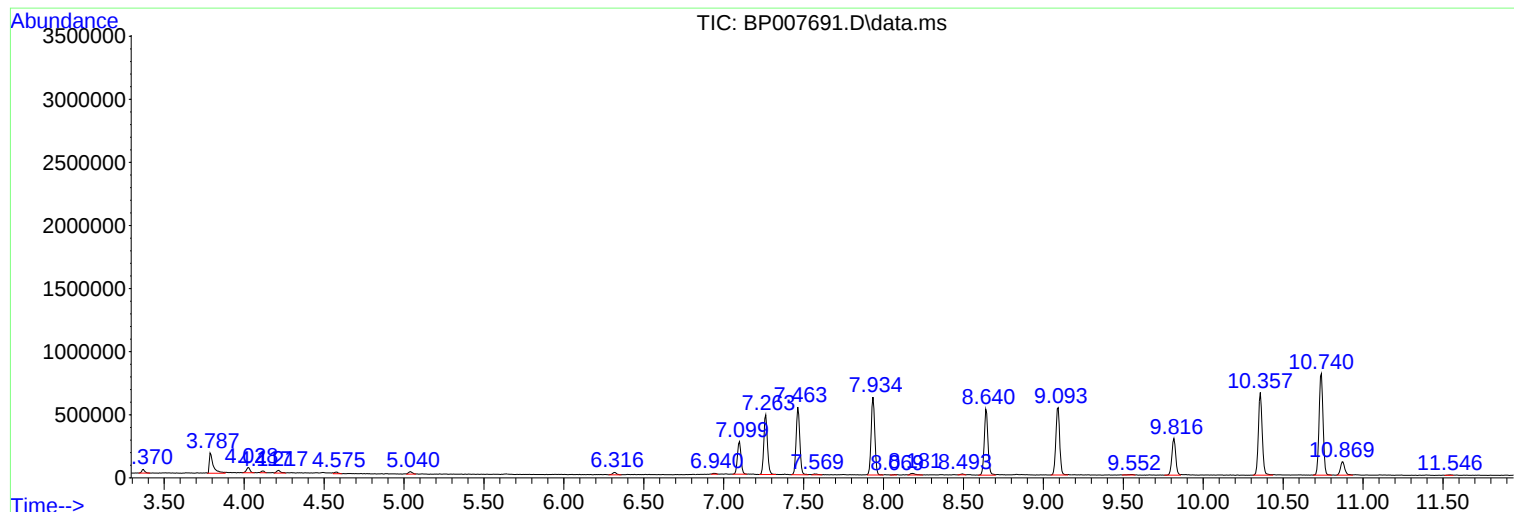

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007691.D
Acq On : 26 Oct 2021 22:26
Operator : CG/JU
Sample : M4291-23
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P050-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007691.D
Acq On : 26 Oct 2021 22:26
Operator : CG/JU
Sample : M4291-23
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P050-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
