

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007692.D
 Acq On : 26 Oct 2021 23:00
 Operator : CG/JU
 Sample : M4291-24
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P052-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007692.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	20	rVB	44111	59600	1.00%	0.123%
2	3.787	83	85	98	rBV	121288	186581	3.13%	0.384%
3	4.022	120	125	131	rVB	34387	54851	0.92%	0.113%
4	4.116	137	141	149	rVB	14639	25711	0.43%	0.053%
5	4.216	154	158	163	rVB6	15273	25369	0.43%	0.052%
6	5.046	294	299	305	rBV3	9056	14056	0.24%	0.029%
7	6.316	510	515	521	rBV4	13663	25646	0.43%	0.053%
8	6.940	618	621	626	rVB6	5572	7337	0.12%	0.015%
9	7.099	638	648	657	rBV	187737	302314	5.07%	0.622%
10	7.263	669	676	688	rVB	646533	1027455	17.23%	2.114%
11	7.463	702	710	719	rBV	649640	1019574	17.09%	2.098%
12	7.569	723	728	733	rVB9	4311	8418	0.14%	0.017%
13	7.934	783	790	799	rBV	671569	1052914	17.65%	2.167%
14	8.004	799	802	808	rVB2	11981	17107	0.29%	0.035%
15	8.181	827	832	840	rBV7	9897	19216	0.32%	0.040%
16	8.499	880	886	890	rBV8	4837	8879	0.15%	0.018%
17	8.640	903	910	919	rBV	520294	824871	13.83%	1.697%
18	9.040	972	978	979	rBV6	5253	6768	0.11%	0.014%
19	9.093	979	987	998	rVB	714703	1201529	20.15%	2.472%
20	9.263	1013	1016	1022	rBV8	4247	8107	0.14%	0.017%
21	9.816	1103	1110	1123	rBV	545458	870944	14.60%	1.792%
22	10.357	1194	1202	1213	rBV	877525	1453746	24.37%	2.991%
23	10.740	1259	1267	1274	rBV	851404	1474878	24.73%	3.035%
24	10.869	1282	1289	1299	rBV	757839	1302386	21.84%	2.680%
25	11.387	1371	1377	1380	rBV8	3593	7109	0.12%	0.015%
26	12.269	1522	1527	1532	rBV4	9306	17605	0.30%	0.036%
27	12.328	1532	1537	1544	rVB2	19138	34465	0.58%	0.071%
28	13.187	1678	1683	1688	rBV8	3664	6215	0.10%	0.013%
29	13.545	1738	1744	1750	rBV8	4787	9952	0.17%	0.020%
30	13.981	1809	1818	1831	rBV	1758698	2473560	41.47%	5.090%
31	14.263	1859	1866	1879	rBV	1944201	2820776	47.29%	5.804%
32	14.569	1911	1918	1932	rBV	1369871	2083857	34.94%	4.288%
33	14.763	1945	1951	1960	rBV2	125231	211489	3.55%	0.435%
34	14.992	1986	1990	1996	rVB8	12939	21044	0.35%	0.043%
35	15.563	2080	2087	2095	rBV	2619246	3818770	64.03%	7.858%
36	15.681	2100	2107	2119	rVV	572267	815122	13.67%	1.677%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007692.D
 Acq On : 26 Oct 2021 23:00
 Operator : CG/JU
 Sample : M4291-24
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P052-TW001-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2123	2128	2135	rVB	19528	33286	0.56%	0.068%
38	16.133	2180	2184	2188	rVB7	3678	6180	0.10%	0.013%
39	16.251	2196	2204	2209	rBV7	6834	18410	0.31%	0.038%
40	17.004	2327	2332	2338	rVB10	5356	8338	0.14%	0.017%
41	17.110	2344	2350	2354	rBV3	8335	16300	0.27%	0.034%
42	17.328	2379	2387	2396	rBV	1690196	2511042	42.10%	5.167%
43	17.428	2396	2404	2416	rBV	3076610	4587271	76.91%	9.439%
44	17.622	2432	2437	2445	rVB	21366	28455	0.48%	0.059%
45	17.698	2445	2450	2455	rBV8	4587	10085	0.17%	0.021%
46	18.004	2499	2502	2506	rVB6	5421	7629	0.13%	0.016%
47	18.222	2535	2539	2542	rBV5	8453	13464	0.23%	0.028%
48	19.239	2707	2712	2717	rBV2	44987	68746	1.15%	0.141%
49	19.304	2719	2723	2728	rVV	45815	64928	1.09%	0.134%
50	19.598	2770	2773	2777	rBV5	17587	23910	0.40%	0.049%
51	19.657	2777	2783	2795	rVV	3948421	5630846	94.41%	11.586%
52	20.563	2934	2937	2940	rBV2	45345	51125	0.86%	0.105%
53	21.416	3077	3082	3088	rBV	2273379	3023285	50.69%	6.221%
54	23.704	3464	3471	3480	rBV2	2925654	5964323	100.00%	12.272%
55	23.862	3491	3498	3509	rVB2	1539301	3213719	53.88%	6.613%




Sum of corrected areas: 48599563

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007692.D
Acq On : 26 Oct 2021 23:00
Operator : CG/JU
Sample : M4291-24
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P052-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

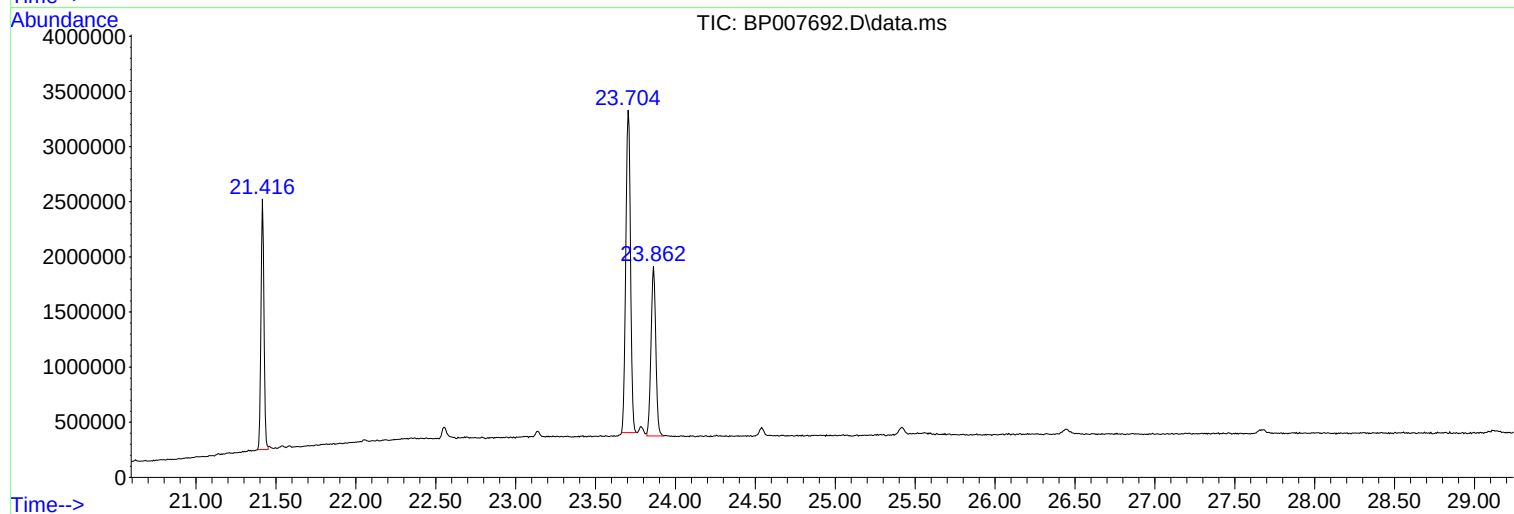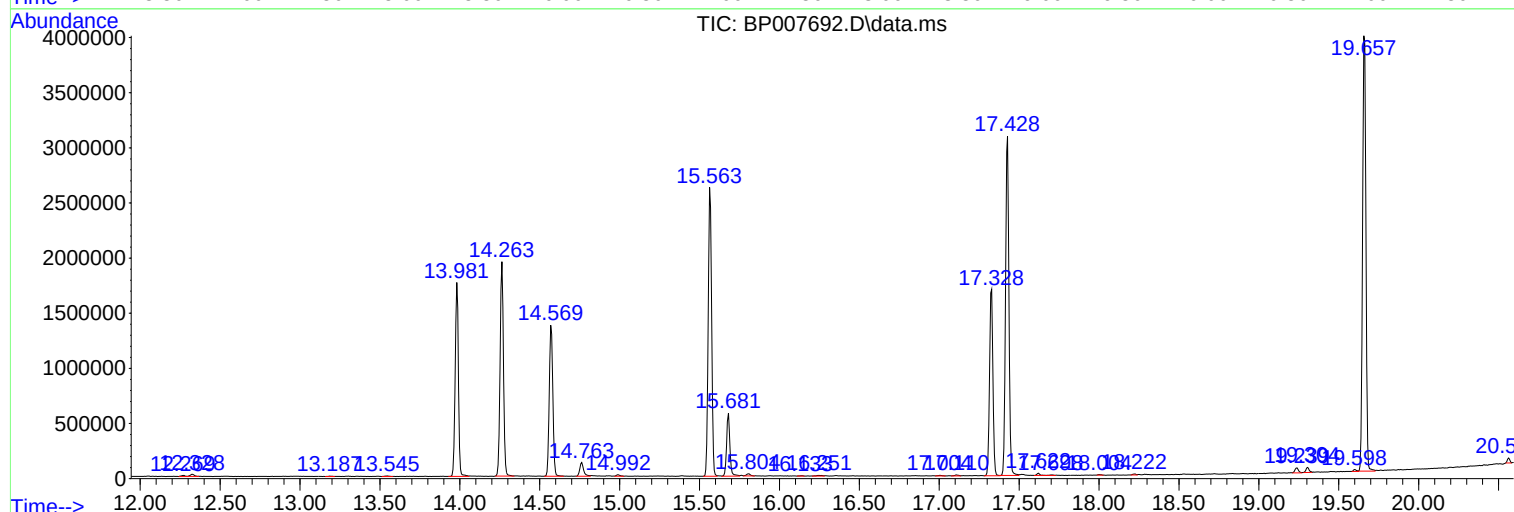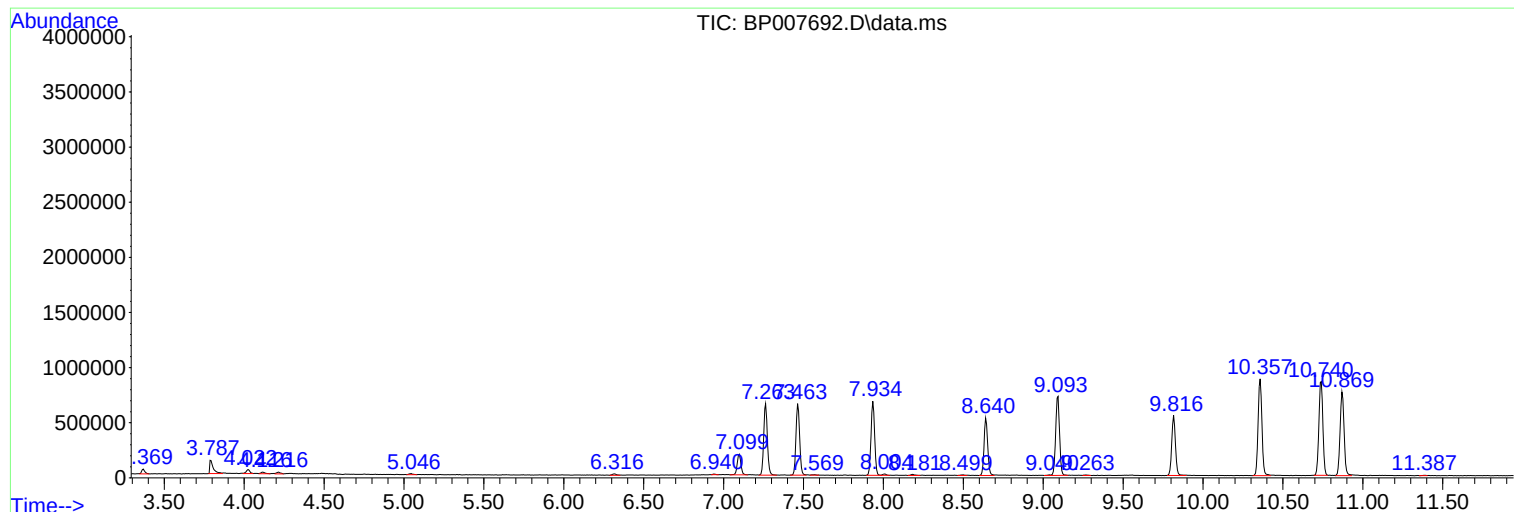

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007692.D
Acq On : 26 Oct 2021 23:00
Operator : CG/JU
Sample : M4291-24
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P052-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007692.D
Acq On : 26 Oct 2021 23:00
Operator : CG/JU
Sample : M4291-24
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P052-TW001-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------