

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007693.D
 Acq On : 26 Oct 2021 23:34
 Operator : CG/JU
 Sample : M4303-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P010-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	9	14	23	rVB	43823	61396	1.00%	0.126%
2	3.787	83	85	102	rBV	191691	317042	5.17%	0.652%
3	4.028	121	126	131	rVB2	31565	45467	0.74%	0.094%
4	4.117	138	141	146	rVB	11529	15527	0.25%	0.032%
5	4.211	154	157	164	rVB2	13155	19442	0.32%	0.040%
6	6.322	510	516	521	rBV3	10767	17878	0.29%	0.037%
7	7.099	641	648	656	rVB	161650	258351	4.21%	0.531%
8	7.263	669	676	686	rBV	612121	974239	15.89%	2.004%
9	7.463	703	710	721	rVB	606092	950274	15.50%	1.954%
10	7.934	782	790	800	rBV	667895	1046641	17.07%	2.152%
11	8.640	902	910	923	rBV	459950	720139	11.75%	1.481%
12	9.087	977	986	1000	rBV	692227	1163683	18.98%	2.393%
13	9.816	1102	1110	1123	rBV	519244	859079	14.01%	1.767%
14	10.357	1194	1202	1215	rBV	844690	1373264	22.40%	2.824%
15	10.522	1225	1230	1238	rBV2	25119	48977	0.80%	0.101%
16	10.740	1257	1267	1276	rBV	859631	1472647	24.02%	3.029%
17	10.869	1279	1289	1304	rBV	774826	1315691	21.46%	2.706%
18	12.322	1530	1536	1545	rVB3	19189	33110	0.54%	0.068%
19	13.193	1679	1684	1687	rBV7	3890	7167	0.12%	0.015%
20	13.481	1726	1733	1739	rBV2	46591	75473	1.23%	0.155%
21	13.545	1740	1744	1749	rVB7	4285	6785	0.11%	0.014%
22	13.781	1779	1784	1788	rBV8	4170	6823	0.11%	0.014%
23	13.981	1811	1818	1831	rBV	1685994	2327523	37.97%	4.787%
24	14.263	1852	1866	1879	rBV	1843473	2694258	43.95%	5.541%
25	14.569	1911	1918	1926	rBV	1387246	2051653	33.47%	4.219%
26	14.763	1944	1951	1957	rBV	133425	213690	3.49%	0.439%
27	14.992	1985	1990	1994	rVB8	7689	11361	0.19%	0.023%
28	15.392	2052	2058	2061	rBV6	4665	7681	0.13%	0.016%
29	15.563	2080	2087	2095	rBV	2609825	3719575	60.68%	7.649%
30	15.681	2099	2107	2118	rBV	695940	992507	16.19%	2.041%
31	15.804	2124	2128	2136	rVB	21369	33637	0.55%	0.069%
32	16.245	2200	2203	2210	rBV9	5312	10476	0.17%	0.022%
33	16.463	2234	2240	2247	rBV9	4215	11586	0.19%	0.024%
34	17.116	2346	2351	2354	rVB3	8008	13041	0.21%	0.027%
35	17.328	2380	2387	2396	rBV	1711688	2561035	41.78%	5.267%
36	17.428	2397	2404	2416	rVV	3093448	4598619	75.02%	9.457%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007693.D
 Acq On : 26 Oct 2021 23:34
 Operator : CG/JU
 Sample : M4303-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P010-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.522	2416	2420	2430	rVB10	19132	35309	0.58%	0.073%
38	18.004	2498	2502	2508	rBV2	20544	29393	0.48%	0.060%
39	18.216	2534	2538	2542	rBV5	26666	37544	0.61%	0.077%
40	19.045	2677	2679	2683	rBV5	8079	13141	0.21%	0.027%
41	19.133	2692	2694	2697	rVB4	17457	18002	0.29%	0.037%
42	19.233	2707	2711	2714	rBV2	49245	67568	1.10%	0.139%
43	19.269	2714	2717	2719	rVV2	31618	35380	0.58%	0.073%
44	19.304	2719	2723	2727	rVB	51303	65789	1.07%	0.135%
45	19.598	2771	2773	2777	rVB5	14899	12393	0.20%	0.025%
46	19.657	2777	2783	2790	rBV	4209879	5744827	93.72%	11.814%
47	21.416	3077	3082	3094	rBV	2467726	3165202	51.64%	6.509%
48	23.704	3463	3471	3481	rBV2	2982813	6129908	100.00%	12.606%
49	23.863	3491	3498	3508	rVB2	1539864	3235642	52.78%	6.654%




Sum of corrected areas: 48625835

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007693.D
Acq On : 26 Oct 2021 23:34
Operator : CG/JU
Sample : M4303-05
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P010-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

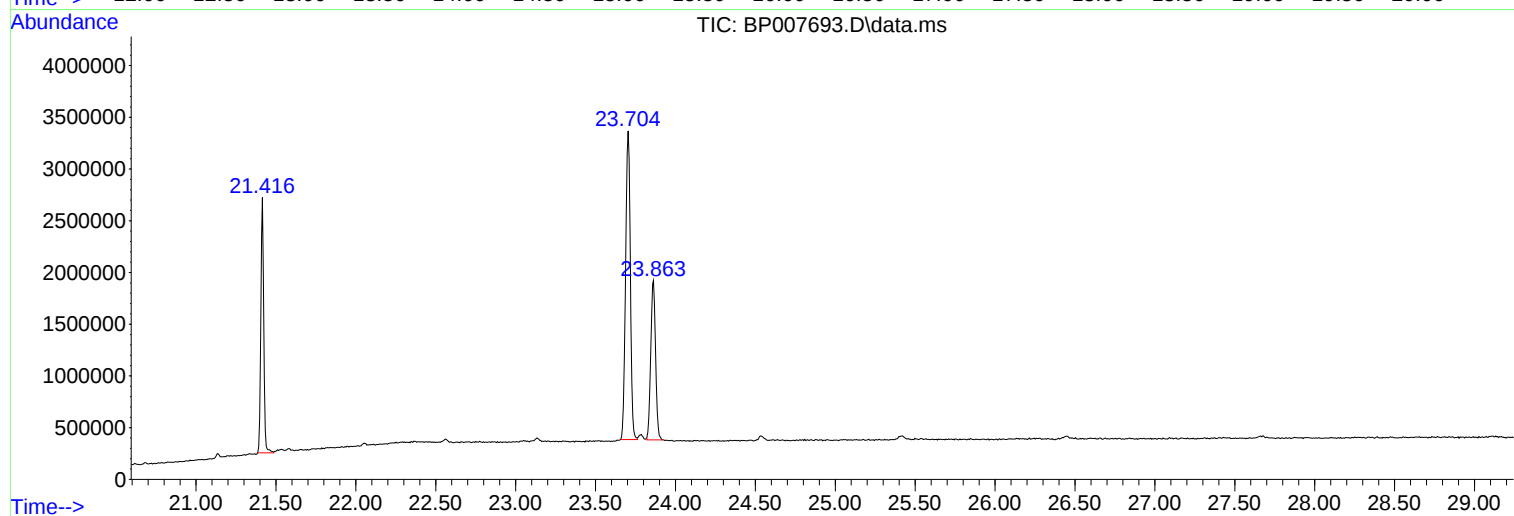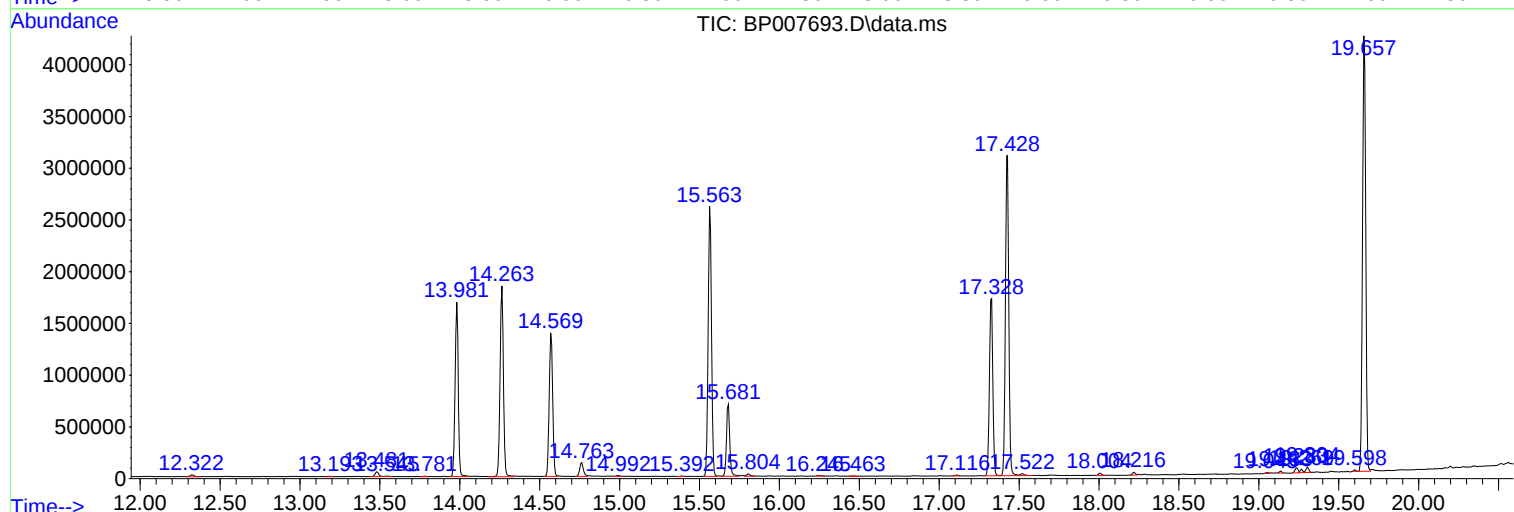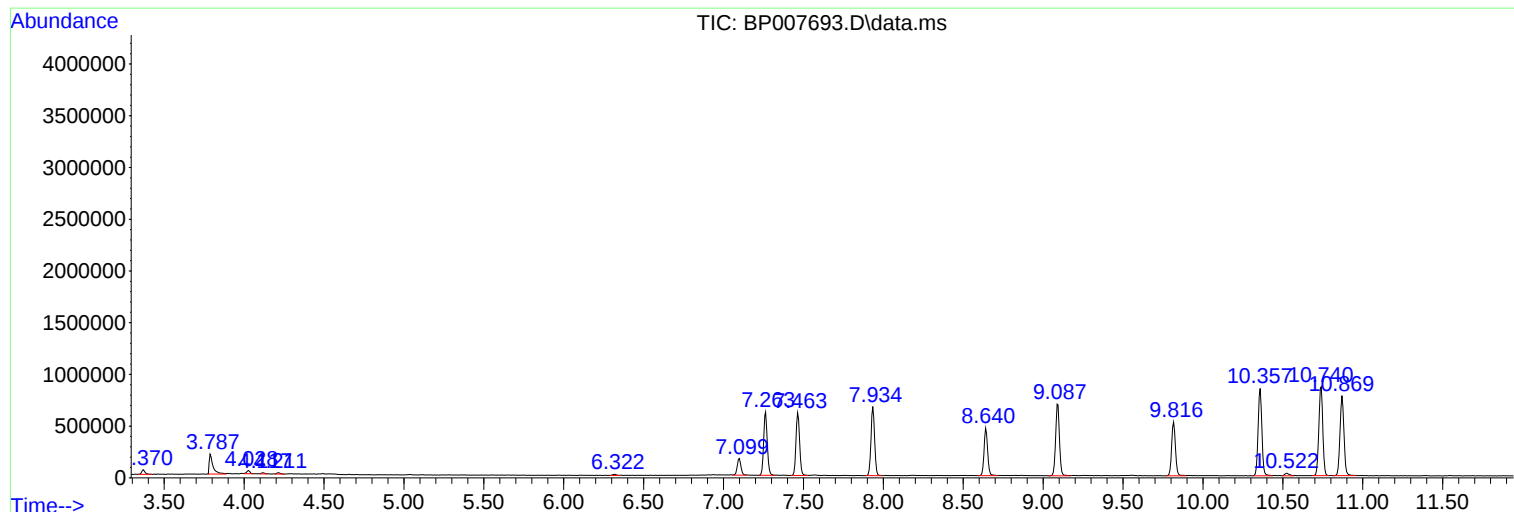

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007693.D
Acq On : 26 Oct 2021 23:34
Operator : CG/JU
Sample : M4303-05
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P010-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007693.D
Acq On : 26 Oct 2021 23:34
Operator : CG/JU
Sample : M4303-05
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P010-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------