

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007694.D
 Acq On : 27 Oct 2021 00:08
 Operator : CG/JU
 Sample : M4303-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P003-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	21	rBV	39138	52888	0.94%	0.118%
2	3.793	84	86	101	rBV	87330	153226	2.73%	0.341%
3	4.022	122	125	132	rVB2	26749	43469	0.77%	0.097%
4	4.122	138	142	148	rVB	12940	18431	0.33%	0.041%
5	4.217	154	158	164	rVB5	12249	21837	0.39%	0.049%
6	5.034	295	297	302	rVB4	6523	7459	0.13%	0.017%
7	6.316	511	515	521	rVB2	10251	16812	0.30%	0.037%
8	7.099	642	648	655	rVB	164699	266938	4.76%	0.594%
9	7.263	669	676	689	rVB	605869	960050	17.11%	2.137%
10	7.463	703	710	724	rBV	612460	968049	17.25%	2.155%
11	7.569	724	728	732	rBV7	4432	5862	0.10%	0.013%
12	7.934	782	790	798	rBV	660731	1018218	18.15%	2.266%
13	8.181	827	832	837	rVB9	3116	6315	0.11%	0.014%
14	8.487	879	884	887	rBV7	3264	6257	0.11%	0.014%
15	8.640	903	910	922	rBV	468395	745522	13.29%	1.659%
16	9.093	979	987	999	rBV	661415	1111958	19.82%	2.475%
17	9.557	1060	1066	1070	rVB9	5145	10347	0.18%	0.023%
18	9.816	1102	1110	1123	rBV	508106	837756	14.93%	1.865%
19	10.357	1194	1202	1218	rBV	806836	1347626	24.02%	2.999%
20	10.528	1223	1231	1239	rBV2	22788	44951	0.80%	0.100%
21	10.734	1259	1266	1276	rVB	818790	1391644	24.80%	3.097%
22	10.869	1281	1289	1298	rBV	572558	983242	17.52%	2.188%
23	12.046	1483	1489	1494	rBV10	3985	7082	0.13%	0.016%
24	12.322	1531	1536	1543	rVB2	18361	30503	0.54%	0.068%
25	12.945	1635	1642	1646	rBV10	4569	12162	0.22%	0.027%
26	13.193	1679	1684	1689	rVB6	5756	9004	0.16%	0.020%
27	13.540	1739	1743	1748	rVB6	4638	8324	0.15%	0.019%
28	13.981	1810	1818	1834	rBV	1617408	2304097	41.06%	5.128%
29	14.263	1857	1866	1878	rBV	1832781	2592808	46.21%	5.771%
30	14.569	1910	1918	1931	rBV	1252345	1883679	33.57%	4.192%
31	14.763	1943	1951	1964	rBV	122797	222581	3.97%	0.495%
32	14.934	1974	1980	1985	rVB9	3891	8596	0.15%	0.019%
33	14.992	1985	1990	1995	rBV9	6651	11765	0.21%	0.026%
34	15.392	2053	2058	2062	rBV7	5070	9203	0.16%	0.020%
35	15.563	2079	2087	2095	rBV	2445867	3494492	62.27%	7.778%
36	15.681	2100	2107	2119	rBV	651791	907843	16.18%	2.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007694.D
 Acq On : 27 Oct 2021 00:08
 Operator : CG/JU
 Sample : M4303-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P003-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2124	2128	2132	rVV2	18602	34693	0.62%	0.077%
38	15.845	2132	2135	2144	rVB5	11912	22129	0.39%	0.049%
39	16.245	2200	2203	2209	rVB7	4812	8658	0.15%	0.019%
40	16.328	2209	2217	2222	rBV	25744	43833	0.78%	0.098%
41	16.716	2279	2283	2286	rVB5	4101	5769	0.10%	0.013%
42	17.110	2346	2350	2354	rBV4	7133	13399	0.24%	0.030%
43	17.151	2354	2357	2363	rVB4	18116	27809	0.50%	0.062%
44	17.328	2380	2387	2393	rBV	1546872	2295545	40.91%	5.109%
45	17.422	2397	2403	2417	rVV2	2813662	4142117	73.82%	9.219%
46	17.757	2458	2460	2464	rBV5	5914	5993	0.11%	0.013%
47	18.004	2499	2502	2507	rVB6	8371	12128	0.22%	0.027%
48	18.192	2532	2534	2535	rBV2	7511	7017	0.13%	0.016%
49	18.216	2535	2538	2541	rVV5	17588	23047	0.41%	0.051%
50	18.281	2547	2549	2553	rVB4	7727	8551	0.15%	0.019%
51	18.369	2562	2564	2568	rVB5	8555	10357	0.18%	0.023%
52	18.969	2662	2666	2670	rBV6	9731	16199	0.29%	0.036%
53	19.233	2708	2711	2715	rVB	38977	48167	0.86%	0.107%
54	19.304	2719	2723	2727	rBV	44953	54574	0.97%	0.121%
55	19.598	2771	2773	2776	rBV4	12219	11073	0.20%	0.025%
56	19.657	2777	2783	2790	rBV	3805604	5155724	91.88%	11.475%
57	21.416	3077	3082	3092	rBV	2112476	2844365	50.69%	6.331%
58	23.704	3463	3471	3480	rBV2	2734063	5611433	100.00%	12.489%
59	23.863	3491	3498	3509	rVB2	1452078	3007047	53.59%	6.693%




Sum of corrected areas: 44930623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007694.D
Acq On : 27 Oct 2021 00:08
Operator : CG/JU
Sample : M4303-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P003-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

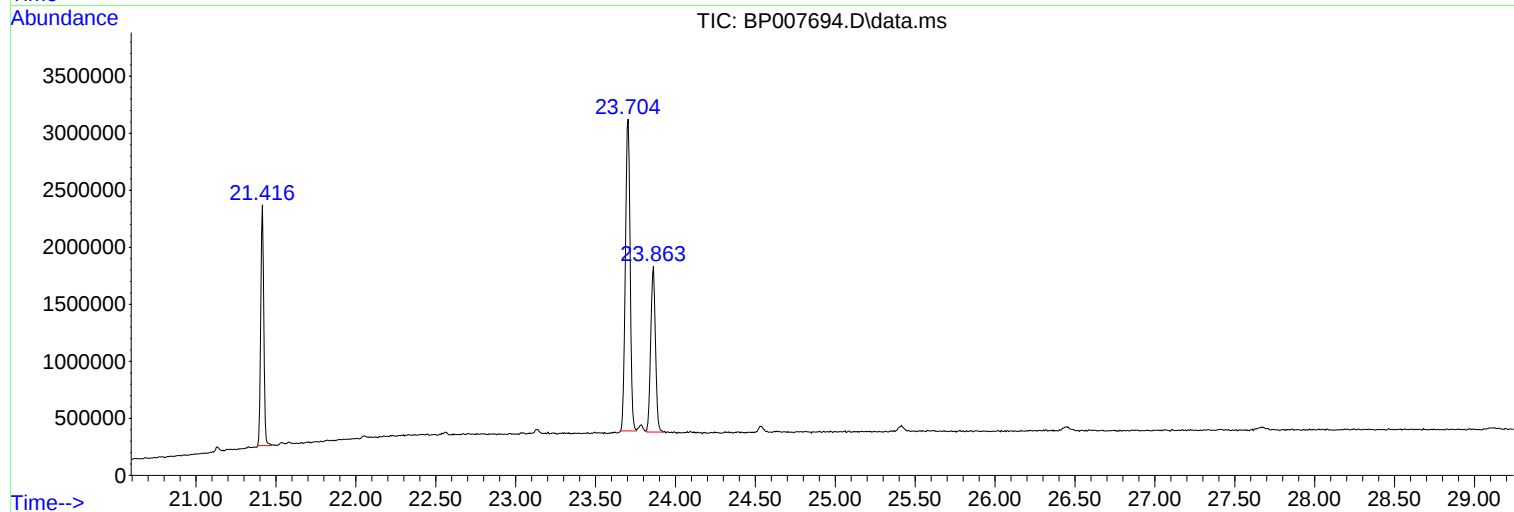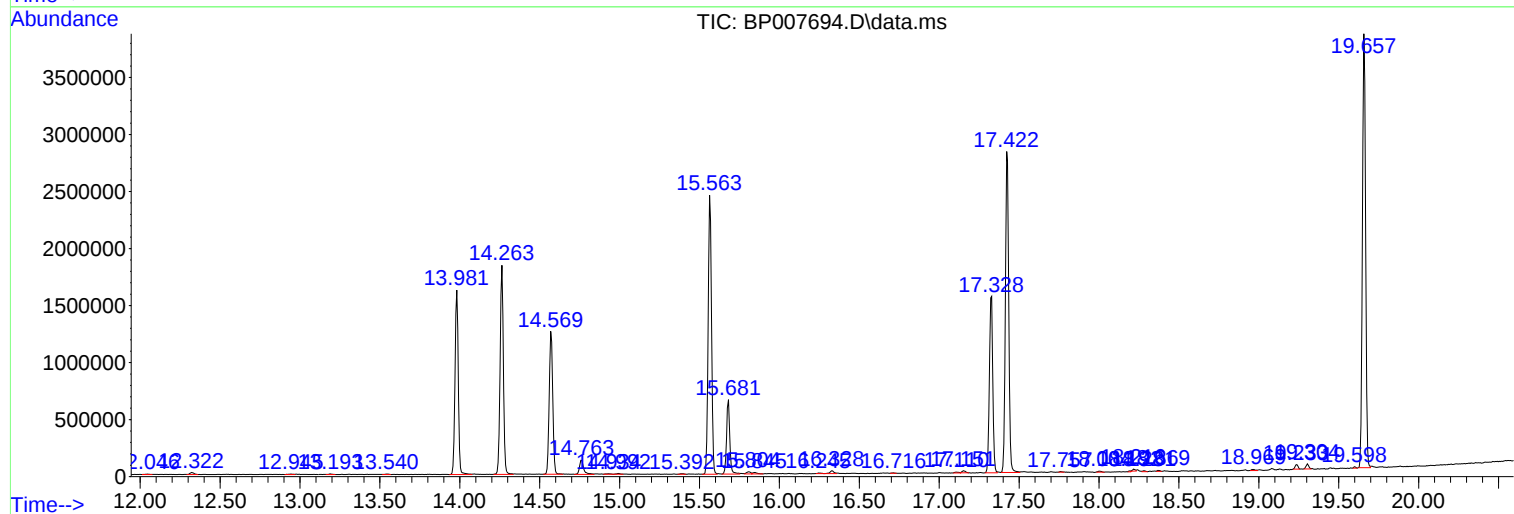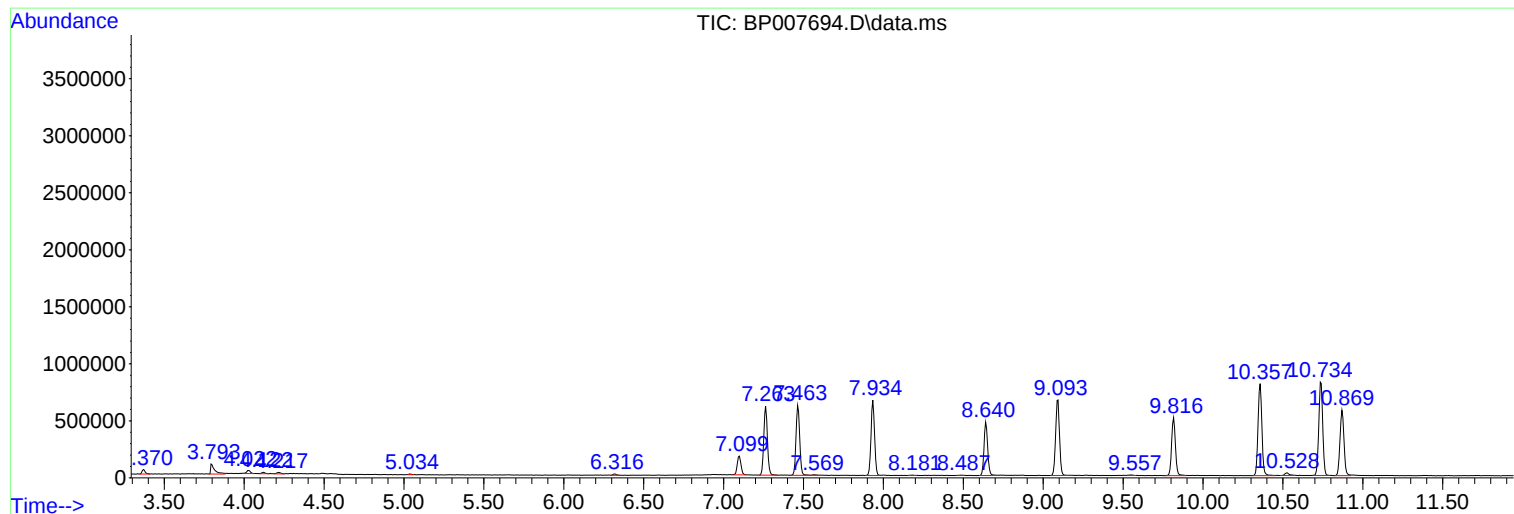

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007694.D
Acq On : 27 Oct 2021 00:08
Operator : CG/JU
Sample : M4303-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P003-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007694.D
Acq On : 27 Oct 2021 00:08
Operator : CG/JU
Sample : M4303-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P003-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
