

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007695.D
 Acq On : 27 Oct 2021 00:42
 Operator : CG/JU
 Sample : M4303-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P004-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	20	rVB	40282	52861	0.84%	0.104%
2	3.793	84	86	99	rBV	65444	108384	1.72%	0.213%
3	4.022	121	125	131	rVB	31296	48165	0.76%	0.095%
4	4.117	138	141	145	rVB2	12258	12704	0.20%	0.025%
5	4.217	154	158	164	rVB6	14237	21541	0.34%	0.042%
6	5.046	294	299	305	rVB5	10599	19199	0.30%	0.038%
7	6.316	510	515	519	rBV2	11479	16711	0.27%	0.033%
8	7.099	640	648	658	rVB	179488	290374	4.61%	0.572%
9	7.263	669	676	686	rVB	646995	1022530	16.22%	2.013%
10	7.463	703	710	724	rBV	654714	1025545	16.27%	2.019%
11	7.934	783	790	799	rBV	708138	1095846	17.39%	2.157%
12	8.640	904	910	923	rBV	517369	819425	13.00%	1.613%
13	9.093	979	987	995	rBV	733777	1234057	19.58%	2.429%
14	9.546	1062	1064	1069	rVB6	5295	6683	0.11%	0.013%
15	9.816	1101	1110	1128	rBV	557772	937155	14.87%	1.845%
16	10.357	1194	1202	1213	rBV	903113	1499026	23.78%	2.951%
17	10.522	1223	1230	1240	rBV5	15632	34998	0.56%	0.069%
18	10.740	1259	1267	1278	rVB	919021	1578141	25.04%	3.106%
19	10.869	1278	1289	1302	rBV	672968	1176217	18.66%	2.315%
20	12.328	1531	1537	1544	rBV	18540	33118	0.53%	0.065%
21	13.187	1680	1683	1688	rVB6	4083	7134	0.11%	0.014%
22	13.540	1740	1743	1748	rVB7	4903	8775	0.14%	0.017%
23	13.981	1811	1818	1833	rBV	1914396	2631335	41.75%	5.179%
24	14.263	1858	1866	1887	rBV	1978064	2975542	47.21%	5.857%
25	14.569	1910	1918	1927	rBV	1503162	2186417	34.69%	4.304%
26	14.757	1944	1950	1965	rBV	148126	252306	4.00%	0.497%
27	14.998	1986	1991	1996	rVB9	4987	8893	0.14%	0.018%
28	15.563	2078	2087	2097	rBV	2764139	3978109	63.11%	7.830%
29	15.681	2101	2107	2116	rBV	747548	1048156	16.63%	2.063%
30	15.804	2124	2128	2133	rVB3	23002	35932	0.57%	0.071%
31	16.239	2196	2202	2209	rBV3	6451	15214	0.24%	0.030%
32	16.351	2219	2221	2229	rVB8	5559	9534	0.15%	0.019%
33	16.998	2329	2331	2337	rVB7	4994	6813	0.11%	0.013%
34	17.110	2344	2350	2354	rBV2	9850	17506	0.28%	0.034%
35	17.322	2380	2386	2396	rVB	1872662	2661684	42.23%	5.239%
36	17.422	2396	2403	2417	rBV2	3208208	4789502	75.98%	9.427%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007695.D
 Acq On : 27 Oct 2021 00:42
 Operator : CG/JU
 Sample : M4303-02
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P004-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.516	2417	2419	2424	rVB4	7531	10399	0.16%	0.020%
38	17.704	2447	2451	2455	rBV6	4237	7100	0.11%	0.014%
39	18.004	2500	2502	2507	rVB6	10358	11113	0.18%	0.022%
40	18.216	2533	2538	2545	rBV7	33848	51913	0.82%	0.102%
41	18.533	2590	2592	2598	rVB7	6342	6516	0.10%	0.013%
42	19.233	2707	2711	2718	rVB2	45518	60493	0.96%	0.119%
43	19.304	2718	2723	2728	rBV	49494	74019	1.17%	0.146%
44	19.451	2745	2748	2754	rBV7	12994	21965	0.35%	0.043%
45	19.598	2770	2773	2777	rBV6	13626	17746	0.28%	0.035%
46	19.657	2777	2783	2790	rBV	4466962	5907872	93.73%	11.629%
47	21.133	3031	3034	3041	rBV3	41055	65654	1.04%	0.129%
48	21.416	3076	3082	3088	rBV	2401728	3235081	51.32%	6.368%
49	23.704	3463	3471	3480	rBV2	3141162	6303270	100.00%	12.407%
50	23.857	3490	3497	3507	rVB2	1609616	3365498	53.39%	6.624%




Sum of corrected areas: 50804171

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007695.D
Acq On : 27 Oct 2021 00:42
Operator : CG/JU
Sample : M4303-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P004-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

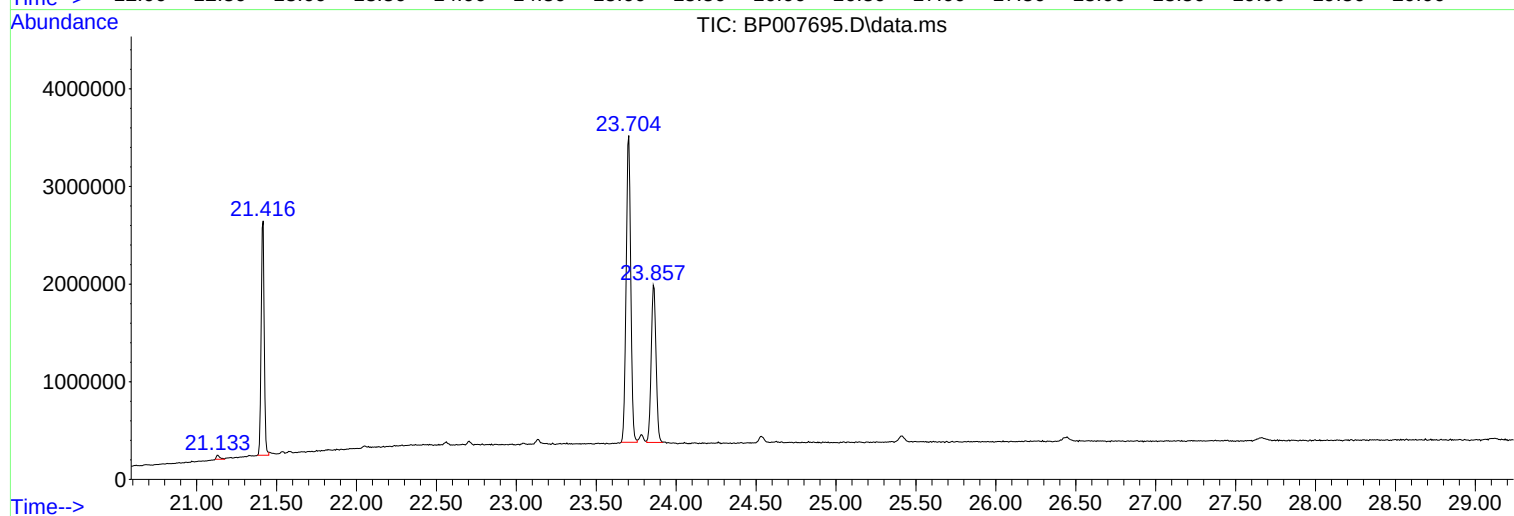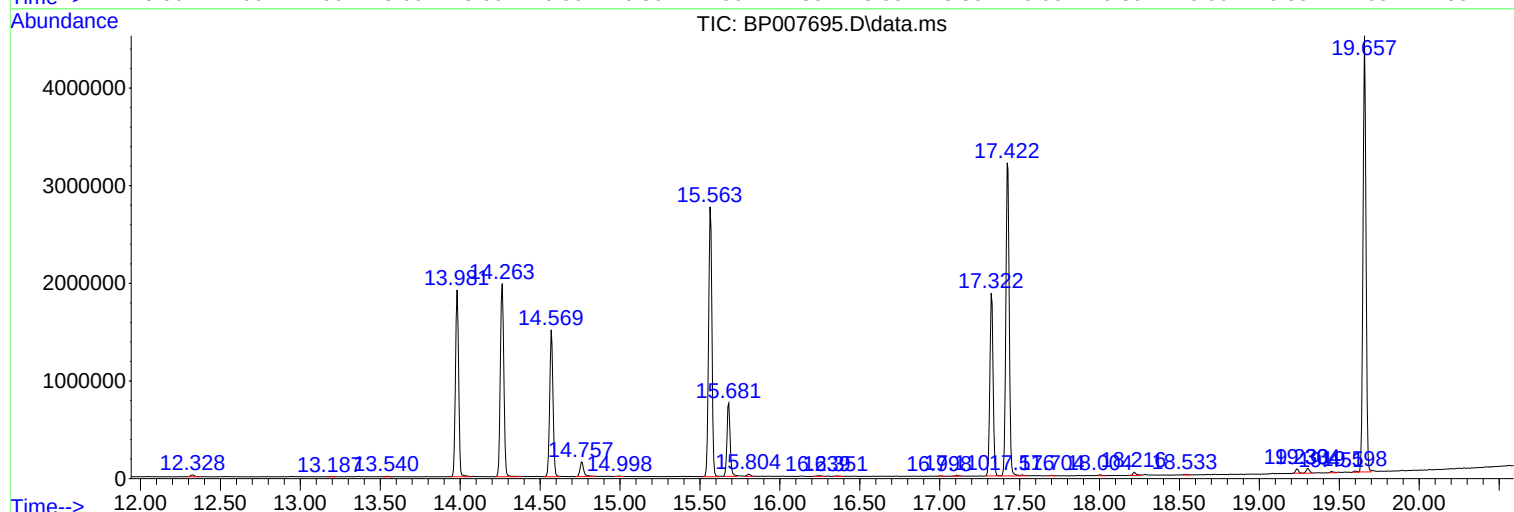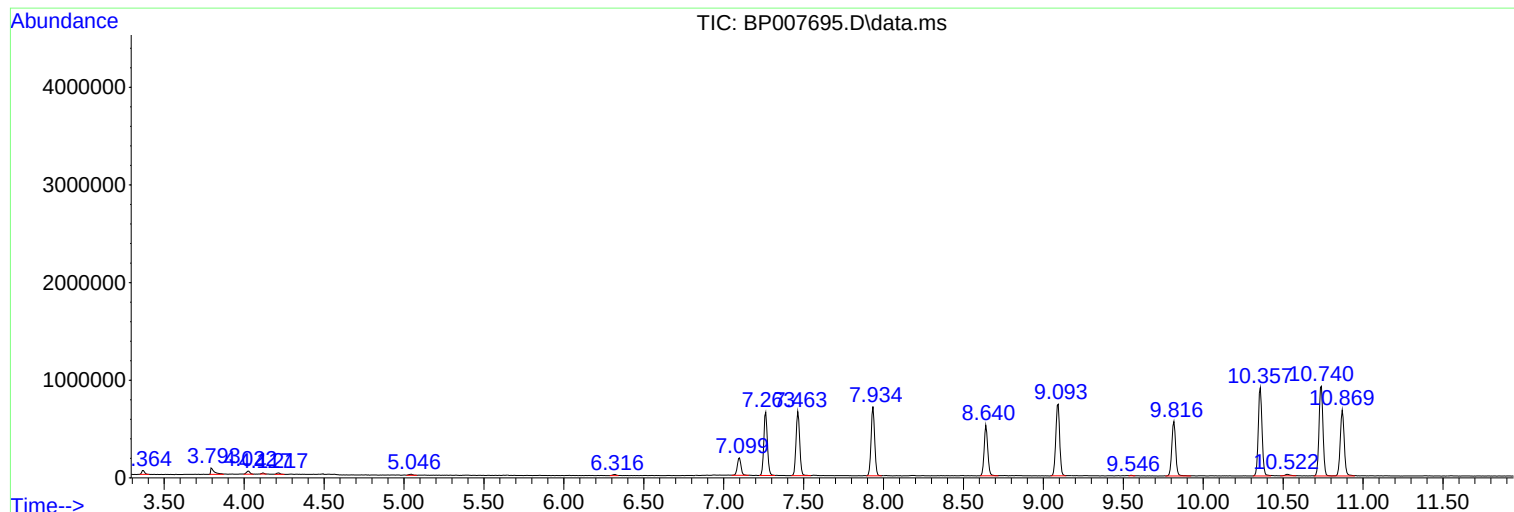

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007695.D
Acq On : 27 Oct 2021 00:42
Operator : CG/JU
Sample : M4303-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P004-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007695.D
Acq On : 27 Oct 2021 00:42
Operator : CG/JU
Sample : M4303-02
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P004-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------