

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007697.D
 Acq On : 27 Oct 2021 01:50
 Operator : CG/JU
 Sample : M4303-04
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P006-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	21	rVB	44381	65038	1.02%	0.122%
2	3.787	82	85	97	rBV	205057	318174	4.99%	0.596%
3	4.023	121	125	132	rVB	32811	51858	0.81%	0.097%
4	4.117	138	141	146	rVB	14188	18159	0.28%	0.034%
5	4.217	154	158	161	rVB3	13020	14880	0.23%	0.028%
6	5.040	293	298	301	rBV5	9347	16031	0.25%	0.030%
7	6.317	510	515	521	rVB5	12898	21894	0.34%	0.041%
8	7.099	641	648	659	rVB	213754	347610	5.45%	0.652%
9	7.264	669	676	688	rVB	687216	1104549	17.32%	2.071%
10	7.464	704	710	721	rBV	729582	1128674	17.70%	2.116%
11	7.934	783	790	799	rBV	735727	1161727	18.22%	2.178%
12	8.175	825	831	838	rVB	5103	13542	0.21%	0.025%
13	8.640	903	910	920	rBV	587197	936086	14.68%	1.755%
14	9.087	976	986	996	rBV	793641	1320229	20.70%	2.475%
15	9.552	1062	1065	1070	rVB7	5670	8617	0.14%	0.016%
16	9.816	1098	1110	1124	rBV	603056	1007583	15.80%	1.889%
17	10.358	1192	1202	1213	rBV	957477	1607189	25.20%	3.013%
18	10.528	1226	1231	1242	rVB6	13192	29315	0.46%	0.055%
19	10.734	1257	1266	1276	rBV	957997	1663322	26.08%	3.118%
20	10.869	1281	1289	1306	rBV	893728	1522464	23.87%	2.854%
21	12.046	1483	1489	1492	rBV8	4275	6910	0.11%	0.013%
22	12.322	1530	1536	1542	rVB	21064	35979	0.56%	0.067%
23	12.940	1636	1641	1645	rBV7	3734	6811	0.11%	0.013%
24	13.187	1679	1683	1690	rVB9	4695	8455	0.13%	0.016%
25	13.981	1811	1818	1832	rBV	1968356	2670921	41.88%	5.007%
26	14.263	1856	1866	1877	rBV	2134935	3111932	48.80%	5.834%
27	14.569	1911	1918	1925	rBV	1572837	2303375	36.12%	4.318%
28	14.763	1944	1951	1963	rBV	169624	291793	4.58%	0.547%
29	14.993	1983	1990	1997	rVB9	11511	19434	0.30%	0.036%
30	15.563	2080	2087	2096	rBV	2825939	4091038	64.15%	7.670%
31	15.681	2101	2107	2122	rVV	769622	1067913	16.75%	2.002%
32	15.804	2124	2128	2134	rVB3	20991	35292	0.55%	0.066%
33	16.245	2199	2203	2209	rVB9	6070	12027	0.19%	0.023%
34	16.357	2219	2222	2228	rVB7	5041	9359	0.15%	0.018%
35	17.010	2329	2333	2338	rVB7	4629	8019	0.13%	0.015%
36	17.110	2345	2350	2353	rBV	10421	13583	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007697.D
 Acq On : 27 Oct 2021 01:50
 Operator : CG/JU
 Sample : M4303-04
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P006-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	17.322	2380	2386	2397	rBV	1968364	2832986	44.42%	5.311%
38	17.422	2397	2403	2416	rVV	3223447	4767680	74.76%	8.938%
39	17.522	2416	2420	2427	rVB9	9713	18307	0.29%	0.034%
40	18.004	2498	2502	2509	rBV9	9798	16100	0.25%	0.030%
41	18.216	2534	2538	2545	rBV4	30349	43360	0.68%	0.081%
42	19.239	2707	2712	2717	rBV3	46556	64526	1.01%	0.121%
43	19.304	2718	2723	2730	rBV	52462	76711	1.20%	0.144%
44	19.451	2745	2748	2752	rBV5	15745	20819	0.33%	0.039%
45	19.657	2777	2783	2798	rBV	4277902	5913606	92.73%	11.087%
46	21.416	3076	3082	3087	rBV	2619991	3498967	54.87%	6.560%
47	23.704	3463	3471	3480	rBV	3160477	6377183	100.00%	11.956%
48	23.863	3491	3498	3508	rVB2	1761849	3660389	57.40%	6.862%




Sum of corrected areas: 53340416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007697.D
Acq On : 27 Oct 2021 01:50
Operator : CG/JU
Sample : M4303-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P006-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

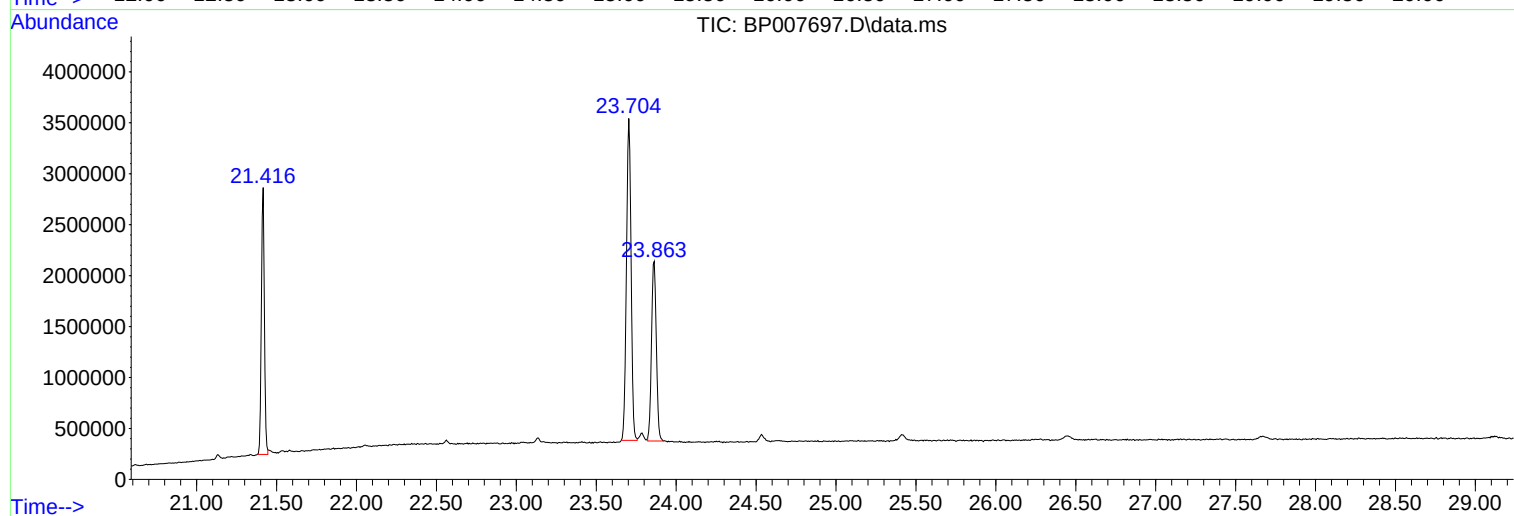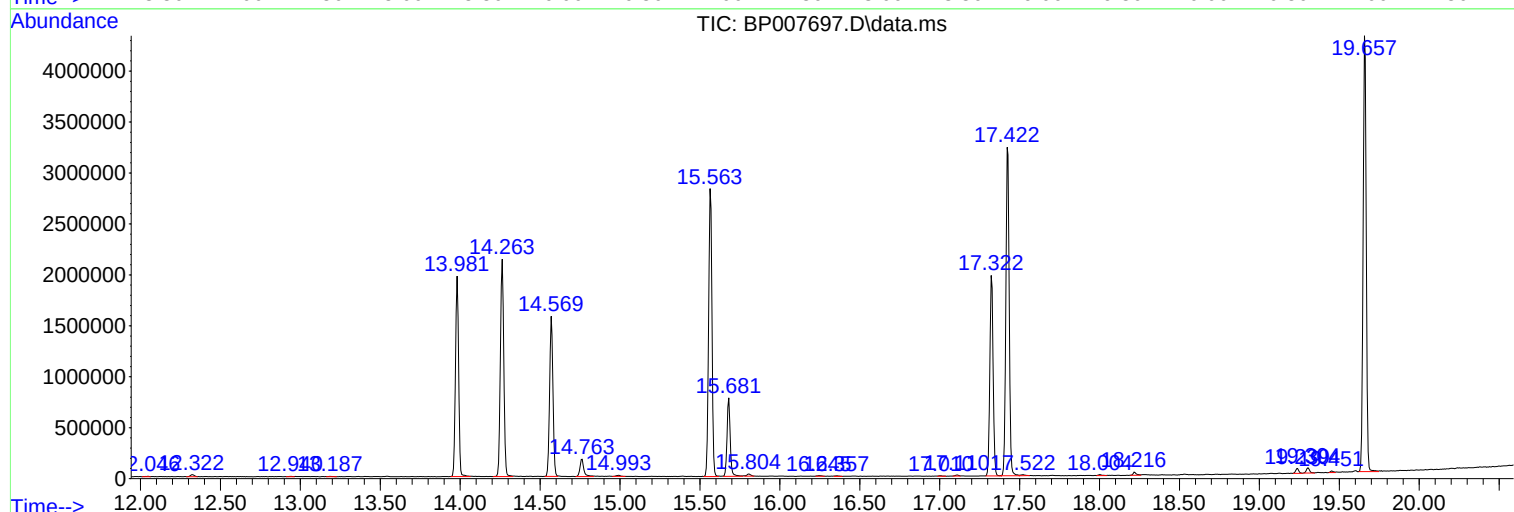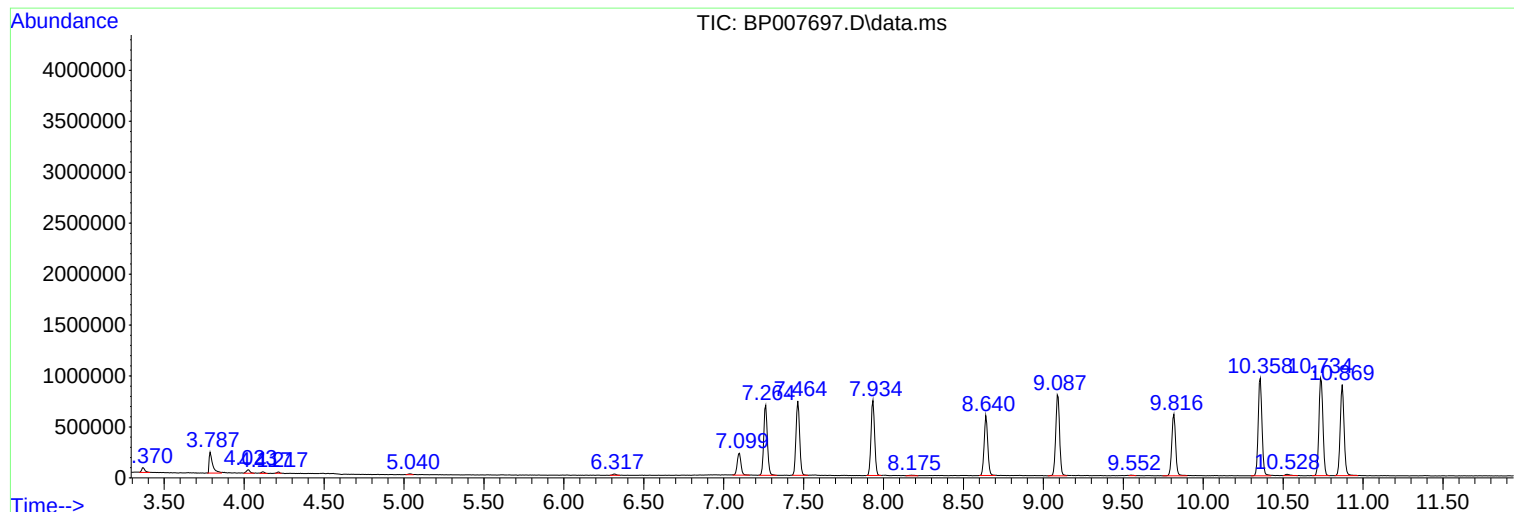

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007697.D
Acq On : 27 Oct 2021 01:50
Operator : CG/JU
Sample : M4303-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P006-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007697.D
Acq On : 27 Oct 2021 01:50
Operator : CG/JU
Sample : M4303-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P006-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------