

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007698.D
 Acq On : 27 Oct 2021 02:24
 Operator : CG/JU
 Sample : M4303-06
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P012-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	7	14	19	rBV	37951	54660	0.83%	0.104%
2	3.787	82	85	100	rBV	158683	258654	3.92%	0.490%
3	4.028	121	126	130	rVB	31985	46310	0.70%	0.088%
4	4.117	138	141	147	rVB3	13490	18388	0.28%	0.035%
5	4.211	154	157	163	rVB2	15721	23848	0.36%	0.045%
6	5.034	295	297	302	rVB4	5360	7463	0.11%	0.014%
7	6.316	508	515	520	rBV4	12503	21469	0.33%	0.041%
8	7.099	642	648	659	rVB	180273	295058	4.47%	0.559%
9	7.263	669	676	687	rBV	643494	1018997	15.43%	1.932%
10	7.463	704	710	720	rVB	656353	1019836	15.44%	1.934%
11	7.563	725	727	732	rVB5	5478	6863	0.10%	0.013%
12	7.934	779	790	797	rBV	704830	1106296	16.75%	2.098%
13	8.005	797	802	808	rVB9	4508	9039	0.14%	0.017%
14	8.181	829	832	839	rVB9	4439	8079	0.12%	0.015%
15	8.640	902	910	919	rBV	508853	809266	12.25%	1.535%
16	9.093	979	987	995	rBV	730605	1226465	18.57%	2.326%
17	9.816	1101	1110	1120	rBV	555105	914676	13.85%	1.734%
18	10.357	1194	1202	1211	rBV	885347	1483457	22.46%	2.813%
19	10.522	1223	1230	1238	rBV	53293	98855	1.50%	0.187%
20	10.740	1259	1267	1274	rBV	913964	1570542	23.78%	2.978%
21	10.869	1280	1289	1302	rBV	746060	1297579	19.64%	2.460%
22	12.322	1529	1536	1543	rBV2	19034	34520	0.52%	0.065%
23	13.187	1678	1683	1689	rBV8	4698	7305	0.11%	0.014%
24	13.410	1717	1721	1725	rBV6	4816	6927	0.10%	0.013%
25	13.781	1778	1784	1788	rBV9	4402	7325	0.11%	0.014%
26	13.981	1810	1818	1833	rBV	1866036	2578648	39.04%	4.890%
27	14.263	1856	1866	1880	rBV	2013312	2981885	45.14%	5.654%
28	14.481	1900	1903	1908	rVB5	7339	9043	0.14%	0.017%
29	14.569	1910	1918	1931	rBV	1501696	2245471	33.99%	4.258%
30	14.757	1943	1950	1961	rBV	148416	256167	3.88%	0.486%
31	14.934	1971	1980	1984	rBV	3246	8102	0.12%	0.015%
32	14.987	1984	1989	1996	rVV10	15649	26985	0.41%	0.051%
33	15.387	2052	2057	2061	rBV8	5815	10402	0.16%	0.020%
34	15.563	2078	2087	2099	rBV	2870399	4117981	62.34%	7.809%
35	15.681	2100	2107	2115	rBV	755015	1036242	15.69%	1.965%
36	15.804	2123	2128	2132	rBV2	20001	31641	0.48%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007698.D
 Acq On : 27 Oct 2021 02:24
 Operator : CG/JU
 Sample : M4303-06
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P012-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	16.134	2179	2184	2185	rBV4	5619	8412	0.13%	0.016%
38	16.257	2196	2205	2208	rBV8	14632	34447	0.52%	0.065%
39	16.328	2210	2217	2226	rVV2	19633	45537	0.69%	0.086%
40	16.469	2237	2241	2246	rBV8	5629	8923	0.14%	0.017%
41	16.681	2273	2277	2280	rBV5	5792	7812	0.12%	0.015%
42	16.992	2327	2330	2331	rBV3	6228	6747	0.10%	0.013%
43	17.110	2346	2350	2353	rBV3	13155	21689	0.33%	0.041%
44	17.151	2355	2357	2365	rVB	19661	27152	0.41%	0.051%
45	17.322	2380	2386	2396	rBV	1841893	2758034	41.75%	5.230%
46	17.428	2397	2404	2414	rVV	3314861	4944230	74.85%	9.375%
47	18.004	2499	2502	2506	rVB3	31172	39633	0.60%	0.075%
48	18.216	2534	2538	2546	rBV	96688	151108	2.29%	0.287%
49	19.233	2708	2711	2715	rBV2	47554	62876	0.95%	0.119%
50	19.304	2720	2723	2727	rVB	49597	57826	0.88%	0.110%
51	19.451	2745	2748	2756	rBV3	52570	86344	1.31%	0.164%
52	19.657	2778	2783	2790	rBV	4516013	6180513	93.56%	11.720%
53	21.133	3030	3034	3041	rBV2	148433	224745	3.40%	0.426%
54	21.416	3077	3082	3094	rBV	2612532	3331133	50.43%	6.317%
55	23.704	3463	3471	3480	rBV2	3264262	6605594	100.00%	12.526%
56	23.863	3491	3498	3510	rVB2	1650992	3479424	52.67%	6.598%




Sum of corrected areas: 52736623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007698.D
Acq On : 27 Oct 2021 02:24
Operator : CG/JU
Sample : M4303-06
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P012-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

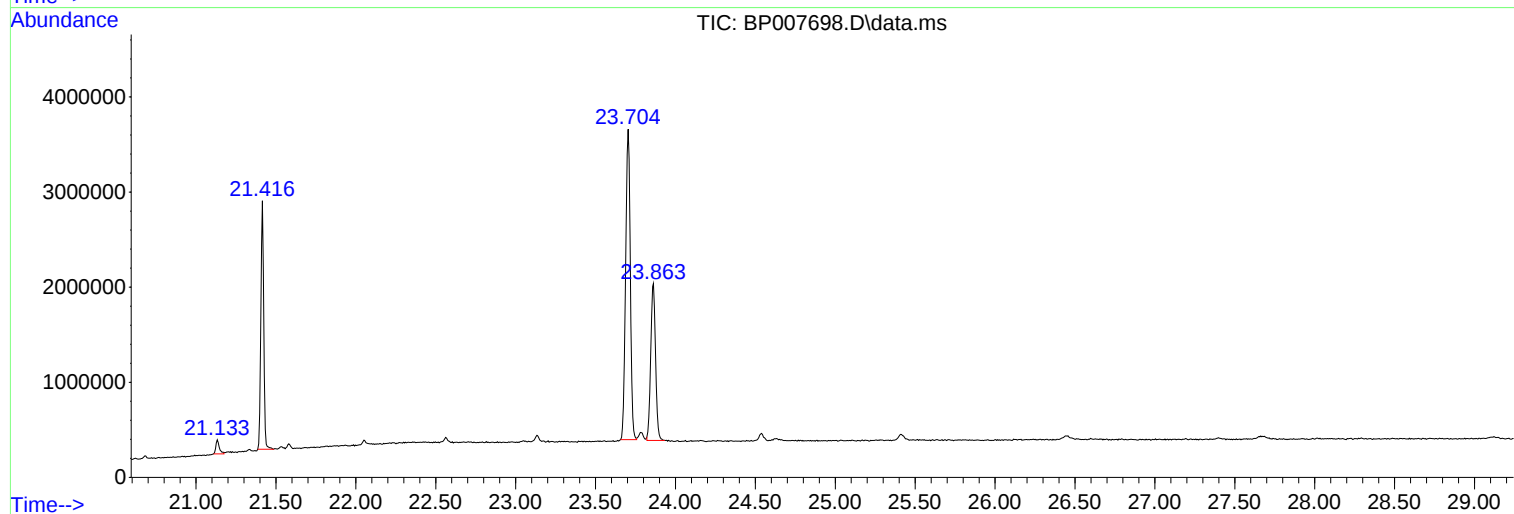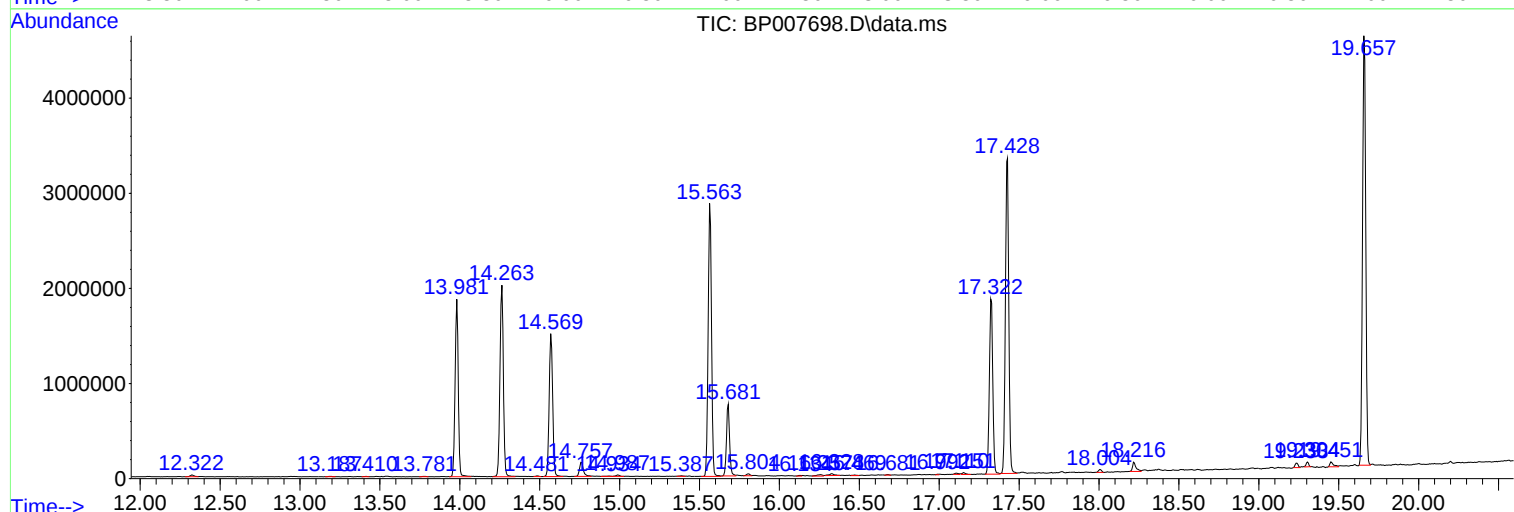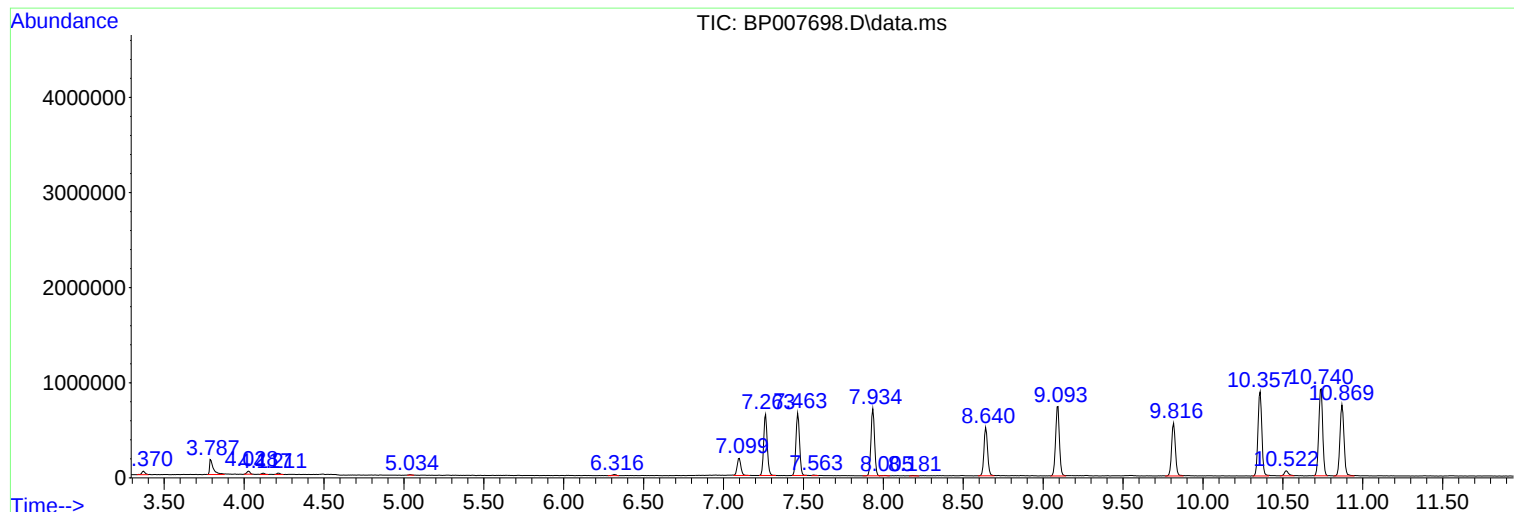

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007698.D
Acq On : 27 Oct 2021 02:24
Operator : CG/JU
Sample : M4303-06
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P012-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007698.D
Acq On : 27 Oct 2021 02:24
Operator : CG/JU
Sample : M4303-06
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P012-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
