

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007699.D
 Acq On : 27 Oct 2021 02:57
 Operator : CG/JU
 Sample : M4303-07
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	10	13	20	rVB	41079	53868	1.02%	0.119%
2	3.787	82	85	102	rBV	189765	305161	5.75%	0.677%
3	4.028	120	126	130	rVB	28048	42651	0.80%	0.095%
4	4.117	138	141	146	rVB	14763	16492	0.31%	0.037%
5	4.216	154	158	163	rVB5	12433	16901	0.32%	0.037%
6	5.040	295	298	303	rVB5	5471	7876	0.15%	0.017%
7	6.316	511	515	520	rBV3	10764	15801	0.30%	0.035%
8	6.934	615	620	624	rVV8	3147	6903	0.13%	0.015%
9	7.099	641	648	657	rVB	155067	254452	4.80%	0.564%
10	7.263	669	676	688	rVB	567646	918990	17.32%	2.037%
11	7.463	703	710	720	rBV	579588	914848	17.24%	2.028%
12	7.934	781	790	798	rBV	672283	1056881	19.92%	2.343%
13	8.181	827	832	835	rBV7	4586	6633	0.13%	0.015%
14	8.640	904	910	922	rBV	454063	713449	13.45%	1.582%
15	9.087	979	986	997	rBV	649470	1087100	20.49%	2.410%
16	9.552	1058	1065	1070	rVB10	6094	13758	0.26%	0.031%
17	9.816	1103	1110	1120	rBV	479980	801660	15.11%	1.777%
18	10.057	1145	1151	1159	rVB	3272	8964	0.17%	0.020%
19	10.357	1192	1202	1214	rBV	770890	1316536	24.82%	2.919%
20	10.528	1226	1231	1239	rBV5	10968	24834	0.47%	0.055%
21	10.734	1259	1266	1274	rBV	856983	1496165	28.20%	3.317%
22	10.869	1280	1289	1302	rBV	731879	1255411	23.66%	2.783%
23	11.369	1370	1374	1377	rBV5	3438	6611	0.12%	0.015%
24	12.322	1530	1536	1543	rBV2	16357	29003	0.55%	0.064%
25	12.940	1637	1641	1647	rBV9	5162	11416	0.22%	0.025%
26	13.187	1679	1683	1686	rBV6	4247	6144	0.12%	0.014%
27	13.540	1737	1743	1749	rBV9	3885	10654	0.20%	0.024%
28	13.887	1800	1802	1810	rVB9	3667	8000	0.15%	0.018%
29	13.981	1810	1818	1825	rBV	1582908	2211788	41.69%	4.904%
30	14.263	1856	1866	1878	rBV	1688083	2532491	47.74%	5.615%
31	14.569	1911	1918	1929	rBV	1421638	2070289	39.02%	4.590%
32	14.763	1942	1951	1965	rBV	105571	194524	3.67%	0.431%
33	14.992	1983	1990	1996	rBV	6875	13642	0.26%	0.030%
34	15.386	2050	2057	2059	rBV8	3902	6565	0.12%	0.015%
35	15.563	2080	2087	2099	rBV	2384228	3417180	64.41%	7.576%
36	15.681	2100	2107	2120	rVV	529877	763777	14.40%	1.693%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007699.D
 Acq On : 27 Oct 2021 02:57
 Operator : CG/JU
 Sample : M4303-07
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-02

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	15.804	2124	2128	2135	rVB4	17470	30751	0.58%	0.068%
38	16.134	2179	2184	2188	rBV7	4201	6859	0.13%	0.015%
39	16.257	2196	2205	2211	rBV6	13284	32507	0.61%	0.072%
40	16.463	2236	2240	2246	rVB9	2780	5880	0.11%	0.013%
41	17.004	2327	2332	2335	rVB7	3765	5417	0.10%	0.012%
42	17.116	2345	2351	2354	rBV3	8955	15218	0.29%	0.034%
43	17.328	2380	2387	2395	rBV	1710900	2541625	47.91%	5.635%
44	17.428	2397	2404	2415	rVV	2725501	3991557	75.24%	8.849%
45	17.522	2417	2420	2424	rVB6	12006	15994	0.30%	0.035%
46	18.004	2497	2502	2508	rBV9	10468	15451	0.29%	0.034%
47	18.216	2534	2538	2547	rBV7	26539	55002	1.04%	0.122%
48	19.233	2707	2711	2716	rBV2	39794	59883	1.13%	0.133%
49	19.304	2719	2723	2727	rBV2	42951	58590	1.10%	0.130%
50	19.451	2746	2748	2751	rVB3	11553	10873	0.20%	0.024%
51	19.657	2777	2783	2791	rBV	3617536	4975280	93.78%	11.030%
52	21.416	3077	3082	3088	rBV	2326678	3064877	57.77%	6.795%
53	23.704	3463	3471	3480	rBV2	2611197	5305230	100.00%	11.762%
54	23.863	3491	3498	3513	rVB2	1607256	3296551	62.14%	7.309%




Sum of corrected areas: 45104963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007699.D
Acq On : 27 Oct 2021 02:57
Operator : CG/JU
Sample : M4303-07
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

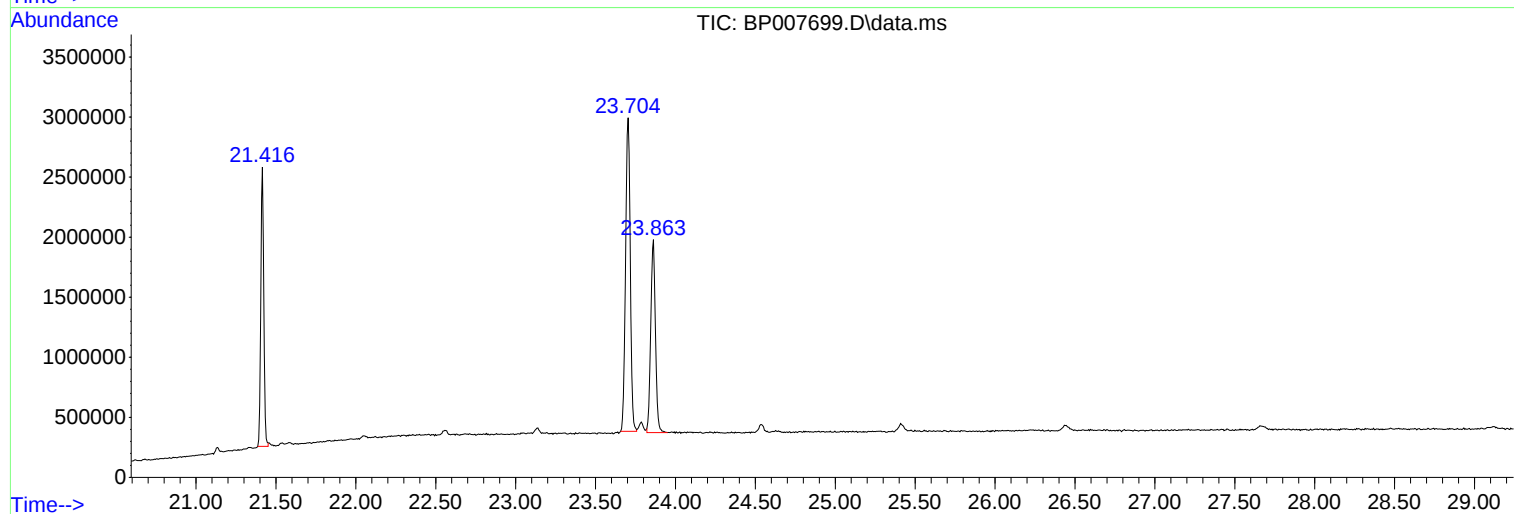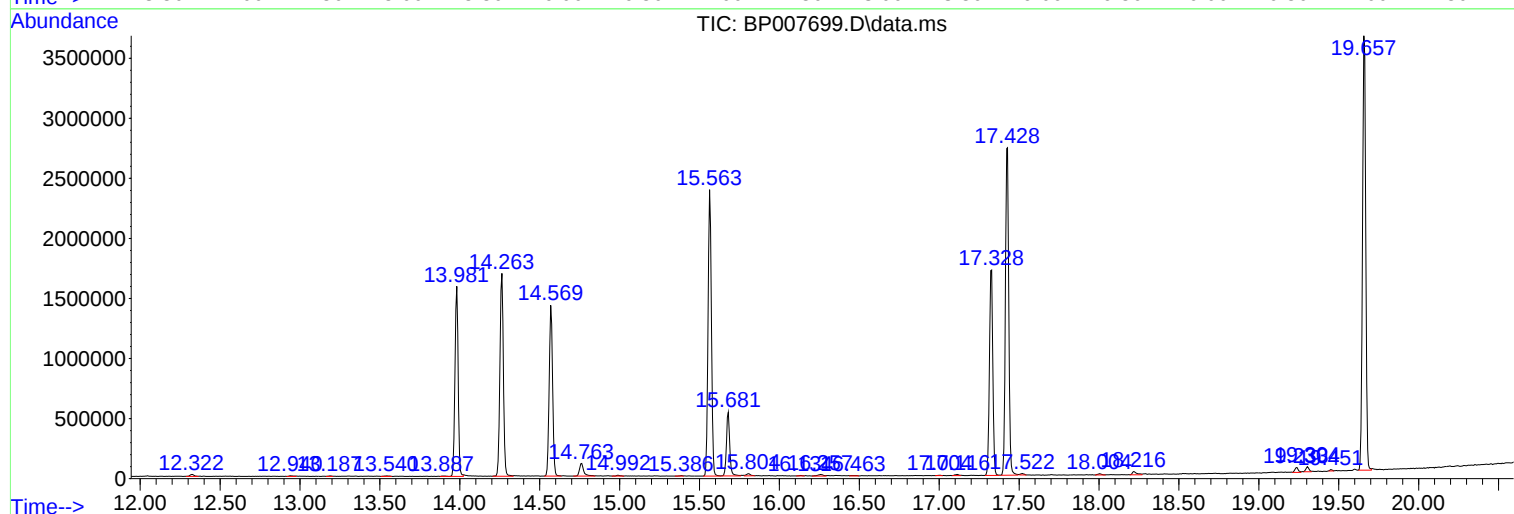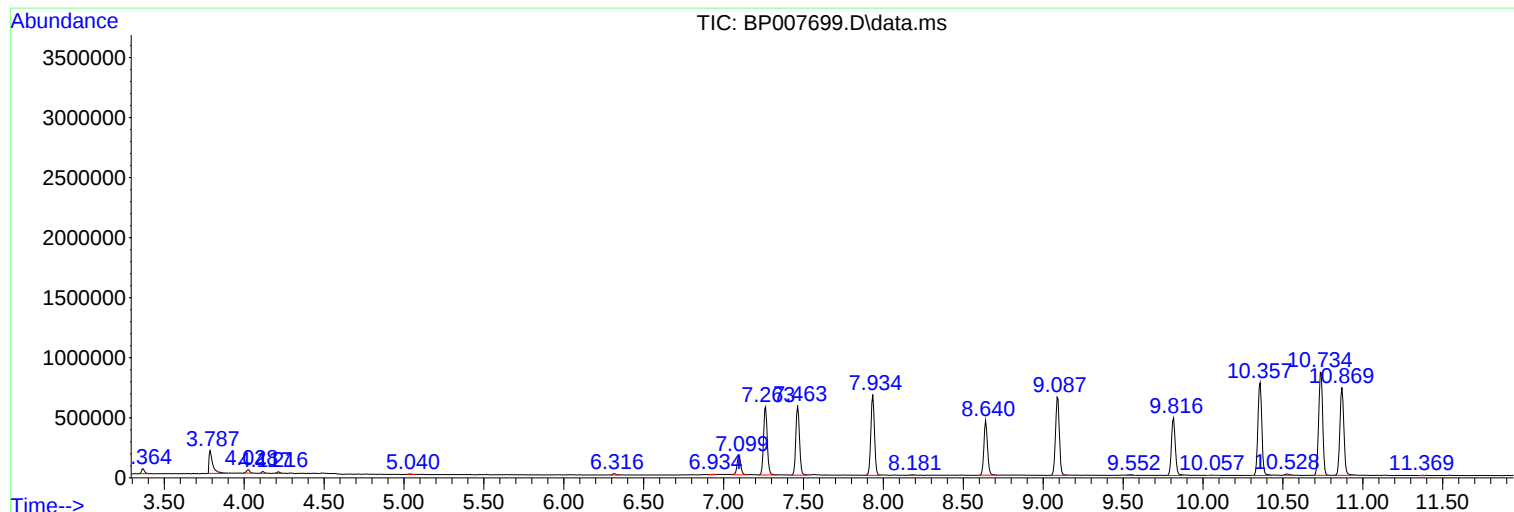

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007699.D
Acq On : 27 Oct 2021 02:57
Operator : CG/JU
Sample : M4303-07
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007699.D
Acq On : 27 Oct 2021 02:57
Operator : CG/JU
Sample : M4303-07
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
