

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007701.D
 Acq On : 27 Oct 2021 04:39
 Operator : CG/JU
 Sample : PB140187BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK187

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	22	rVB	51762	68218	1.32%	0.139%
2	3.781	81	84	98	rBV	713201	1041479	20.21%	2.129%
3	4.111	138	140	144	rVB3	10500	13035	0.25%	0.027%
4	7.093	640	647	656	rBV	766161	1228675	23.84%	2.512%
5	7.263	669	676	685	rVB	613717	968302	18.79%	1.979%
6	7.463	703	710	724	rBV	806745	1255974	24.37%	2.568%
7	7.934	783	790	799	rBV	638345	995147	19.31%	2.034%
8	8.640	902	910	923	rBV	946047	1521630	29.53%	3.111%
9	9.087	979	986	999	rBV	697393	1148941	22.30%	2.349%
10	9.816	1101	1110	1121	rBV	552379	912440	17.71%	1.865%
11	10.357	1194	1202	1216	rBV	927822	1552496	30.13%	3.174%
12	10.734	1258	1266	1276	rVB	836382	1414574	27.45%	2.892%
13	10.869	1281	1289	1303	rBV	913139	1570080	30.47%	3.210%
14	12.328	1531	1537	1542	rBV	18167	32405	0.63%	0.066%
15	13.540	1739	1743	1748	rVV7	4644	6877	0.13%	0.014%
16	13.981	1811	1818	1832	rBV	1692638	2376896	46.12%	4.859%
17	14.263	1858	1866	1878	rBV	1839204	2733416	53.04%	5.588%
18	14.569	1909	1918	1932	rVB	1336203	1968077	38.19%	4.023%
19	14.757	1944	1950	1967	rBV	732421	1109847	21.54%	2.269%
20	15.563	2080	2087	2097	rBV	2463856	3532021	68.54%	7.220%
21	15.681	2101	2107	2118	rBV	614815	865733	16.80%	1.770%
22	15.804	2124	2128	2134	rVB3	18512	30214	0.59%	0.062%
23	16.251	2199	2204	2209	rVB8	5141	9760	0.19%	0.020%
24	17.110	2346	2350	2355	rBV3	7729	14330	0.28%	0.029%
25	17.322	2379	2386	2396	rBV	1697169	2434001	47.23%	4.976%
26	17.422	2397	2403	2415	rVV	2736105	3911289	75.90%	7.996%
27	17.998	2498	2501	2506	rBV7	4640	7258	0.14%	0.015%
28	19.239	2708	2712	2716	rVB3	37952	52146	1.01%	0.107%
29	19.304	2719	2723	2727	rBV	39431	53949	1.05%	0.110%
30	19.657	2777	2783	2795	rBV	3572294	4856645	94.24%	9.928%
31	21.416	3077	3082	3092	rBV	2280070	2967138	57.58%	6.066%
32	23.704	3463	3471	3480	rBV2	2544524	5153313	100.00%	10.535%
33	23.857	3491	3497	3509	rVB2	1462608	3111329	60.38%	6.360%




Sum of corrected areas: 48917635

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007701.D
Acq On : 27 Oct 2021 04:39
Operator : CG/JU
Sample : PB140187BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK187

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

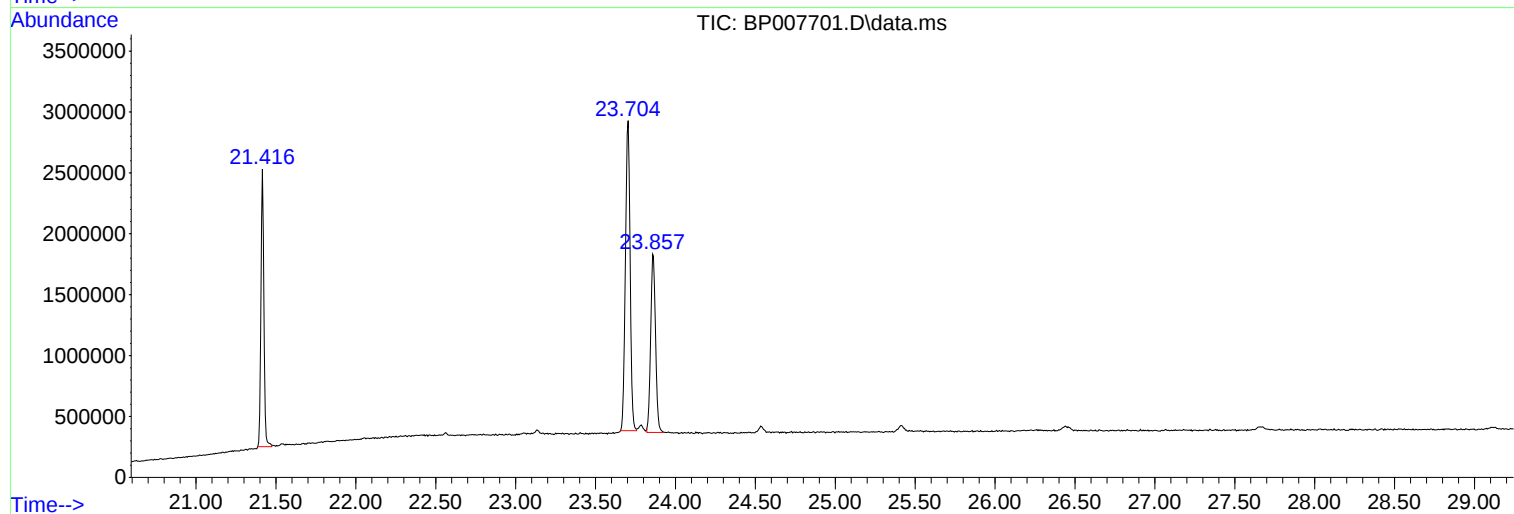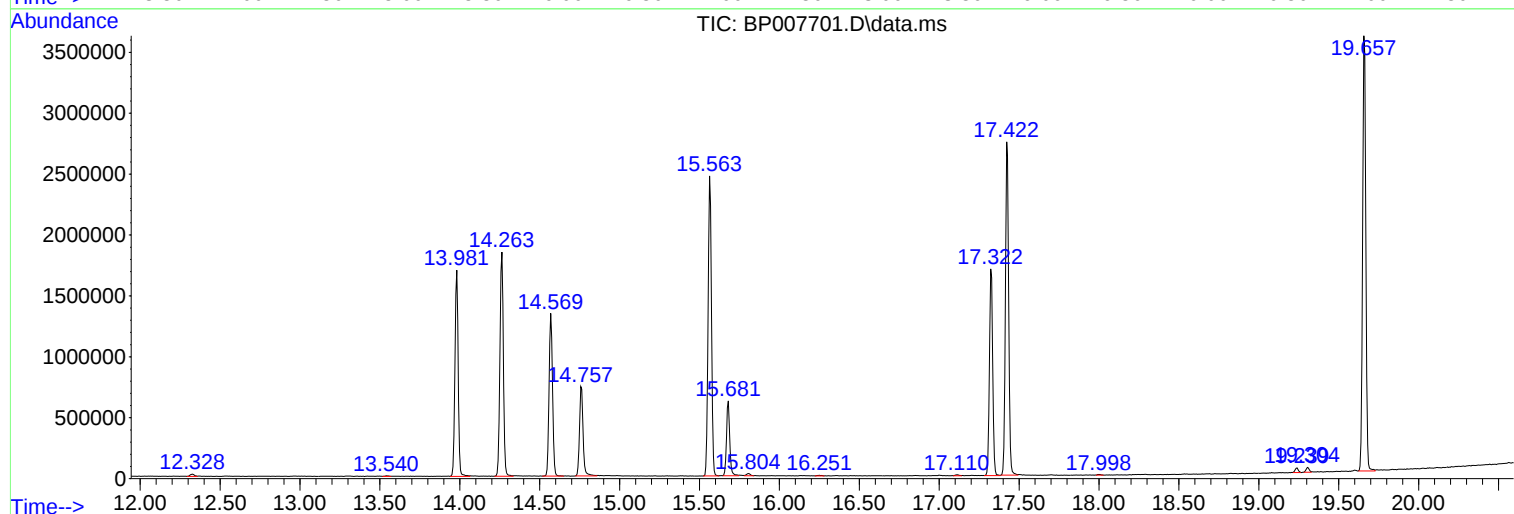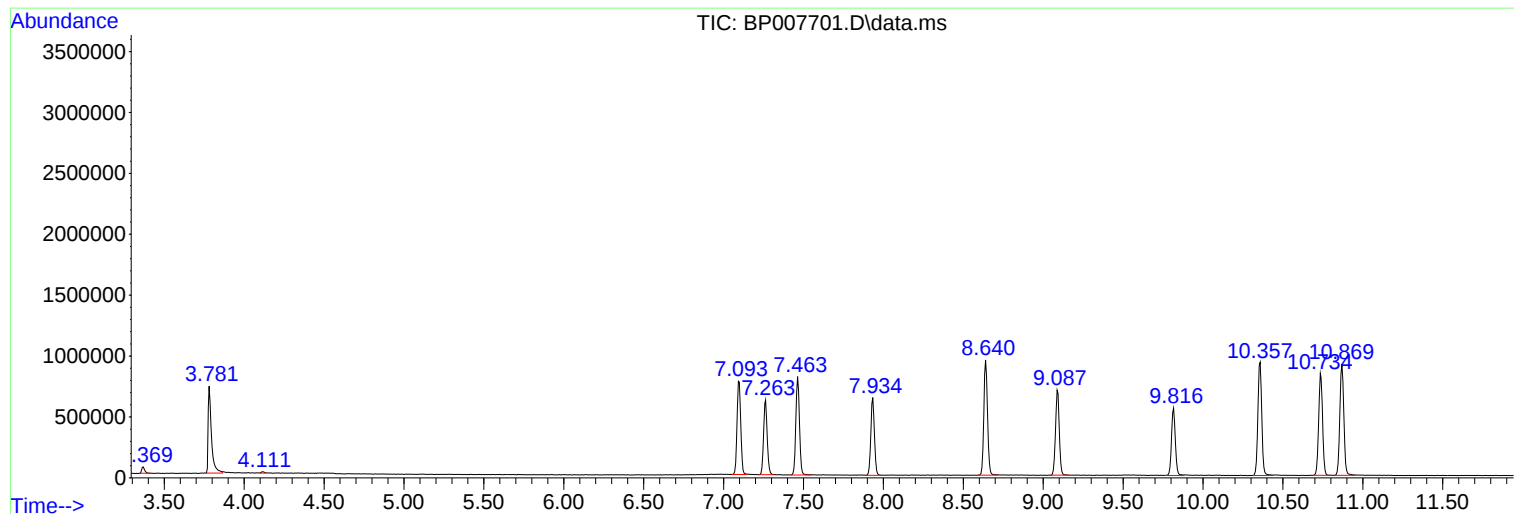

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007701.D
Acq On : 27 Oct 2021 04:39
Operator : CG/JU
Sample : PB140187BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK187

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007701.D
Acq On : 27 Oct 2021 04:39
Operator : CG/JU
Sample : PB140187BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK187

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------