

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007705.D
 Acq On : 27 Oct 2021 06:55
 Operator : CG/JU
 Sample : M4303-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

Signal : TIC: BP007705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	6	9	10	rBV3	9094	9508	0.18%	0.022%
2	3.370	10	14	21	rVB	57346	78936	1.50%	0.179%
3	3.499	35	36	41	rBV5	4853	6676	0.13%	0.015%
4	3.781	81	84	99	rBV	323248	534270	10.12%	1.209%
5	4.022	120	125	133	rVB	60315	96090	1.82%	0.217%
6	4.117	138	141	144	rVB3	12846	16062	0.30%	0.036%
7	4.211	153	157	165	rVB2	24662	38921	0.74%	0.088%
8	4.487	201	204	209	rBV7	6165	9887	0.19%	0.022%
9	5.034	293	297	305	rVB	18586	31195	0.59%	0.071%
10	6.316	509	515	522	rVB6	7570	13400	0.25%	0.030%
11	7.099	640	648	654	rVB	33510	60795	1.15%	0.138%
12	7.263	669	676	685	rBV	594522	958426	18.15%	2.169%
13	7.463	704	710	717	rBV	26717	48232	0.91%	0.109%
14	7.569	723	728	734	rBV8	6749	12744	0.24%	0.029%
15	7.752	756	759	763	rVB5	4845	6993	0.13%	0.016%
16	7.934	782	790	798	rBV	734236	1166487	22.09%	2.640%
17	8.181	827	832	840	rBV9	6623	13593	0.26%	0.031%
18	8.640	901	910	919	rBV	212968	350528	6.64%	0.793%
19	8.822	939	941	948	rBV7	3979	6015	0.11%	0.014%
20	9.087	980	986	996	rBV	689735	1156376	21.90%	2.617%
21	9.546	1055	1064	1075	rVB	7357	21431	0.41%	0.049%
22	9.893	1120	1123	1128	rVB6	6355	8546	0.16%	0.019%
23	10.357	1196	1202	1211	rBV	35213	63165	1.20%	0.143%
24	10.522	1228	1230	1237	rVB6	7134	12203	0.23%	0.028%
25	10.734	1259	1266	1275	rBV	969246	1661896	31.48%	3.762%
26	10.869	1280	1289	1300	rBV	829928	1443566	27.34%	3.267%
27	11.381	1370	1376	1378	rBV6	4259	7427	0.14%	0.017%
28	11.546	1397	1404	1411	rBV7	18183	35617	0.67%	0.081%
29	12.051	1485	1490	1494	rBV6	5359	8379	0.16%	0.019%
30	12.134	1499	1504	1509	rBV3	26014	42433	0.80%	0.096%
31	12.328	1531	1537	1543	rBV3	17997	31773	0.60%	0.072%
32	12.946	1636	1642	1646	rBV7	6683	12319	0.23%	0.028%
33	13.187	1679	1683	1686	rBV6	5971	8578	0.16%	0.019%
34	13.540	1740	1743	1751	rVB9	11934	18737	0.35%	0.042%
35	13.893	1796	1803	1811	rBV	95965	148234	2.81%	0.336%
36	13.981	1811	1818	1824	rBV	1733302	2306410	43.68%	5.221%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
 Data File : BP007705.D
 Acq On : 27 Oct 2021 06:55
 Operator : CG/JU
 Sample : M4303-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P013-TW001-03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
 Title : SVOA CALIBRATION

37	14.263	1857	1866	1877	rBV	1917808	2785522	52.76%	6.305%
38	14.569	1910	1918	1928	rBV	1583561	2365726	44.81%	5.355%
39	15.387	2054	2057	2062	rBV4	6490	10250	0.19%	0.023%
40	15.563	2079	2087	2101	rBV	2460752	3605968	68.30%	8.162%
41	15.804	2123	2128	2132	rBV2	17188	26932	0.51%	0.061%
42	15.845	2132	2135	2140	rVB6	9217	13541	0.26%	0.031%
43	16.134	2181	2184	2188	rBV6	4860	7295	0.14%	0.017%
44	16.239	2195	2202	2204	rBV8	5704	11656	0.22%	0.026%
45	16.328	2213	2217	2226	rVB5	18683	35803	0.68%	0.081%
46	16.616	2262	2266	2273	rBV10	4845	10003	0.19%	0.023%
47	16.675	2274	2276	2281	rVB5	4362	6573	0.12%	0.015%
48	17.004	2324	2332	2336	rVB5	4729	11947	0.23%	0.027%
49	17.063	2337	2342	2345	rBV7	4443	9440	0.18%	0.021%
50	17.110	2347	2350	2353	rVV3	10374	14063	0.27%	0.032%
51	17.151	2354	2357	2362	rVB5	12328	18698	0.35%	0.042%
52	17.328	2380	2387	2393	rBV	1990894	2923454	55.37%	6.617%
53	17.428	2397	2404	2418	rVV	2894716	4171237	79.00%	9.442%
54	17.563	2424	2427	2431	rVV	13169	16552	0.31%	0.037%
55	17.910	2484	2486	2493	rVB6	7983	10454	0.20%	0.024%
56	18.051	2506	2510	2515	rBV8	5426	9009	0.17%	0.020%
57	18.198	2531	2535	2538	rBV3	11113	17256	0.33%	0.039%
58	18.239	2540	2542	2547	rVV4	14931	20358	0.39%	0.046%
59	18.292	2548	2551	2554	rVB2	7999	9350	0.18%	0.021%
60	18.375	2561	2565	2569	rVB3	7511	9269	0.18%	0.021%
61	18.575	2597	2599	2602	rVB4	4948	5694	0.11%	0.013%
62	19.239	2708	2712	2718	rBV2	42357	55958	1.06%	0.127%
63	19.304	2719	2723	2729	rVV2	41182	55512	1.05%	0.126%
64	19.598	2771	2773	2777	rBV5	16962	18133	0.34%	0.041%
65	19.657	2778	2783	2790	rBV	3675510	5089131	96.39%	11.519%
66	21.416	3077	3082	3096	rBV	2724298	3517866	66.63%	7.963%
67	23.704	3464	3471	3480	rBV2	2619828	5279880	100.00%	11.951%
68	23.863	3491	3498	3508	rVB2	1720519	3591284	68.02%	8.129%




Sum of corrected areas: 44179662

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007705.D
Acq On : 27 Oct 2021 06:55
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

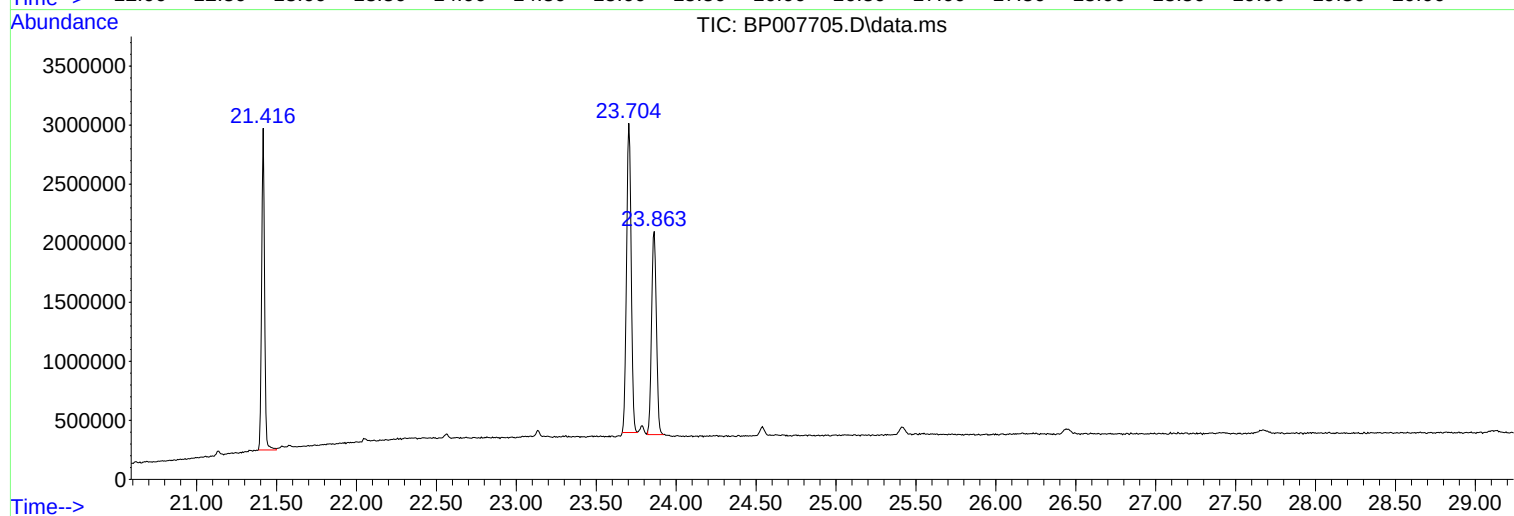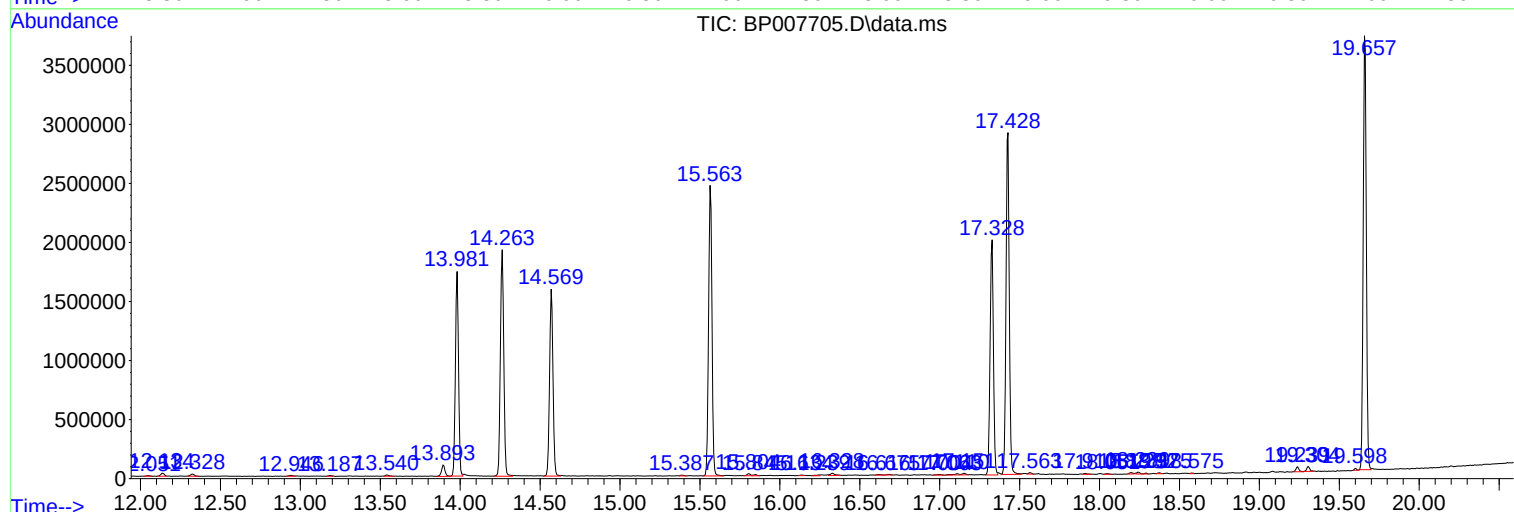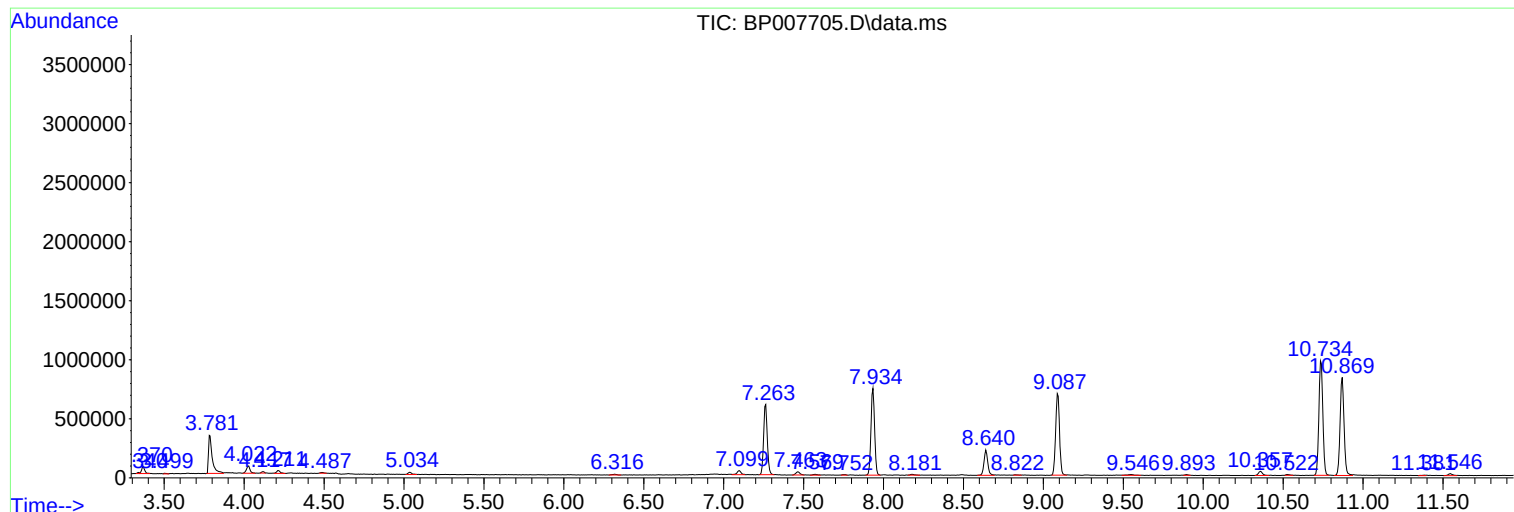

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007705.D
Acq On : 27 Oct 2021 06:55
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP102521\
Data File : BP007705.D
Acq On : 27 Oct 2021 06:55
Operator : CG/JU
Sample : M4303-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P013-TW001-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP102521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------